

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037797.D
 Acq On : 10 Oct 2024 12:12
 Operator : SY/MD
 Sample : P4363-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 11 05:12:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	597247	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	591709	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	261862	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	200750	38.290	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.580%
7) Chloroethane-d5	1.532	69	173745	42.694	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.380%
11) 1,1-Dichloroethene-d2	2.060	65	92143	42.066	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.140%
21) 2-Butanone-d5	3.799	46	162336	86.931	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.930%
24) Chloroform-d	4.243	84	413530	44.333	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.660%
26) 1,2-Dichloroethane-d4	4.937	65	258164	47.285	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.560%
32) Benzene-d6	4.953	84	825726	44.596	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.200%
36) 1,2-Dichloropropane-d6	5.982	67	261863	44.414	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.820%
41) Toluene-d8	7.236	98	724648	43.161	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.320%
43) trans-1,3-Dichloroprop...	7.551	79	109682	40.046	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.100%
47) 2-Hexanone-d5	8.024	63	99107	79.605	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.600%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	298967	43.641	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.280%
66) 1,2-Dichlorobenzene-d4	11.551	152	273282	49.526	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.060%
Target Compounds						
39) cis-1,3-Dichloropropene	6.908	75	7133	0.970	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037797.D
Acq On : 10 Oct 2024 12:12
Operator : SY/MD
Sample : P4363-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 11 05:12:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

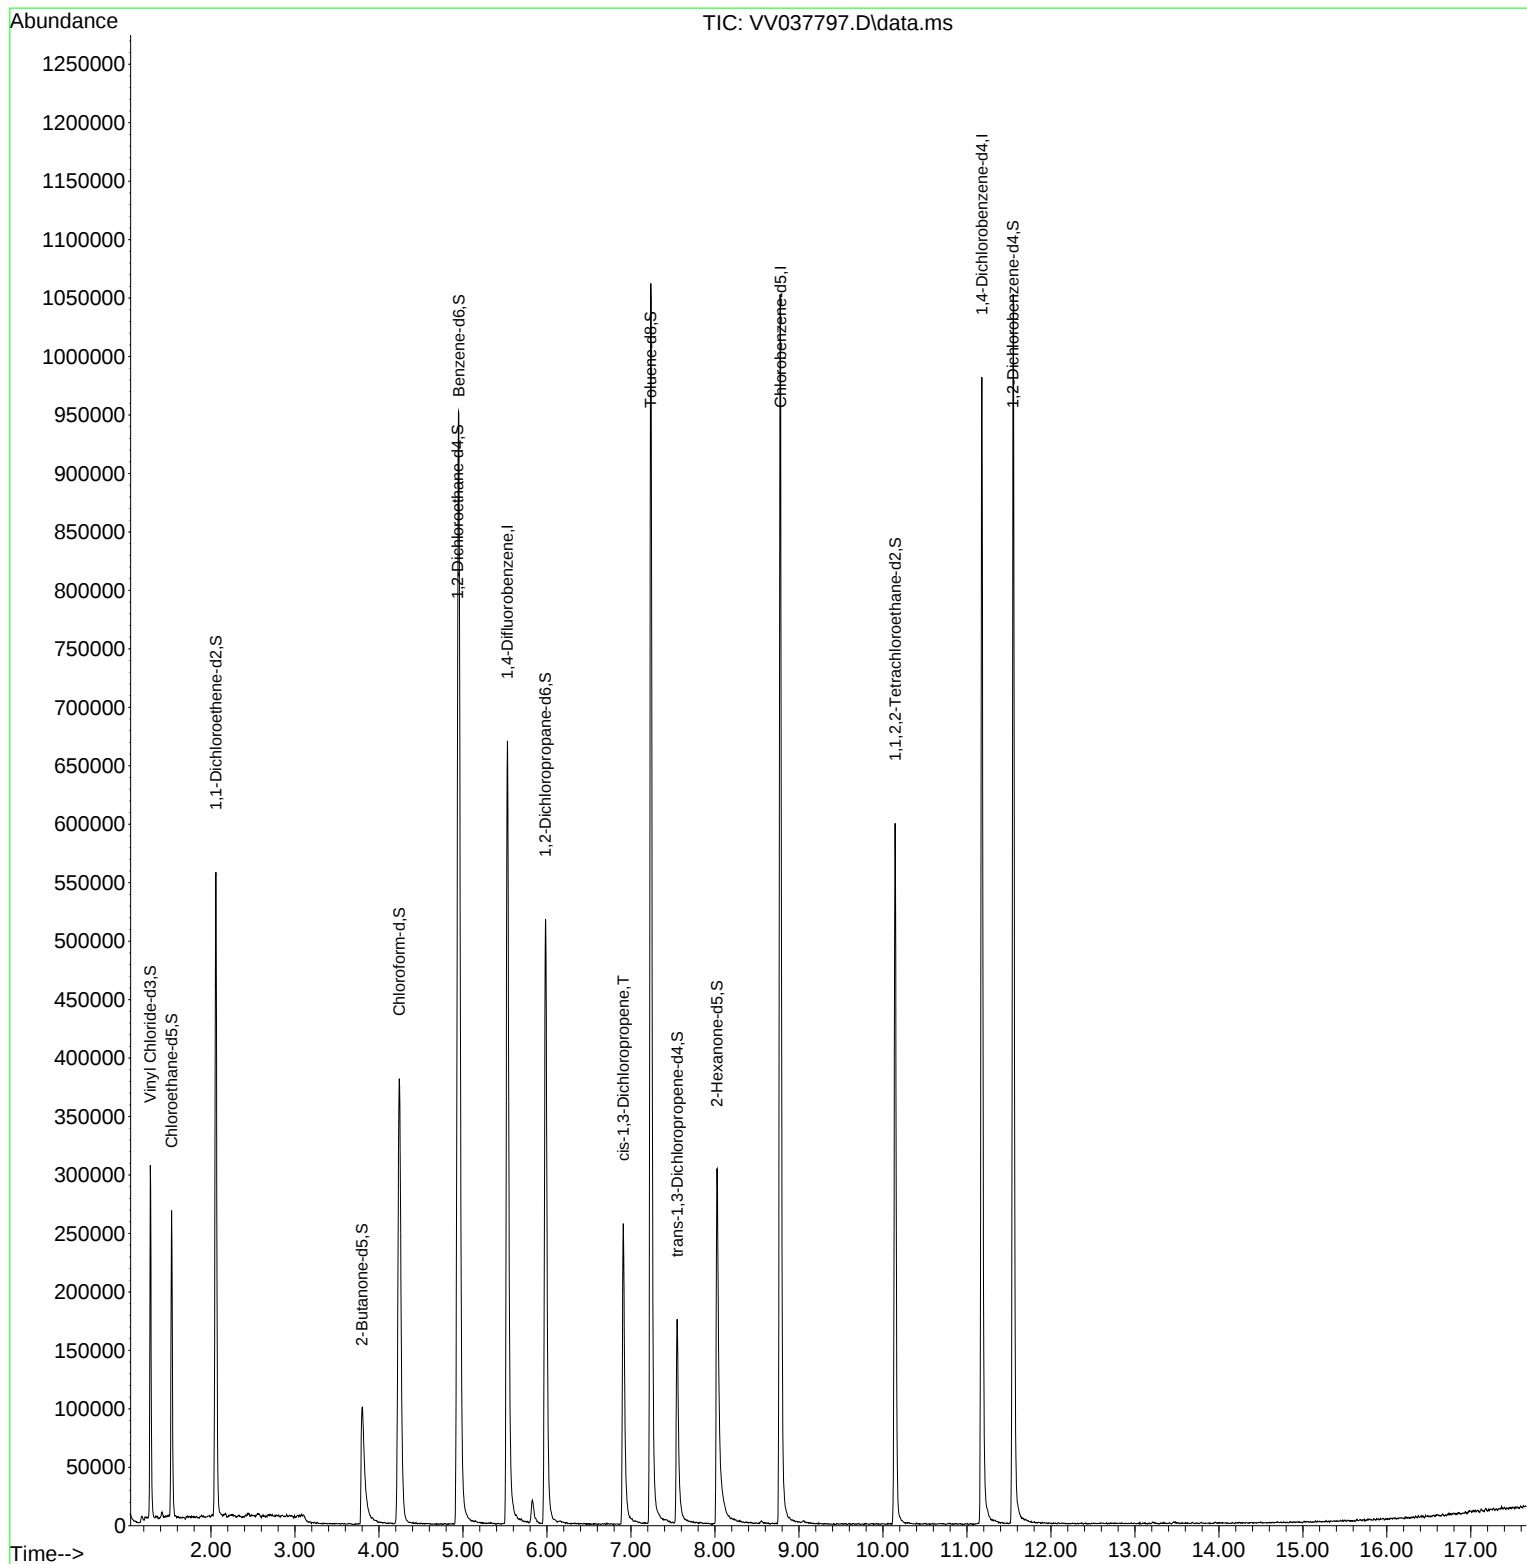

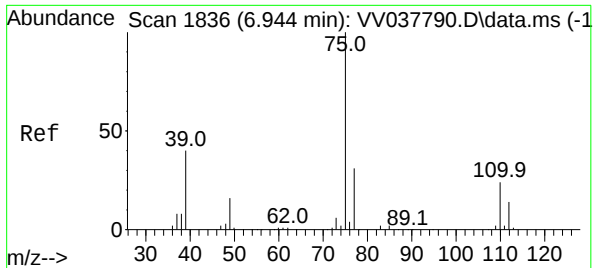

#39
 cis-1,3-Dichloropropene
 Concen: 0.970 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV037797.D
 Acq: 10 Oct 2024 12:12

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 7133
 Ion Ratio Lower Upper
 75 100
 77 52.2 21.8 40.4#

