

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037805.D
 Acq On : 10 Oct 2024 15:04
 Operator : SY/MD
 Sample : P4379-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 11 05:14:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	593711	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	596472	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	258659	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	198319	38.052	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.100%		
7) Chloroethane-d5	1.532	69	169056	41.789	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.580%		
11) 1,1-Dichloroethene-d2	2.056	65	92106	42.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.600%		
21) 2-Butanone-d5	3.796	46	163034	87.825	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.820%		
24) Chloroform-d	4.243	84	421014	45.405	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.800%		
26) 1,2-Dichloroethane-d4	4.934	65	254258	46.847	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.700%		
32) Benzene-d6	4.950	84	822758	44.081	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.160%		
36) 1,2-Dichloropropane-d6	5.982	67	265705	44.706	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.420%		
41) Toluene-d8	7.236	98	724401	42.801	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.600%		
43) trans-1,3-Dichloroprop...	7.551	79	110887	40.163	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.320%		
47) 2-Hexanone-d5	8.024	63	105385	83.972	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.970%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	308374	44.654	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.300%		
66) 1,2-Dichlorobenzene-d4	11.551	152	280587	51.479	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.960%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.908	75	6754	0.911	ug/L	# 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037805.D
Acq On : 10 Oct 2024 15:04
Operator : SY/MD
Sample : P4379-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 11 05:14:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

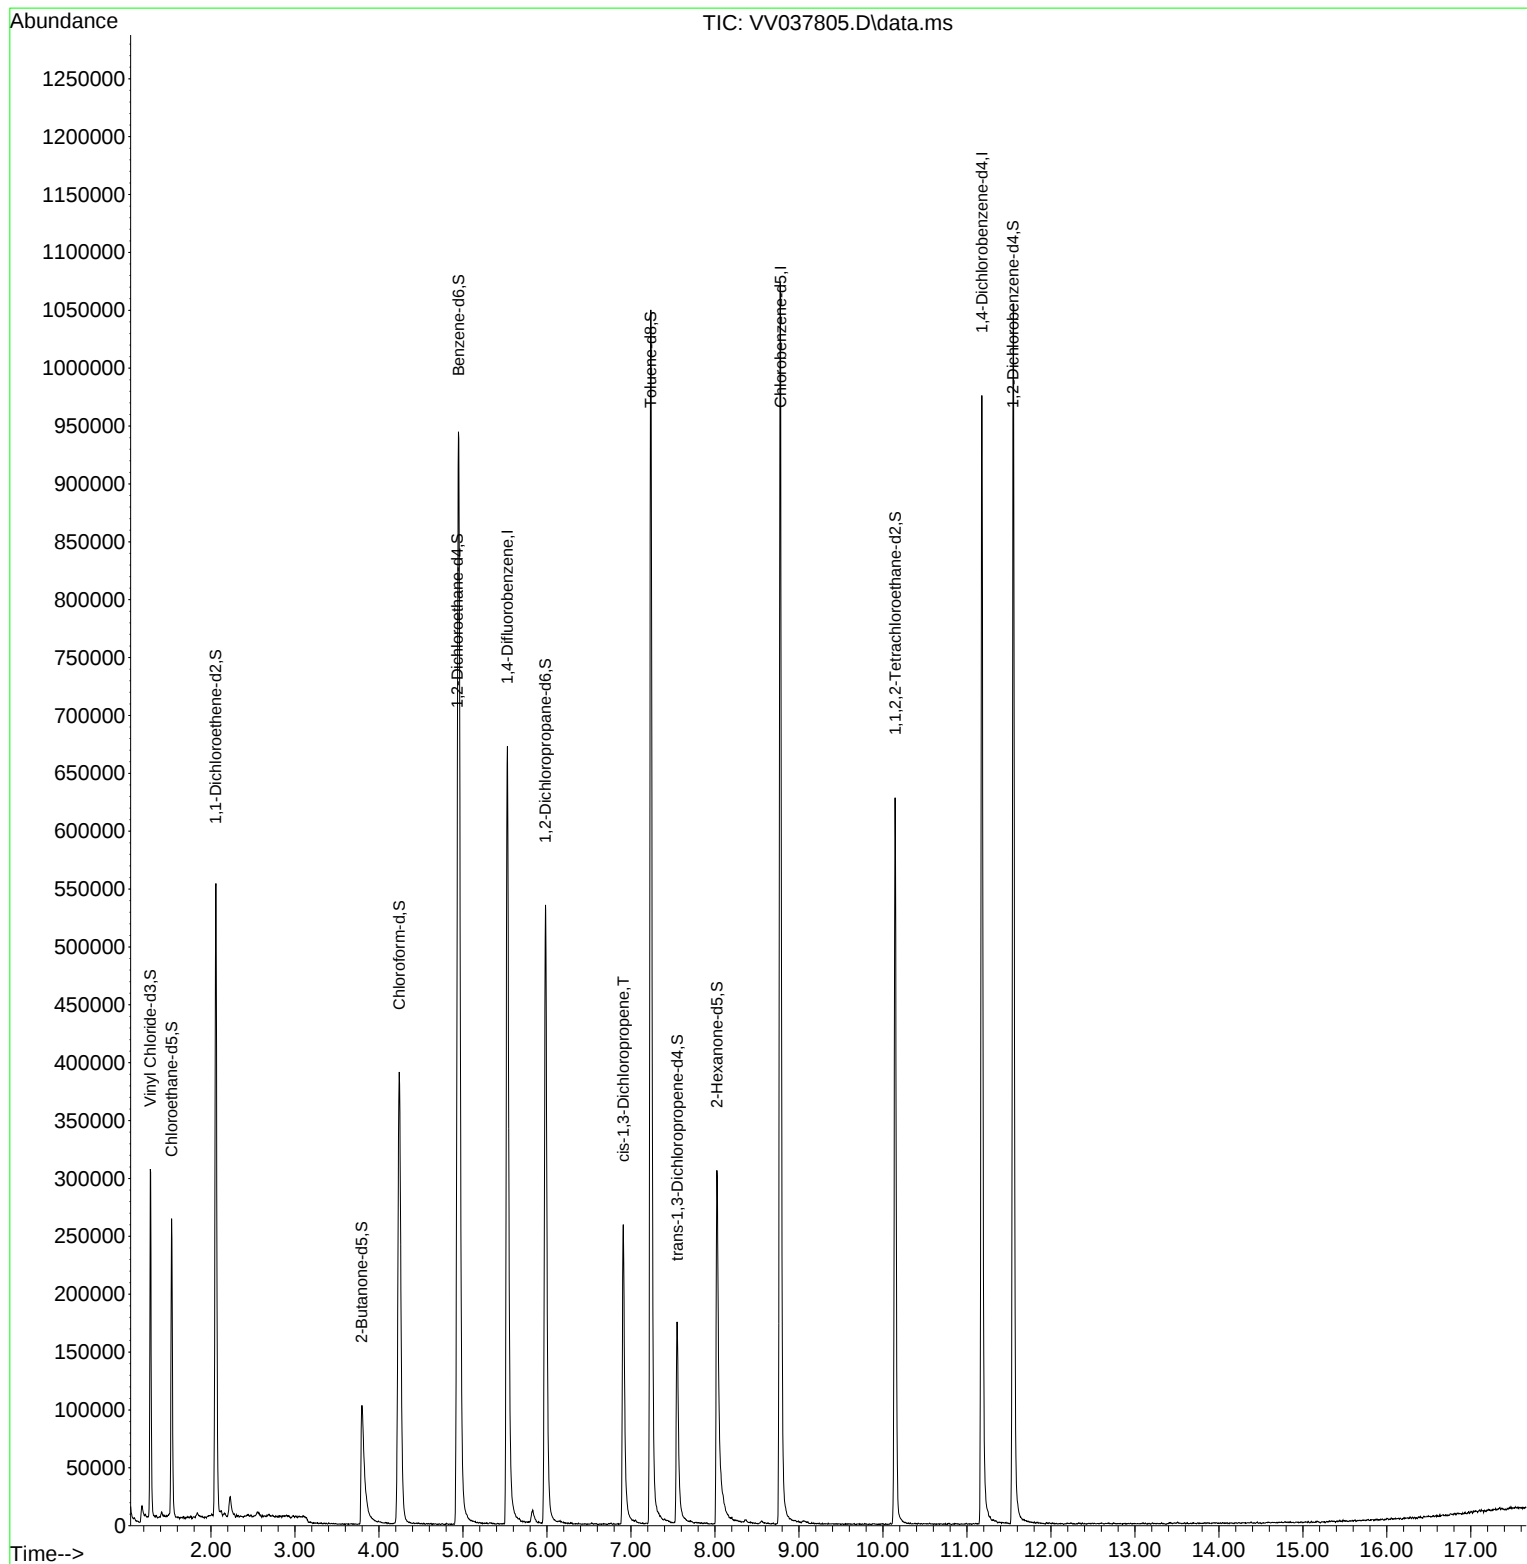

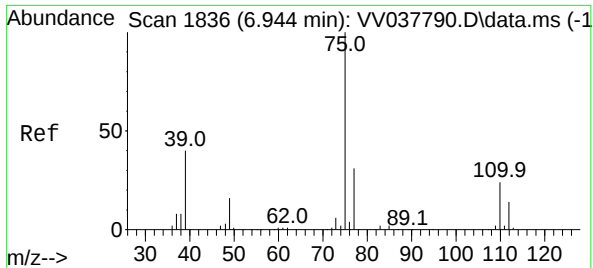

#39
 cis-1,3-Dichloropropene
 Concen: 0.911 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.035 min
 Lab File: VV037805.D
 Acq: 10 Oct 2024 15:04

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6754
 Ion Ratio Lower Upper
 75 100
 77 56.0 21.8 40.4#

