

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037807.D
 Acq On : 10 Oct 2024 15:47
 Operator : SY/MD
 Sample : P4379-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 11 05:14:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	590763	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	590044	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	262953	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	191502	36.927	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	73.860%
7) Chloroethane-d5	1.532	69	171119	42.510	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.020%
11) 1,1-Dichloroethene-d2	2.060	65	92335	42.617	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.240%
21) 2-Butanone-d5	3.799	46	161903	87.651	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.650%
24) Chloroform-d	4.243	84	418501	45.359	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.720%
26) 1,2-Dichloroethane-d4	4.937	65	257765	47.730	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.460%
32) Benzene-d6	4.953	84	817794	44.292	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.580%
36) 1,2-Dichloropropane-d6	5.982	67	269431	45.826	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.660%
41) Toluene-d8	7.236	98	714587	42.682	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.360%
43) trans-1,3-Dichloroprop...	7.551	79	107962	39.529	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.060%
47) 2-Hexanone-d5	8.024	63	100320	80.807	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.810%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	301967	44.203	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.400%
66) 1,2-Dichlorobenzene-d4	11.554	152	275354	49.694	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.380%
Target Compounds						
39) cis-1,3-Dichloropropene	6.911	75	6750	0.920	ug/L	Qvalue # 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037807.D
Acq On : 10 Oct 2024 15:47
Operator : SY/MD
Sample : P4379-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 11 05:14:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

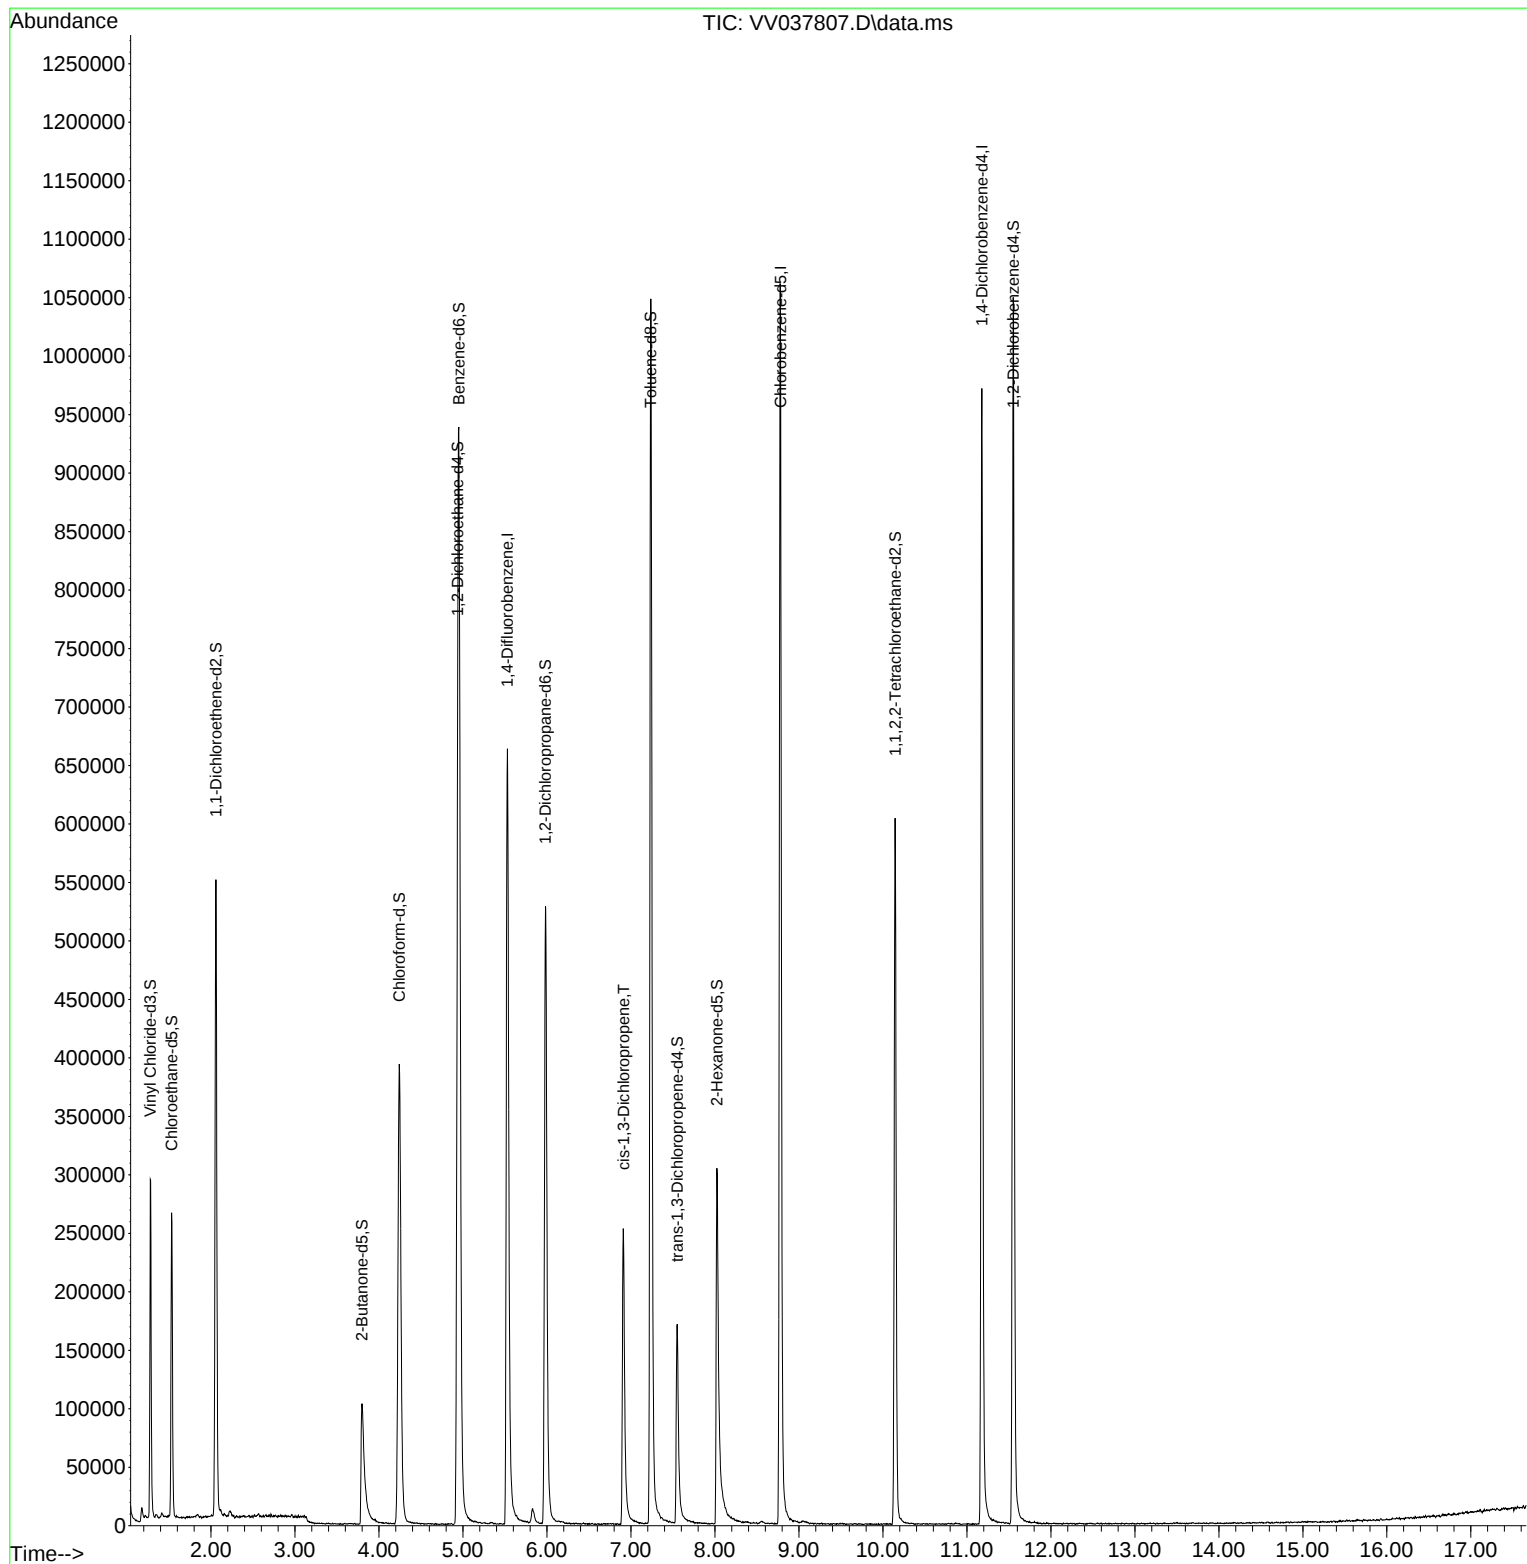

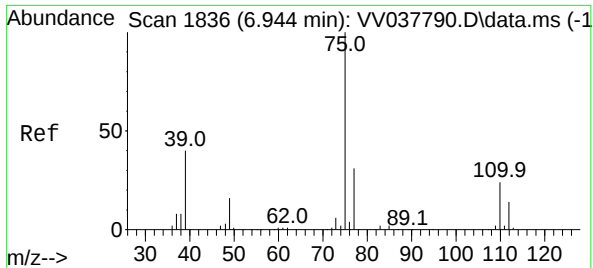

#39
 cis-1,3-Dichloropropene
 Concen: 0.920 ug/L
 RT: 6.911 min Scan# 11
 Delta R.T. -0.032 min
 Lab File: VV037807.D
 Acq: 10 Oct 2024 15:47

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 6750
 Ion Ratio Lower Upper
 75 100
 77 53.4 21.8 40.4#

