

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037793.D
 Acq On : 10 Oct 2024 10:46
 Operator : SY/MD
 Sample : P4352-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE0

Quant Time: Oct 11 05:11:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	613590	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	611691	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	280455	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	210857	39.147	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	78.300%		
7) Chloroethane-d5	1.532	69	180957	43.281	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.560%		
11) 1,1-Dichloroethene-d2	2.059	65	98525	43.782	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.560%		
21) 2-Butanone-d5	3.796	46	158227	82.474	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.470%		
24) Chloroform-d	4.239	84	435094	45.403	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.800%		
26) 1,2-Dichloroethane-d4	4.934	65	264406	47.138	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.280%		
32) Benzene-d6	4.950	84	854949	44.666	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.340%		
36) 1,2-Dichloropropane-d6	5.982	67	277415	45.515	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.020%		
41) Toluene-d8	7.236	98	756455	43.583	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.160%		
43) trans-1,3-Dichloroprop...	7.548	79	116487	41.141	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.280%		
47) 2-Hexanone-d5	8.021	63	94314	73.280	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	73.280%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	295932	41.786	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.580%		
66) 1,2-Dichlorobenzene-d4	11.551	152	291108	49.259	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.520%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	65091	34.609	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037793.D
Acq On : 10 Oct 2024 10:46
Operator : SY/MD
Sample : P4352-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE0

Quant Time: Oct 11 05:11:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

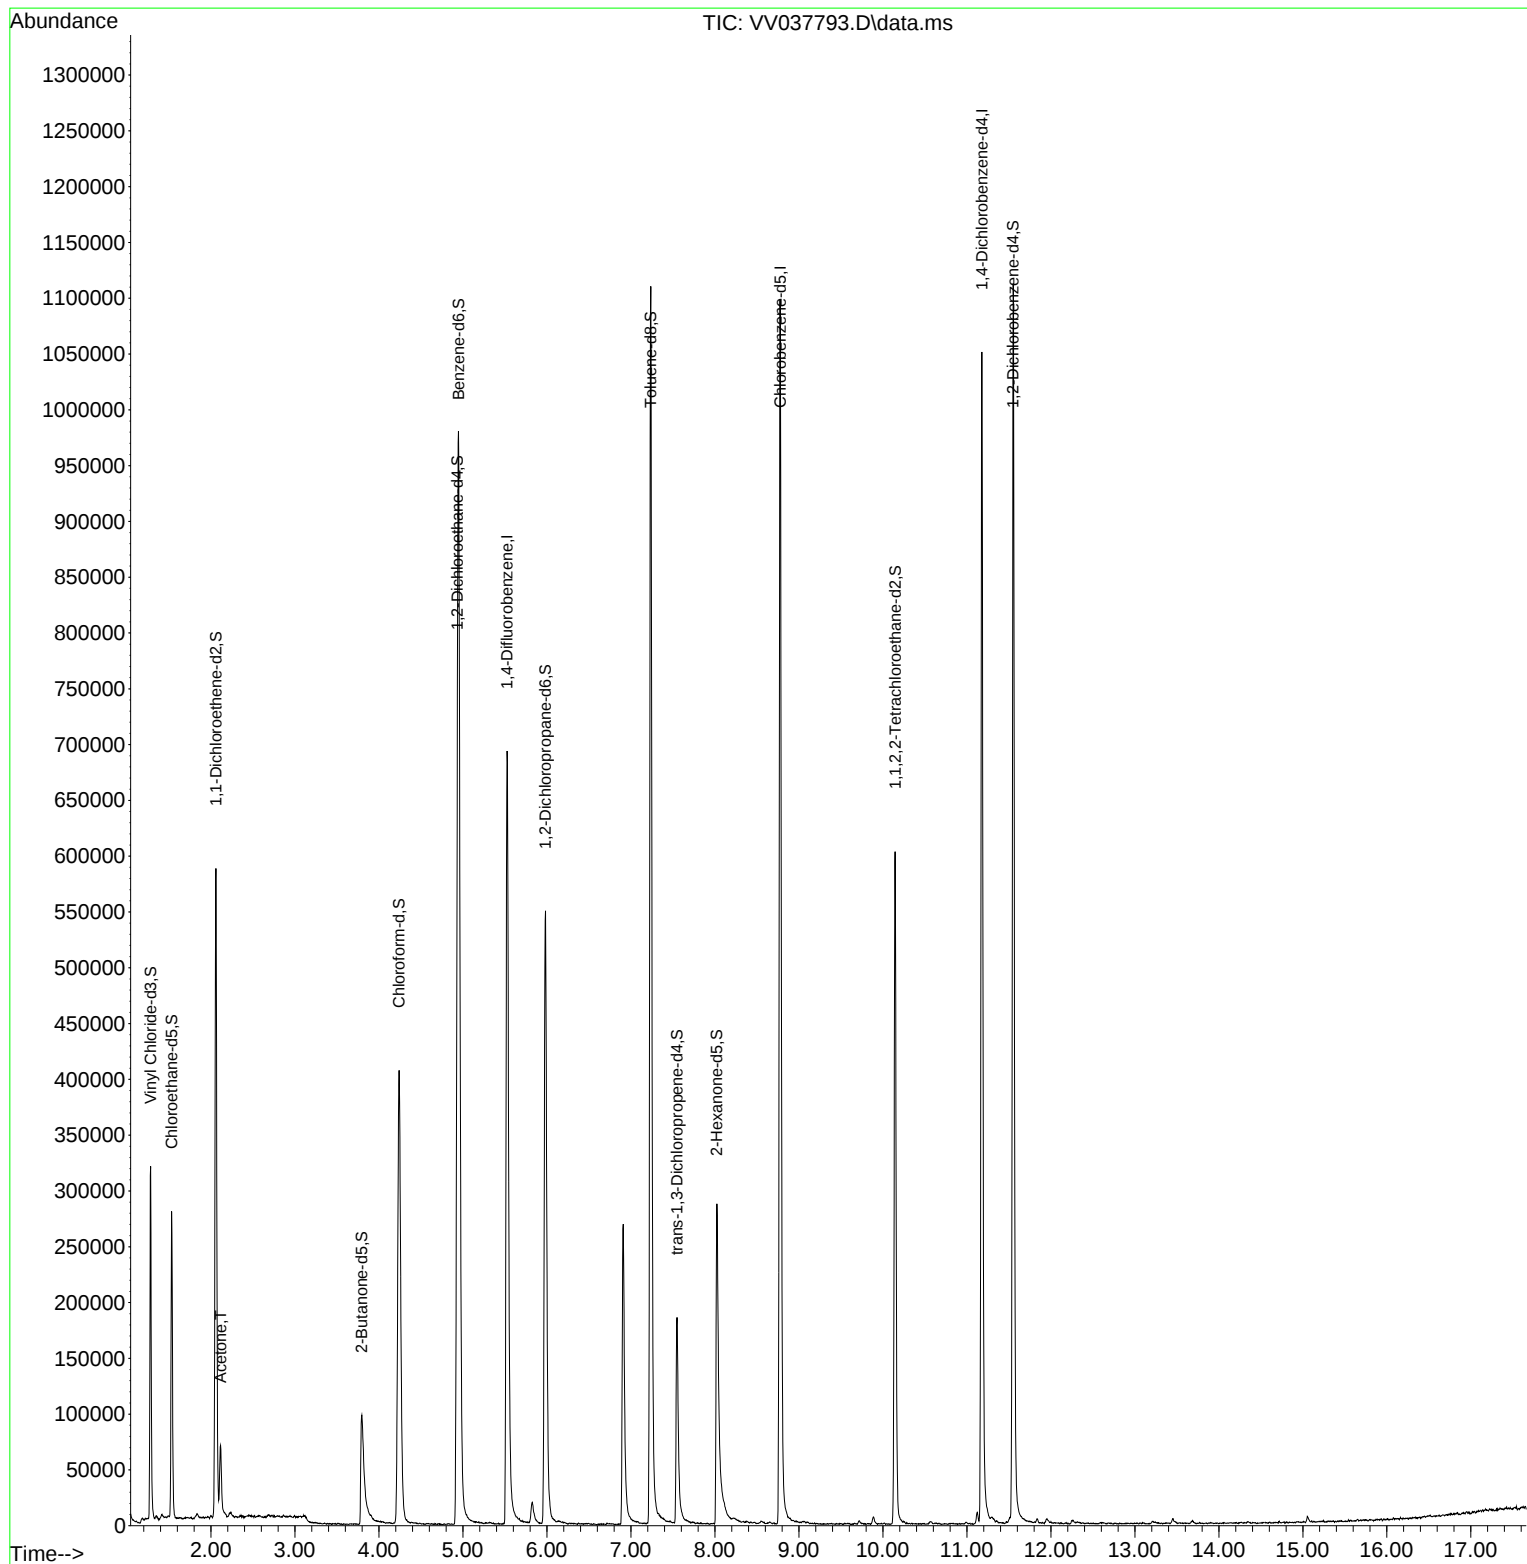

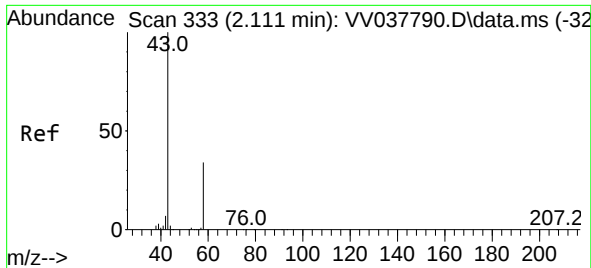

#13

Acetone

Concen: 34.609 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV037793.D


Acq: 10 Oct 2024 10:46

Instrument :

MSVOA_V

ClientSampleId :

A4FE0

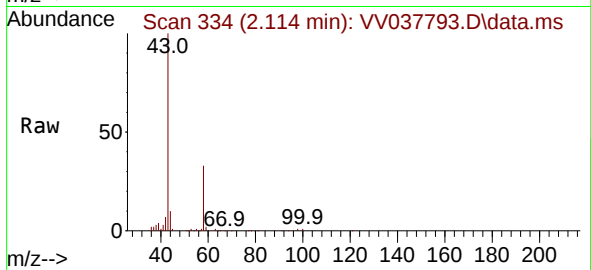

Tgt Ion: 43 Resp: 65091

Ion Ratio Lower Upper

43 100

58 34.0 0.0 66.6

