

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037795.D
 Acq On : 10 Oct 2024 11:29
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Quant Time: Oct 11 05:12:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	585692	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	581747	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	262422	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	195115	37.949	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.900%
7) Chloroethane-d5	1.532	69	167230	41.903	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.800%
11) 1,1-Dichloroethene-d2	2.056	65	89825	41.817	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.640%
21) 2-Butanone-d5	3.799	46	155173	84.735	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	84.730%
24) Chloroform-d	4.243	84	404585	44.230	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.460%
26) 1,2-Dichloroethane-d4	4.937	65	248998	46.506	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.020%
32) Benzene-d6	4.953	84	798906	43.886	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.780%
36) 1,2-Dichloropropane-d6	5.982	67	252733	43.599	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.200%
41) Toluene-d8	7.236	98	703464	42.616	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.240%
43) trans-1,3-Dichloroprop...	7.551	79	108539	40.307	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.620%
47) 2-Hexanone-d5	8.024	63	92043	75.197	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.200%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	284670	42.265	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.540%
66) 1,2-Dichlorobenzene-d4	11.551	152	269742	48.780	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.560%
Target Compounds						
13) Acetone	2.114	43	107381	59.815	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037795.D
Acq On : 10 Oct 2024 11:29
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6


Quant Time: Oct 11 05:12:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

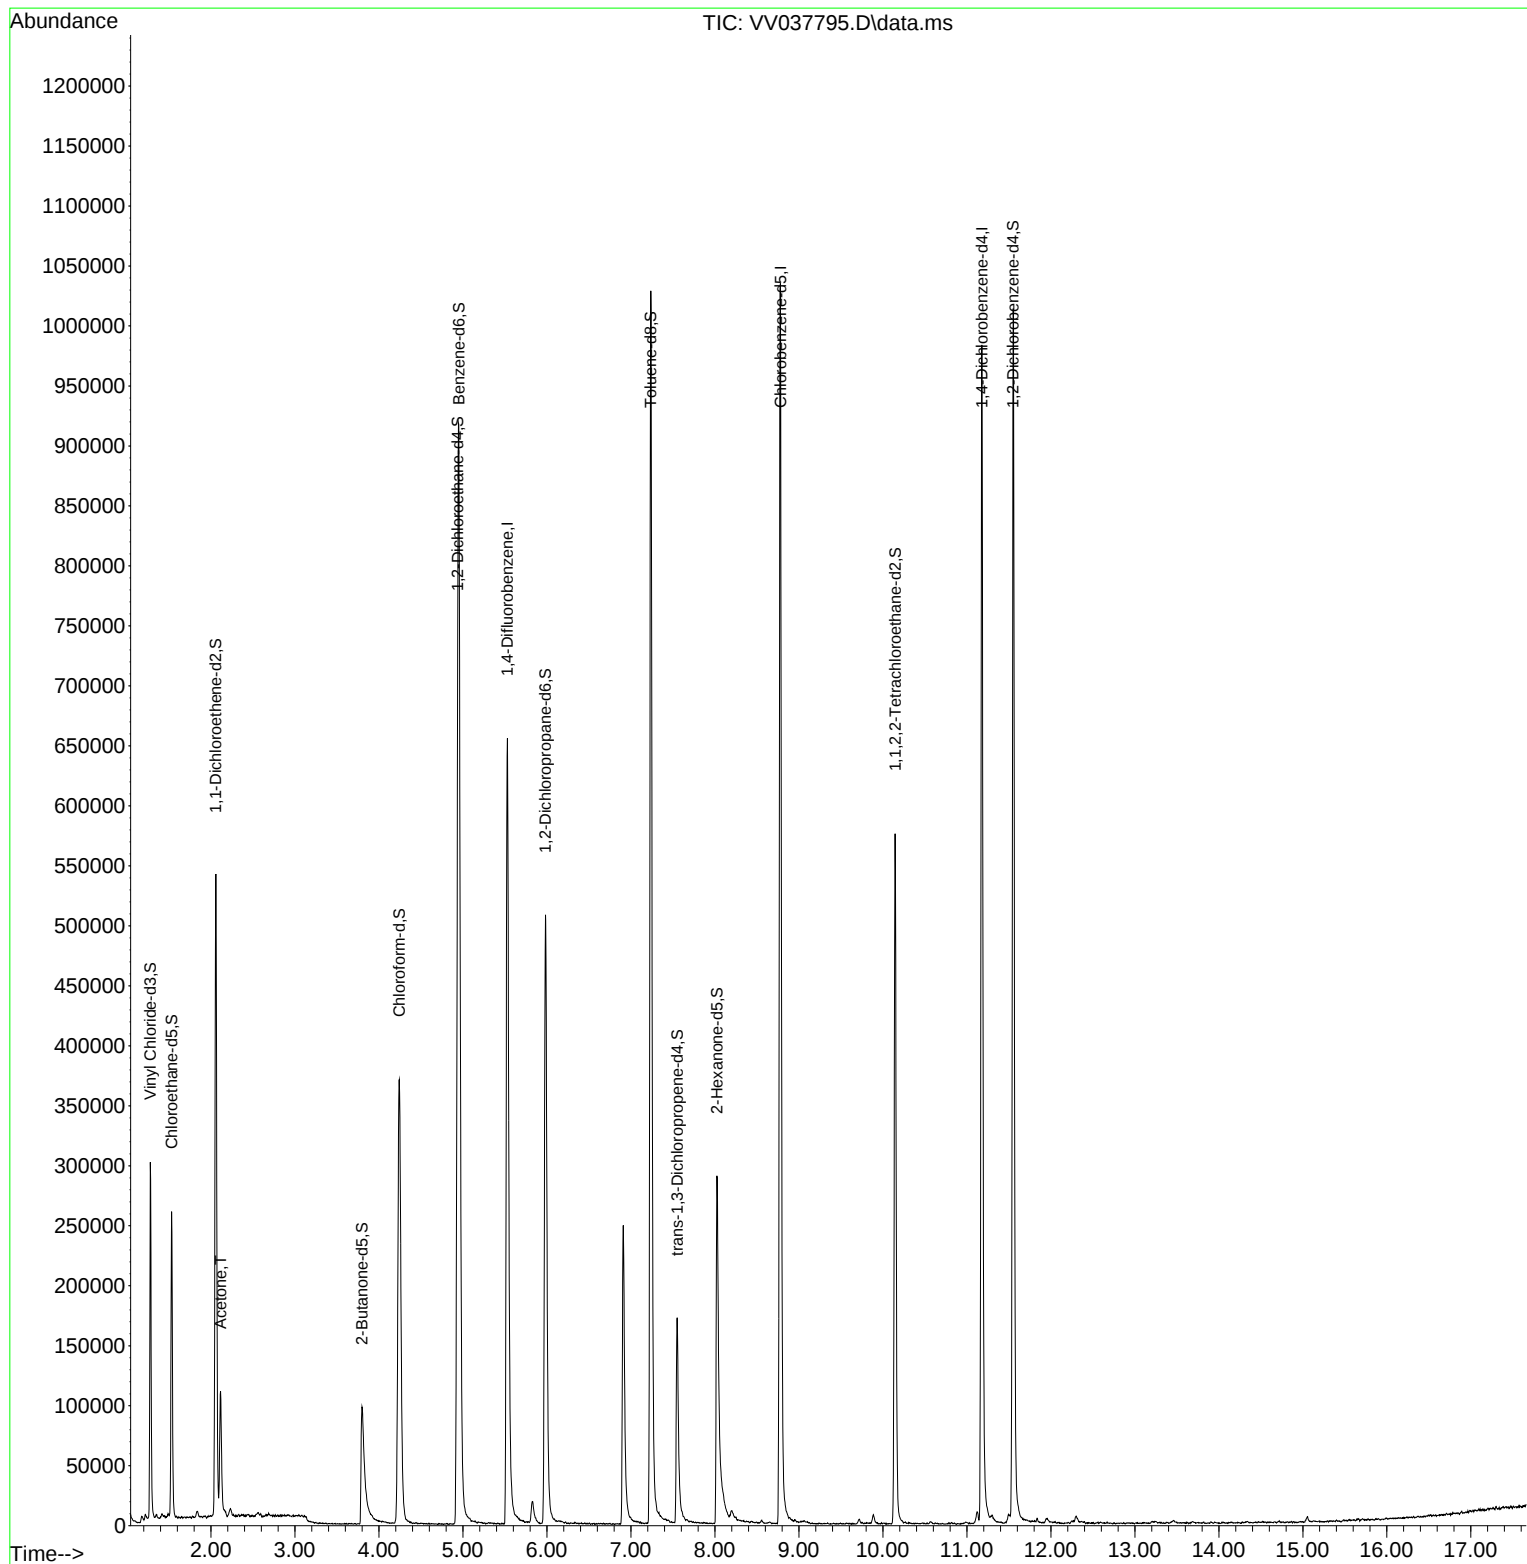

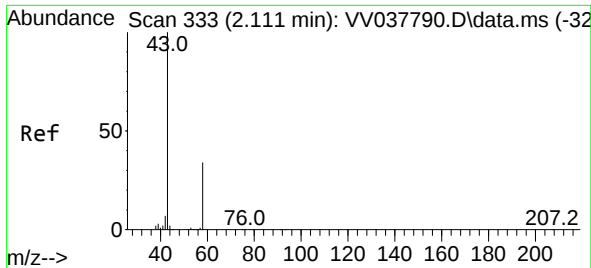

#13
Acetone
Concen: 59.815 ug/L
RT: 2.114 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV037795.D
Acq: 10 Oct 2024 11:29

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

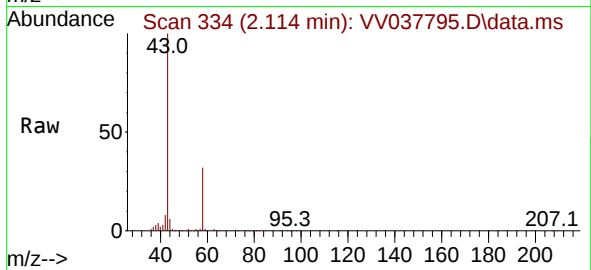

Tgt Ion: 43 Resp: 107381
Ion Ratio Lower Upper
43 100
58 31.8 0.0 66.6

