

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037804.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4379-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL96

Quant Time: Oct 11 05:14:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	567574	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	568130	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	249210	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	188387	37.811	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.620%
7) Chloroethane-d5	1.532	69	165793	42.869	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.740%
11) 1,1-Dichloroethene-d2	2.060	65	88782	42.651	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.300%
21) 2-Butanone-d5	3.796	46	160645	90.523	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.520%
24) Chloroform-d	4.243	84	407677	45.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.980%
26) 1,2-Dichloroethane-d4	4.937	65	248031	47.804	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.600%
32) Benzene-d6	4.950	84	794998	44.718	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.440%
36) 1,2-Dichloropropane-d6	5.982	67	258381	45.642	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.280%
41) Toluene-d8	7.236	98	695217	43.126	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.260%
43) trans-1,3-Dichloroprop...	7.548	79	108780	41.365	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.720%
47) 2-Hexanone-d5	8.024	63	100773	84.302	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.300%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	295936	44.991	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.980%
66) 1,2-Dichlorobenzene-d4	11.554	152	264686	50.403	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds						
20) cis-1,2-Dichloroethene	3.806	96	113252	25.317	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037804.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4379-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL96


Quant Time: Oct 11 05:14:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

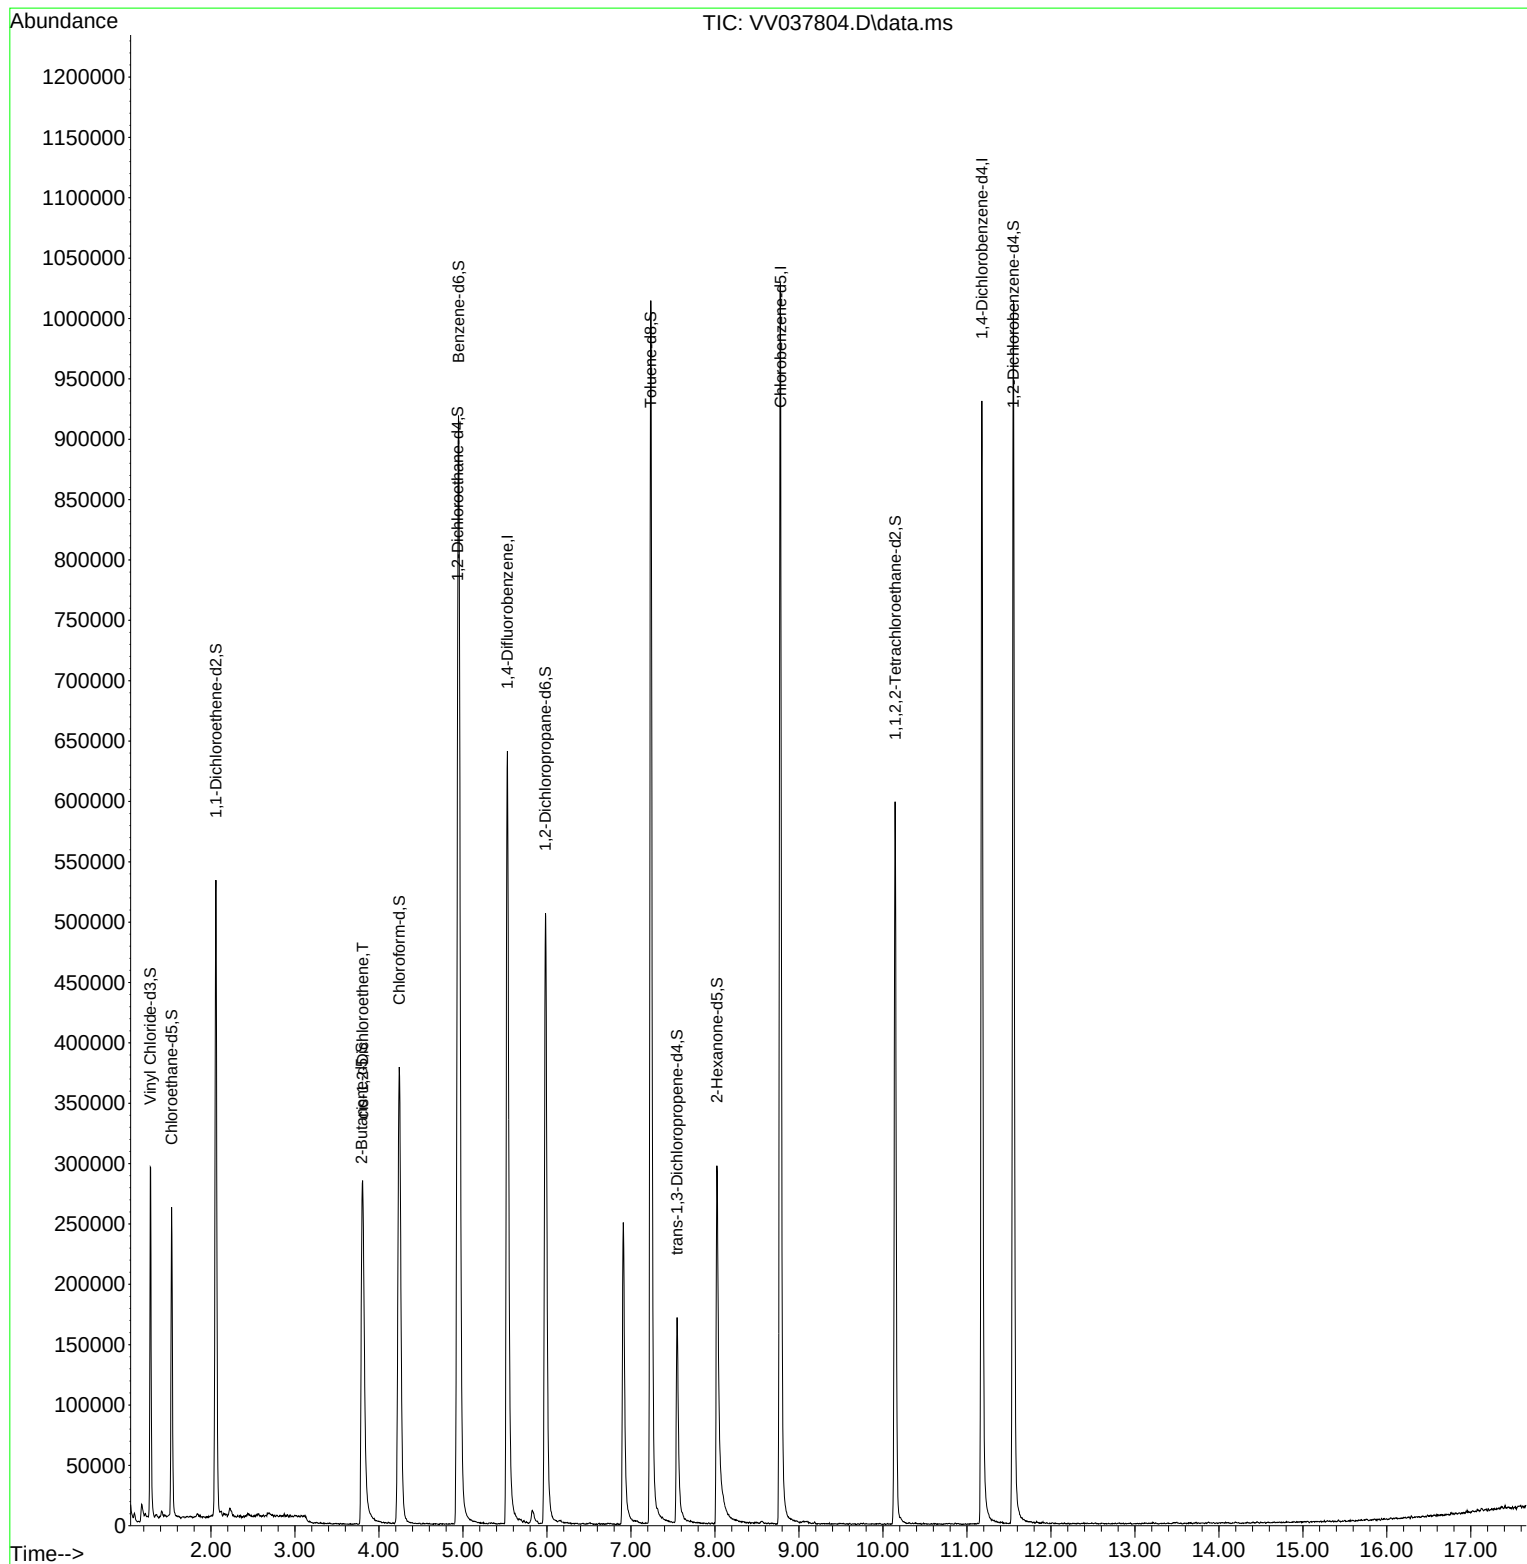

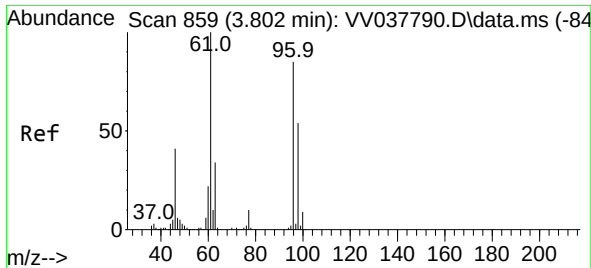

#20
 cis-1,2-Dichloroethene
 Concen: 25.317 ug/L
 RT: 3.806 min Scan# 80
 Delta R.T. 0.003 min
 Lab File: VV037804.D
 Acq: 10 Oct 2024 14:42

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL96

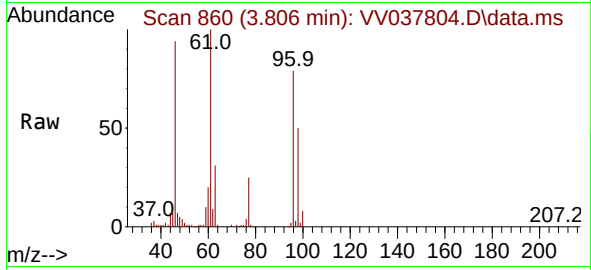

Tgt Ion:	96	Resp:	113252
Ion	Ratio	Lower	Upper
96	100		
61	126.9	85.0	157.8
98	63.5	44.2	82.0

