

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037792.D
 Acq On : 10 Oct 2024 10:16
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.178	37	43	45	rBV2	3137	3253	0.13%	0.018%
2	1.281	67	75	89	rBV	312398	335780	13.62%	1.908%
3	1.532	145	153	168	rVB	277634	330620	13.42%	1.879%
4	2.059	307	317	332	rBV	577168	825337	33.49%	4.690%
5	3.323	708	710	715	rBV4	557	473	0.02%	0.003%
6	3.358	719	721	726	rVB3	835	538	0.02%	0.003%
7	3.571	784	787	790	rBV	894	644	0.03%	0.004%
8	3.748	839	842	846	rVB2	506	473	0.02%	0.003%
9	3.799	849	858	897	rBV	110608	340467	13.82%	1.935%
10	4.143	963	965	970	rVB4	959	758	0.03%	0.004%
11	4.243	980	996	1026	rVV2	408247	1049613	42.59%	5.965%
12	4.458	1061	1063	1068	rBV3	594	476	0.02%	0.003%
13	4.516	1077	1081	1083	rBV4	746	483	0.02%	0.003%
14	4.529	1083	1085	1089	rVB5	797	444	0.02%	0.003%
15	4.596	1104	1106	1111	rBV2	653	719	0.03%	0.004%
16	4.802	1166	1170	1175	rVB4	1030	728	0.03%	0.004%
17	4.870	1190	1191	1196	rVB3	988	492	0.02%	0.003%
18	4.895	1196	1199	1200	rBV	766	475	0.02%	0.003%
19	4.947	1200	1215	1248	rBV2	985914	2464467	100.00%	14.005%
20	5.529	1385	1396	1428	rBV	653806	1352348	54.87%	7.685%
21	5.825	1478	1488	1507	rBV4	16033	38662	1.57%	0.220%
22	5.924	1516	1519	1520	rBV2	720	435	0.02%	0.002%
23	5.982	1525	1537	1574	rBV	550201	1152758	46.78%	6.551%
24	6.387	1661	1663	1666	rVB4	916	425	0.02%	0.002%
25	6.403	1666	1668	1675	rVB3	520	473	0.02%	0.003%
26	6.436	1675	1678	1681	rBV3	639	517	0.02%	0.003%
27	6.474	1685	1690	1693	rBV2	884	872	0.04%	0.005%
28	6.661	1745	1748	1751	rVB4	897	437	0.02%	0.002%
29	6.728	1764	1769	1773	rBV5	737	721	0.03%	0.004%
30	6.866	1806	1812	1814	rBV2	760	717	0.03%	0.004%
31	6.908	1815	1825	1859	rBV	270694	526795	21.38%	2.994%
32	7.198	1910	1915	1916	rBV5	1094	861	0.03%	0.005%
33	7.236	1916	1927	1956	rBV	1070219	1896142	76.94%	10.776%
34	7.548	2016	2024	2057	rBV	183846	345860	14.03%	1.965%
35	7.860	2118	2121	2122	rBV2	926	484	0.02%	0.003%
36	7.895	2129	2132	2134	rBV3	1066	744	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037792.D
 Acq On : 10 Oct 2024 10:16
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.024	2164	2172	2213	rBV2	310525	706009	28.65%	4.012%
38	8.416	2292	2294	2300	rVB6	1217	1140	0.05%	0.006%
39	8.548	2329	2335	2336	rBV4	1770	1747	0.07%	0.010%
40	8.776	2395	2406	2436	rBV	1022036	1724775	69.99%	9.802%
41	9.159	2520	2525	2527	rBV4	760	548	0.02%	0.003%
42	9.355	2584	2586	2591	rVB3	873	674	0.03%	0.004%
43	9.484	2619	2626	2629	rBV4	1205	1518	0.06%	0.009%
44	9.574	2647	2654	2657	rBV8	1087	1355	0.05%	0.008%
45	9.619	2666	2668	2676	rVB4	878	838	0.03%	0.005%
46	9.654	2676	2679	2681	rBV2	1003	620	0.03%	0.004%
47	9.712	2691	2697	2698	rBV2	588	499	0.02%	0.003%
48	9.738	2701	2705	2709	rVV3	867	900	0.04%	0.005%
49	9.757	2709	2711	2715	rVV2	890	569	0.02%	0.003%
50	9.834	2732	2735	2737	rBV3	580	450	0.02%	0.003%
51	9.869	2742	2746	2749	rBV4	1489	1533	0.06%	0.009%
52	9.905	2755	2757	2761	rVB3	949	614	0.02%	0.003%
53	10.146	2819	2832	2865	rBV	660472	1051695	42.67%	5.977%
54	10.445	2922	2925	2930	rVB6	1000	642	0.03%	0.004%
55	10.471	2930	2933	2936	rBV3	800	571	0.02%	0.003%
56	10.496	2938	2941	2947	rVB4	860	925	0.04%	0.005%
57	10.522	2947	2949	2955	rBV2	725	551	0.02%	0.003%
58	10.586	2965	2969	2973	rVB3	617	569	0.02%	0.003%
59	10.612	2973	2977	2979	rBV2	562	485	0.02%	0.003%
60	10.789	3026	3032	3036	rBV5	1323	1494	0.06%	0.008%
61	10.857	3049	3053	3055	rBV4	1023	827	0.03%	0.005%
62	11.014	3098	3102	3105	rVB5	696	606	0.02%	0.003%
63	11.059	3112	3116	3120	rBV3	809	696	0.03%	0.004%
64	11.136	3130	3140	3142	rBV5	2224	3529	0.14%	0.020%
65	11.178	3142	3153	3183	rBV	979663	1577867	64.02%	8.967%
66	11.422	3225	3229	3230	rBV4	627	499	0.02%	0.003%
67	11.551	3256	3269	3301	rBV	1116871	1784846	72.42%	10.143%
68	11.750	3329	3331	3335	rVB2	852	596	0.02%	0.003%
69	11.828	3353	3355	3363	rVB4	1135	1044	0.04%	0.006%
70	12.014	3410	3413	3418	rVB6	825	652	0.03%	0.004%
71	12.088	3432	3436	3438	rBV2	779	653	0.03%	0.004%
72	12.136	3447	3451	3454	rVB4	679	535	0.02%	0.003%
73	12.191	3464	3468	3472	rBV5	1003	958	0.04%	0.005%
74	12.233	3479	3481	3486	rVB	960	740	0.03%	0.004%
75	12.258	3486	3489	3493	rBV4	723	620	0.03%	0.004%
76	12.284	3495	3497	3499	rBV2	688	446	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037792.D
 Acq On : 10 Oct 2024 10:16
 Operator : SY/MD
 Sample : VV1010WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.329	3506	3511	3513	rBV2	626	572	0.02%	0.003%
78	12.403	3530	3534	3536	rBV3	728	481	0.02%	0.003%
79	12.422	3536	3540	3543	rBV3	560	465	0.02%	0.003%
80	12.467	3552	3554	3558	rBV2	870	663	0.03%	0.004%
81	12.564	3580	3584	3585	rBV	759	438	0.02%	0.002%
82	12.586	3585	3591	3592	rBV5	1660	1353	0.05%	0.008%
83	12.699	3624	3626	3630	rVB3	1109	788	0.03%	0.004%
84	12.911	3689	3692	3697	rVV5	680	713	0.03%	0.004%
85	12.969	3706	3710	3714	rBV3	596	464	0.02%	0.003%
86	13.075	3740	3743	3746	rBV4	645	435	0.02%	0.002%
87	13.146	3759	3765	3769	rVB5	628	705	0.03%	0.004%
88	13.210	3777	3785	3797	rBV10	3524	6903	0.28%	0.039%
89	13.300	3809	3813	3818	rVB4	789	745	0.03%	0.004%
90	13.455	3850	3861	3868	rBV4	6483	13470	0.55%	0.077%
91	13.545	3886	3889	3894	rVB3	667	626	0.03%	0.004%
92	13.683	3922	3932	3946	rBV6	5354	9904	0.40%	0.056%
93	13.975	4019	4023	4027	rBV3	2069	1714	0.07%	0.010%
94	14.094	4055	4060	4061	rBV3	909	728	0.03%	0.004%
95	14.139	4070	4074	4076	rBV2	715	592	0.02%	0.003%
96	14.355	4138	4141	4144	rBV2	779	511	0.02%	0.003%
97	14.471	4175	4177	4180	rBV3	940	450	0.02%	0.003%
98	14.763	4262	4268	4272	rBV6	1132	1123	0.05%	0.006%
99	15.030	4349	4351	4356	rBV5	956	781	0.03%	0.004%
100	15.798	4588	4590	4593	rBV3	1271	656	0.03%	0.004%




Sum of corrected areas: 17596606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037792.D
Acq On : 10 Oct 2024 10:16
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

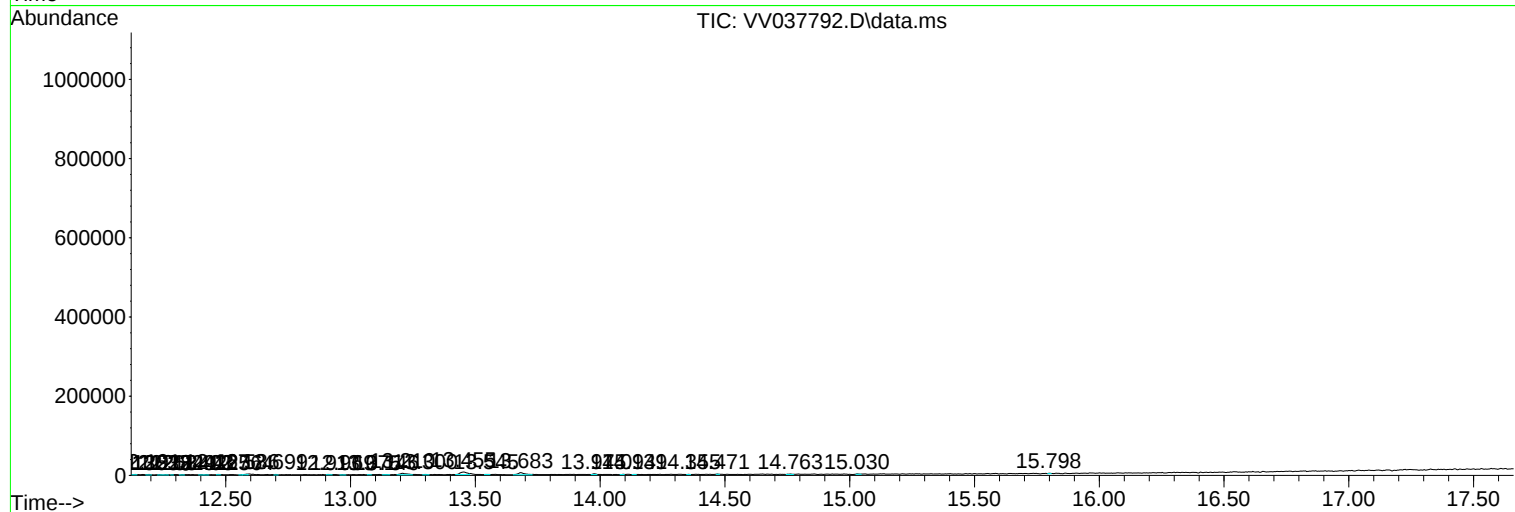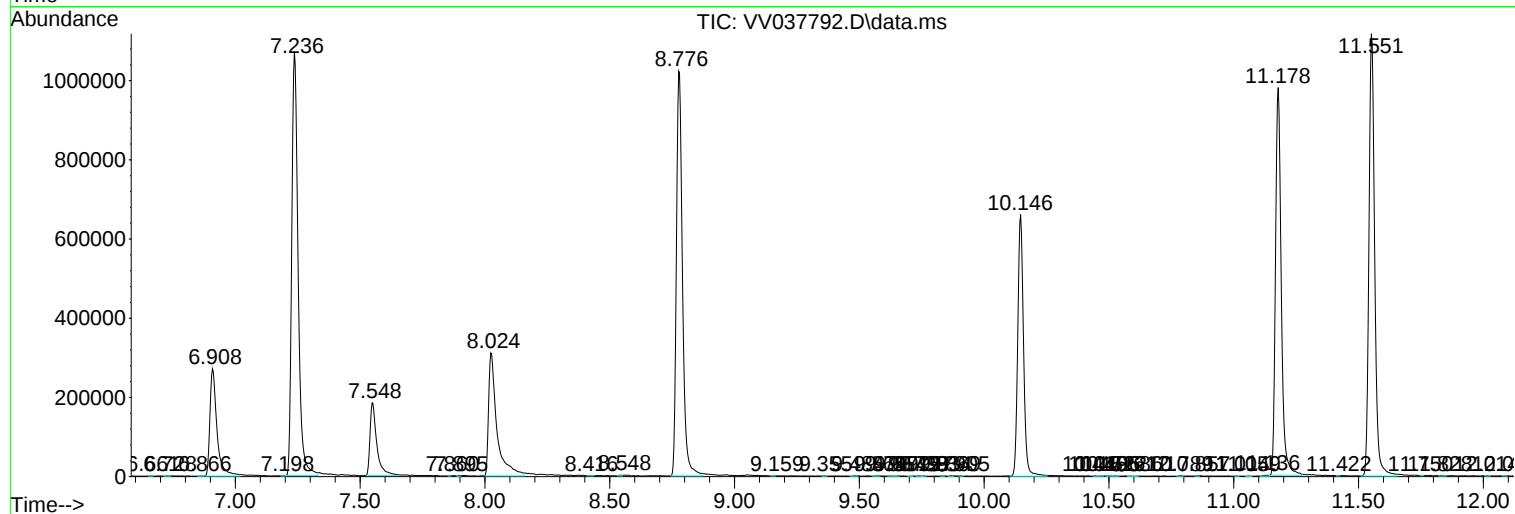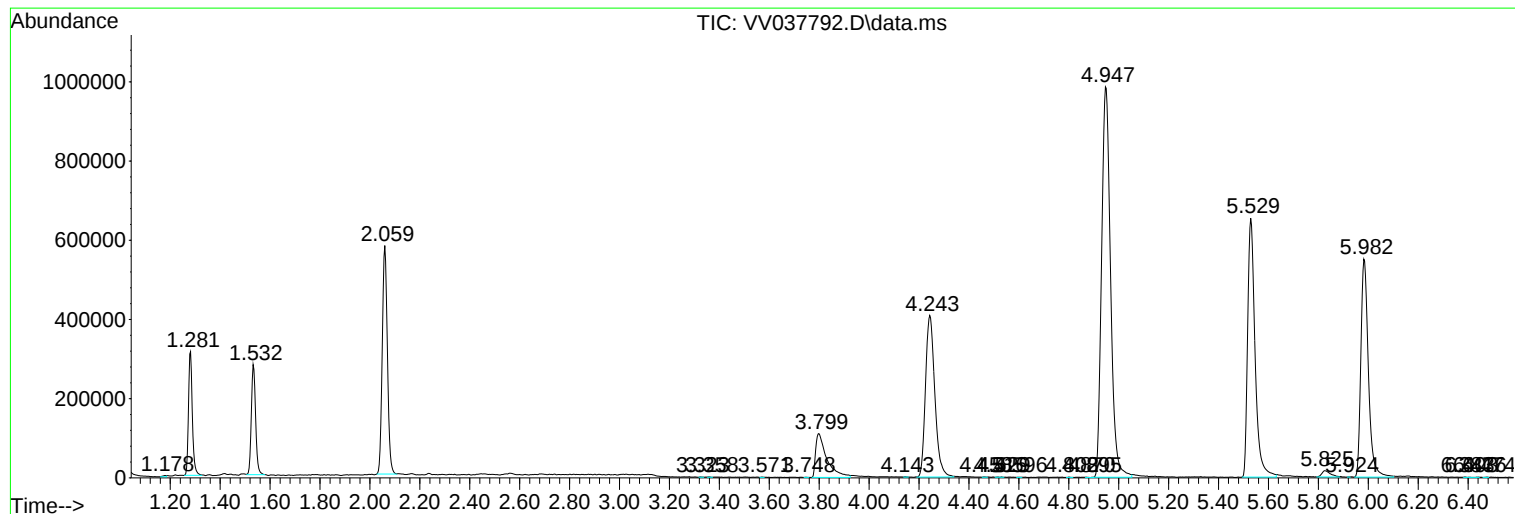

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037792.D
Acq On : 10 Oct 2024 10:16
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037792.D
Acq On : 10 Oct 2024 10:16
Operator : SY/MD
Sample : VV1010WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------