

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037795.D
 Acq On : 10 Oct 2024 11:29
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	50	rBV2	5388	9175	0.40%	0.054%
2	1.220	52	56	63	rVV3	5306	7237	0.31%	0.043%
3	1.278	67	74	89	rVV	296579	315706	13.67%	1.870%
4	1.532	145	153	167	rVB	254716	302870	13.11%	1.794%
5	2.060	307	317	327	rBV	533220	770140	33.35%	4.562%
6	2.114	327	334	348	rVB	99582	153628	6.65%	0.910%
7	3.561	780	784	787	rBV	527	504	0.02%	0.003%
8	3.799	849	858	903	rBV2	97655	310964	13.47%	1.842%
9	4.243	979	996	1026	rBV	369406	947593	41.03%	5.613%
10	4.378	1036	1038	1044	rVB4	1578	1342	0.06%	0.008%
11	4.596	1100	1106	1109	rVB5	990	827	0.04%	0.005%
12	4.622	1109	1114	1117	rBV4	641	564	0.02%	0.003%
13	4.712	1139	1142	1146	rBV3	834	758	0.03%	0.004%
14	4.854	1183	1186	1192	rVB3	610	599	0.03%	0.004%
15	4.947	1198	1215	1254	rBV2	917832	2309343	100.00%	13.679%
16	5.185	1285	1289	1291	rBV3	995	835	0.04%	0.005%
17	5.307	1322	1327	1331	rBV6	925	1001	0.04%	0.006%
18	5.529	1385	1396	1425	rBV	654900	1353908	58.63%	8.020%
19	5.777	1471	1473	1477	rBV4	909	573	0.02%	0.003%
20	5.831	1480	1490	1500	rBV5	16339	34748	1.50%	0.206%
21	5.982	1524	1537	1568	rBV	507145	1048953	45.42%	6.213%
22	6.223	1607	1612	1616	rVB7	1429	1334	0.06%	0.008%
23	6.333	1644	1646	1651	rVV5	964	674	0.03%	0.004%
24	6.368	1655	1657	1661	rVB3	988	704	0.03%	0.004%
25	6.391	1661	1664	1665	rBV3	736	504	0.02%	0.003%
26	6.506	1696	1700	1704	rVB5	1213	1076	0.05%	0.006%
27	6.532	1704	1708	1711	rBV4	686	548	0.02%	0.003%
28	6.555	1711	1715	1716	rBV2	679	538	0.02%	0.003%
29	6.613	1731	1733	1738	rVB5	623	522	0.02%	0.003%
30	6.751	1772	1776	1780	rVB4	948	806	0.03%	0.005%
31	6.786	1784	1787	1792	rVB5	1002	840	0.04%	0.005%
32	6.908	1815	1825	1850	rBV	249157	482391	20.89%	2.857%
33	7.117	1888	1890	1893	rVB4	1094	562	0.02%	0.003%
34	7.172	1903	1907	1909	rBV5	544	485	0.02%	0.003%
35	7.236	1916	1927	1956	rBV	1027196	1825875	79.06%	10.816%
36	7.551	2016	2025	2056	rBV	170711	327036	14.16%	1.937%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037795.D
 Acq On : 10 Oct 2024 11:29
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.024	2162	2172	2217	rBV3	289991	681699	29.52%	4.038%
38	8.555	2334	2337	2345	rVB4	2515	2752	0.12%	0.016%
39	8.690	2375	2379	2382	rBV4	638	539	0.02%	0.003%
40	8.780	2395	2407	2437	rBV	1033762	1734934	75.13%	10.277%
41	9.342	2579	2582	2587	rVB5	978	744	0.03%	0.004%
42	9.413	2601	2604	2607	rBV4	714	511	0.02%	0.003%
43	9.452	2614	2616	2622	rVB2	740	544	0.02%	0.003%
44	9.493	2627	2629	2633	rVV4	841	528	0.02%	0.003%
45	9.564	2648	2651	2654	rBV4	774	515	0.02%	0.003%
46	9.635	2671	2673	2676	rVB3	1024	554	0.02%	0.003%
47	9.654	2676	2679	2683	rBV3	855	635	0.03%	0.004%
48	9.718	2690	2699	2706	rVV10	3739	5898	0.26%	0.035%
49	9.754	2706	2710	2714	rVB4	949	733	0.03%	0.004%
50	9.886	2742	2751	2761	rBV8	7287	12422	0.54%	0.074%
51	9.982	2777	2781	2784	rBV4	1269	791	0.03%	0.005%
52	10.005	2784	2788	2789	rBV2	641	512	0.02%	0.003%
53	10.050	2800	2802	2806	rBV3	642	496	0.02%	0.003%
54	10.075	2806	2810	2813	rBV5	569	579	0.03%	0.003%
55	10.146	2816	2832	2856	rBV	575378	929490	40.25%	5.506%
56	10.387	2903	2907	2910	rBV5	698	510	0.02%	0.003%
57	10.526	2947	2950	2954	rVB4	933	678	0.03%	0.004%
58	10.622	2977	2980	2986	rBV6	971	980	0.04%	0.006%
59	10.706	3002	3006	3011	rBV5	626	584	0.03%	0.003%
60	10.786	3029	3031	3034	rVB2	1307	672	0.03%	0.004%
61	10.815	3035	3040	3044	rBV4	1176	1215	0.05%	0.007%
62	10.853	3050	3052	3056	rVB2	982	605	0.03%	0.004%
63	10.889	3060	3063	3065	rBV2	828	638	0.03%	0.004%
64	10.985	3086	3093	3101	rBV8	1333	2287	0.10%	0.014%
65	11.034	3105	3108	3111	rBV3	1028	642	0.03%	0.004%
66	11.088	3122	3125	3126	rBV2	1113	589	0.03%	0.003%
67	11.120	3126	3135	3142	rBV7	8786	14789	0.64%	0.088%
68	11.178	3143	3153	3181	rVV	979010	1561225	67.60%	9.248%
69	11.493	3243	3251	3258	rBV8	6599	13003	0.56%	0.077%
70	11.551	3258	3269	3301	rVB	1009249	1647777	71.35%	9.761%
71	11.767	3333	3336	3338	rBV5	943	596	0.03%	0.004%
72	11.834	3353	3357	3363	rBV5	3087	2824	0.12%	0.017%
73	11.905	3376	3379	3383	rBV5	935	645	0.03%	0.004%
74	11.943	3383	3391	3393	rBV9	3537	4053	0.18%	0.024%
75	12.053	3423	3425	3428	rVB4	1107	527	0.02%	0.003%
76	12.204	3469	3472	3474	rBV4	771	490	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037795.D
 Acq On : 10 Oct 2024 11:29
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.249	3478	3486	3489	rBV8	2256	2937	0.13%	0.017%
78	12.304	3496	3503	3513	rVB9	4904	8966	0.39%	0.053%
79	12.397	3529	3532	3537	rVB4	1655	1454	0.06%	0.009%
80	12.538	3573	3576	3578	rVV4	740	482	0.02%	0.003%
81	12.561	3581	3583	3585	rVB2	1385	563	0.02%	0.003%
82	12.751	3637	3642	3643	rBV2	1006	678	0.03%	0.004%
83	13.005	3718	3721	3723	rBV2	893	676	0.03%	0.004%
84	13.091	3744	3748	3749	rBV3	853	501	0.02%	0.003%
85	13.204	3778	3783	3786	rBV5	1323	1392	0.06%	0.008%
86	13.374	3833	3836	3838	rBV3	915	619	0.03%	0.004%
87	13.619	3910	3912	3915	rBV3	1178	755	0.03%	0.004%
88	13.667	3924	3927	3929	rBV3	992	686	0.03%	0.004%
89	13.821	3971	3975	3979	rVB4	1106	870	0.04%	0.005%
90	13.869	3986	3990	3994	rBV3	589	561	0.02%	0.003%
91	13.905	3997	4001	4003	rBV4	1069	751	0.03%	0.004%
92	13.950	4011	4015	4022	rBV10	1050	1299	0.06%	0.008%
93	14.152	4076	4078	4083	rVB3	1027	743	0.03%	0.004%
94	14.278	4114	4117	4121	rVV4	1122	764	0.03%	0.005%
95	14.467	4174	4176	4179	rBV3	953	566	0.02%	0.003%
96	14.580	4208	4211	4214	rBV2	1107	790	0.03%	0.005%
97	14.664	4232	4237	4241	rBV6	914	1158	0.05%	0.007%
98	14.889	4303	4307	4310	rBV5	1216	1062	0.05%	0.006%
99	15.056	4349	4359	4366	rBV9	4551	7473	0.32%	0.044%
100	15.316	4437	4440	4442	rBV4	1014	734	0.03%	0.004%




Sum of corrected areas: 16881848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037795.D
Acq On : 10 Oct 2024 11:29
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

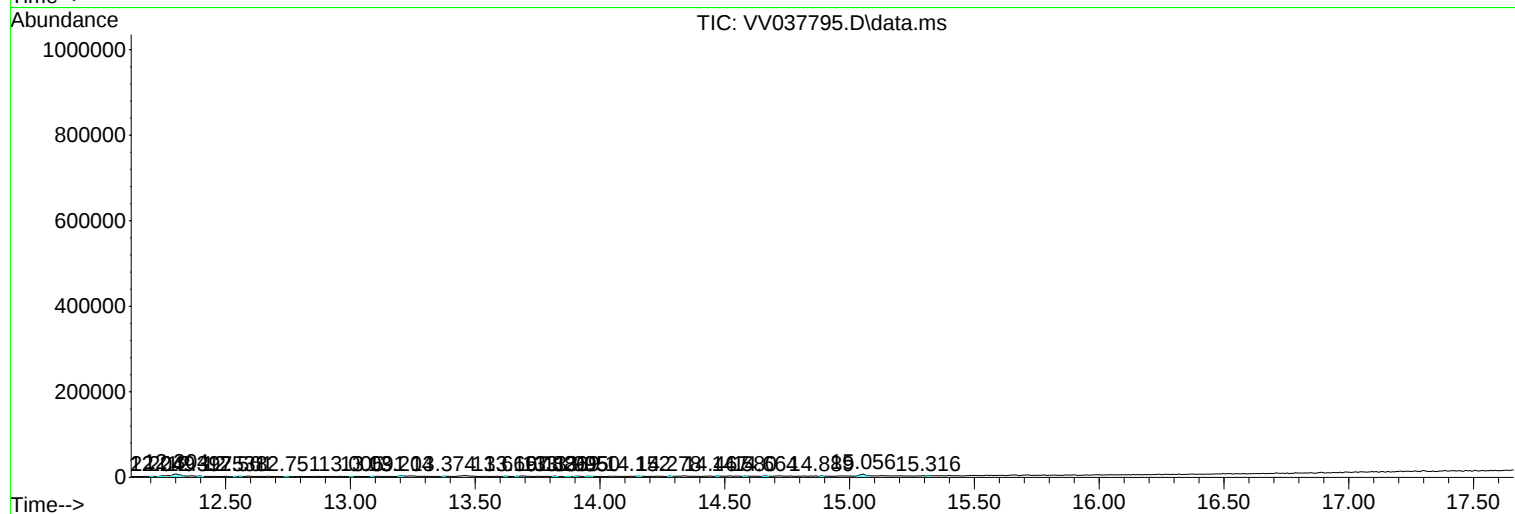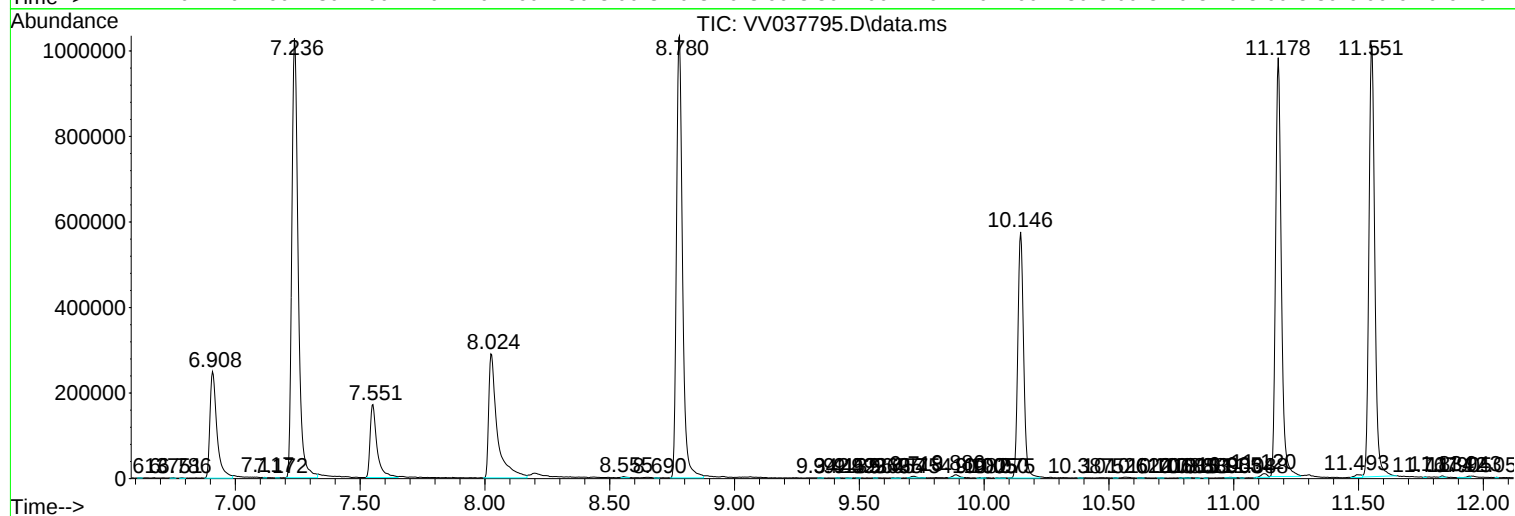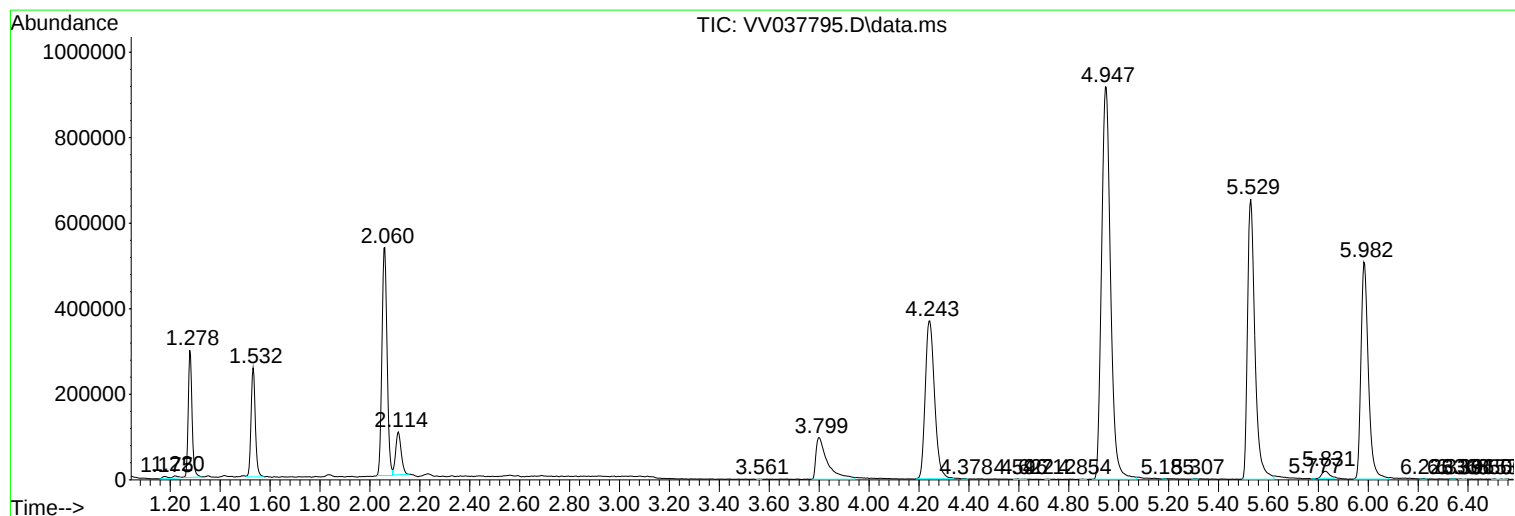

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037795.D
Acq On : 10 Oct 2024 11:29
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037795.D
Acq On : 10 Oct 2024 11:29
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc