

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037796.D
 Acq On : 10 Oct 2024 11:50
 Operator : SY/MD
 Sample : P4363-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	304148	320966	13.53%	1.877%
2	1.532	146	153	168	rVB	260729	306994	12.94%	1.796%
3	2.059	307	317	339	rVB	543111	795441	33.53%	4.652%
4	3.448	746	749	752	rBV3	452	343	0.01%	0.002%
5	3.497	759	764	767	rBV5	756	674	0.03%	0.004%
6	3.657	812	814	819	rVB2	599	437	0.02%	0.003%
7	3.686	819	823	825	rBV2	508	468	0.02%	0.003%
8	3.735	836	838	839	rBV	400	155	0.01%	0.001%
9	3.799	850	858	885	rBV2	103554	298361	12.58%	1.745%
10	4.243	980	996	1023	rBV	380126	970480	40.91%	5.676%
11	4.622	1112	1114	1118	rVB3	661	448	0.02%	0.003%
12	4.641	1118	1120	1121	rBV	299	135	0.01%	0.001%
13	4.706	1139	1140	1146	rBV	227	153	0.01%	0.001%
14	4.731	1146	1148	1153	rBV3	461	359	0.02%	0.002%
15	4.809	1170	1172	1177	rVB3	815	575	0.02%	0.003%
16	4.831	1177	1179	1181	rBV2	594	350	0.01%	0.002%
17	4.883	1193	1195	1196	rBV2	467	197	0.01%	0.001%
18	4.947	1199	1215	1253	rBV2	937031	2372412	100.00%	13.876%
19	5.317	1325	1330	1334	rBV5	1626	1846	0.08%	0.011%
20	5.484	1380	1382	1385	rBV3	610	287	0.01%	0.002%
21	5.529	1385	1396	1428	rBV	676133	1410648	59.46%	8.251%
22	5.982	1525	1537	1568	rBV	523027	1084651	45.72%	6.344%
23	6.368	1650	1657	1659	rBV5	1135	1059	0.04%	0.006%
24	6.381	1659	1661	1663	rBV2	473	280	0.01%	0.002%
25	6.426	1673	1675	1676	rBV	503	164	0.01%	0.001%
26	6.448	1680	1682	1686	rBV4	676	417	0.02%	0.002%
27	6.551	1711	1714	1715	rBV2	489	329	0.01%	0.002%
28	6.583	1721	1724	1729	rBV5	1080	806	0.03%	0.005%
29	6.690	1754	1757	1761	rBV3	440	386	0.02%	0.002%
30	6.728	1767	1769	1771	rBV3	674	382	0.02%	0.002%
31	6.783	1784	1786	1788	rBV2	553	303	0.01%	0.002%
32	6.815	1794	1796	1798	rVB2	547	242	0.01%	0.001%
33	6.828	1798	1800	1801	rBV2	288	115	0.00%	0.001%
34	6.841	1801	1804	1805	rBV2	416	152	0.01%	0.001%
35	6.870	1811	1813	1814	rBV3	314	135	0.01%	0.001%
36	6.908	1814	1825	1859	rVV	256698	500741	21.11%	2.929%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037796.D
Acq On : 10 Oct 2024 11:50
Operator : SY/MD
Sample : P4363-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAY5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

37	7.236	1917	1927	1970	rBV	1053148	1874689	79.02%	10.965%
38	7.548	2015	2024	2060	rBV	172800	336190	14.17%	1.966%
39	7.789	2096	2099	2102	rBV2	921	826	0.03%	0.005%
40	7.821	2107	2109	2113	rBV4	917	582	0.02%	0.003%
41	8.024	2162	2172	2215	rBV2	309879	719285	30.32%	4.207%
42	8.535	2328	2331	2332	rBV2	1146	689	0.03%	0.004%
43	8.664	2369	2371	2374	rBV3	582	315	0.01%	0.002%
44	8.680	2374	2376	2379	rVB2	698	351	0.01%	0.002%
45	8.776	2396	2406	2440	rBV	1066095	1796756	75.74%	10.509%
46	9.329	2576	2578	2579	rBV2	593	221	0.01%	0.001%
47	9.464	2617	2620	2622	rBV3	1201	777	0.03%	0.005%
48	9.535	2639	2642	2645	rBV2	658	580	0.02%	0.003%
49	9.580	2652	2656	2658	rBV3	775	520	0.02%	0.003%
50	9.590	2658	2659	2661	rBV	390	167	0.01%	0.001%
51	9.612	2663	2666	2667	rBV2	476	230	0.01%	0.001%
52	9.664	2681	2682	2683	rBV2	436	138	0.01%	0.001%
53	9.702	2689	2694	2695	rBV3	891	692	0.03%	0.004%
54	9.725	2700	2701	2704	rBV2	430	249	0.01%	0.001%
55	9.754	2708	2710	2711	rBV	505	191	0.01%	0.001%
56	9.802	2722	2725	2727	rVB2	679	338	0.01%	0.002%
57	9.866	2743	2745	2747	rBV	411	211	0.01%	0.001%
58	9.895	2749	2754	2758	rVB5	1443	1542	0.06%	0.009%
59	9.918	2759	2761	2763	rBV2	564	280	0.01%	0.002%
60	9.995	2783	2785	2787	rBV3	504	215	0.01%	0.001%
61	10.011	2788	2790	2792	rVV2	303	96	0.00%	0.001%
62	10.053	2801	2803	2805	rBV	554	198	0.01%	0.001%
63	10.082	2810	2812	2814	rBV	356	195	0.01%	0.001%
64	10.146	2819	2832	2855	rBV	605051	961869	40.54%	5.626%
65	10.361	2895	2899	2901	rBV3	492	442	0.02%	0.003%
66	10.561	2957	2961	2965	rBV3	832	893	0.04%	0.005%
67	10.599	2971	2973	2975	rBV2	621	226	0.01%	0.001%
68	10.654	2988	2990	2992	rVB2	630	247	0.01%	0.001%
69	10.667	2992	2994	2995	rBV	305	119	0.01%	0.001%
70	10.680	2995	2998	3000	rVB2	728	383	0.02%	0.002%
71	10.699	3000	3004	3008	rVB4	728	571	0.02%	0.003%
72	10.728	3008	3013	3014	rVB2	511	359	0.02%	0.002%
73	10.738	3014	3016	3019	rBV2	460	334	0.01%	0.002%
74	10.792	3031	3033	3034	rBV2	679	280	0.01%	0.002%
75	10.850	3049	3051	3054	rBV3	459	193	0.01%	0.001%
76	10.873	3054	3058	3059	rBV4	545	364	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037796.D
Acq On : 10 Oct 2024 11:50
Operator : SY/MD
Sample : P4363-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAY5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	10.898	3064	3066	3068	rBV2	416	239	0.01%	0.001%
78	10.959	3083	3085	3087	rBV2	509	200	0.01%	0.001%
79	11.178	3142	3153	3182	rBV	999620	1607765	67.77%	9.404%
80	11.458	3238	3240	3242	rBV2	976	401	0.02%	0.002%
81	11.554	3258	3270	3301	rBV	1039741	1696809	71.52%	9.925%
82	12.104	3438	3441	3443	rBV4	1135	719	0.03%	0.004%
83	12.220	3475	3477	3479	rBV3	662	260	0.01%	0.002%
84	12.355	3517	3519	3520	rBV	683	234	0.01%	0.001%
85	12.686	3618	3622	3625	rBV2	768	673	0.03%	0.004%
86	16.702	4868	4871	4880	rVB	18018	15076	0.64%	0.088%




Sum of corrected areas: 17097070

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037796.D
Acq On : 10 Oct 2024 11:50
Operator : SY/MD
Sample : P4363-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

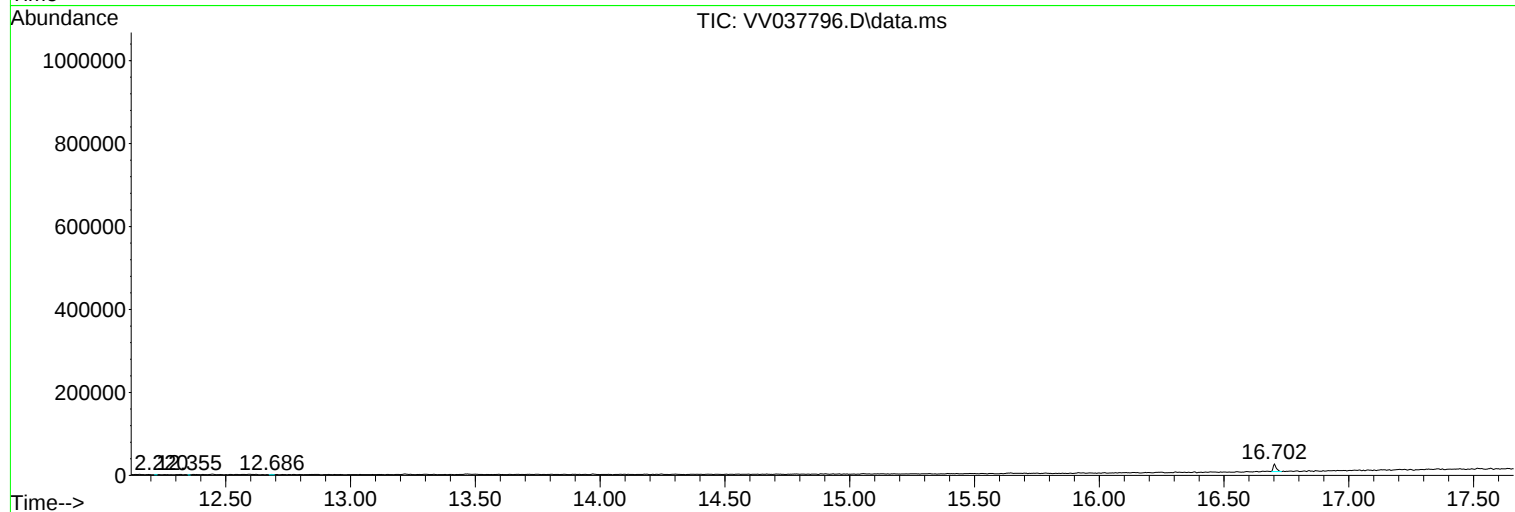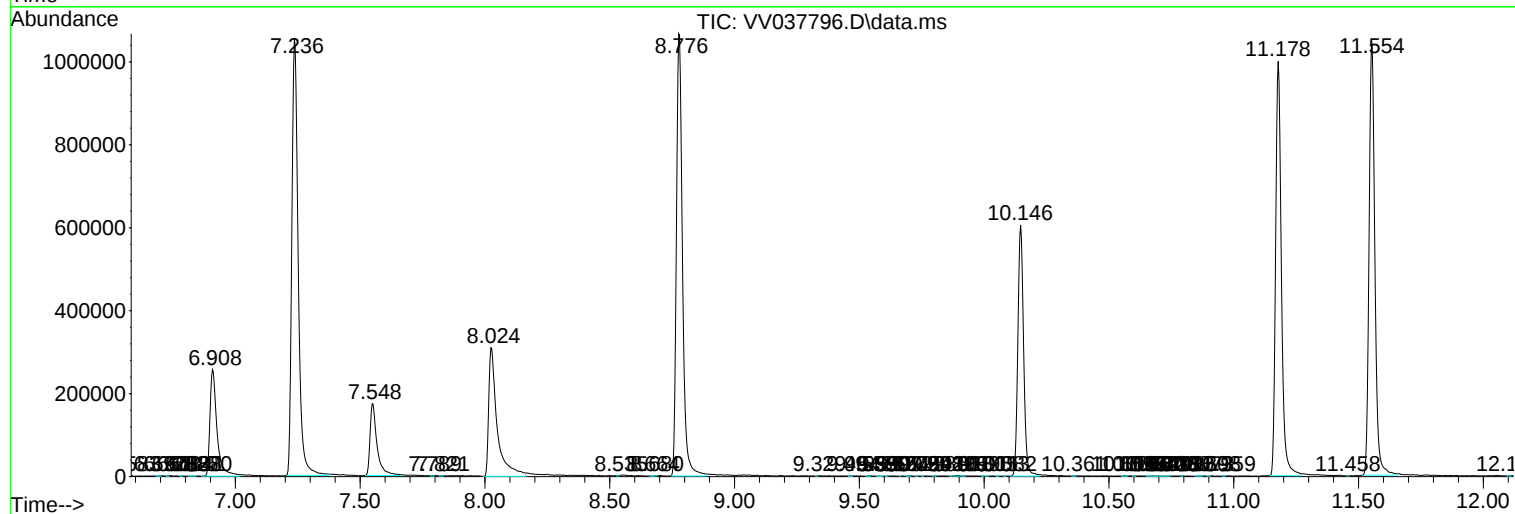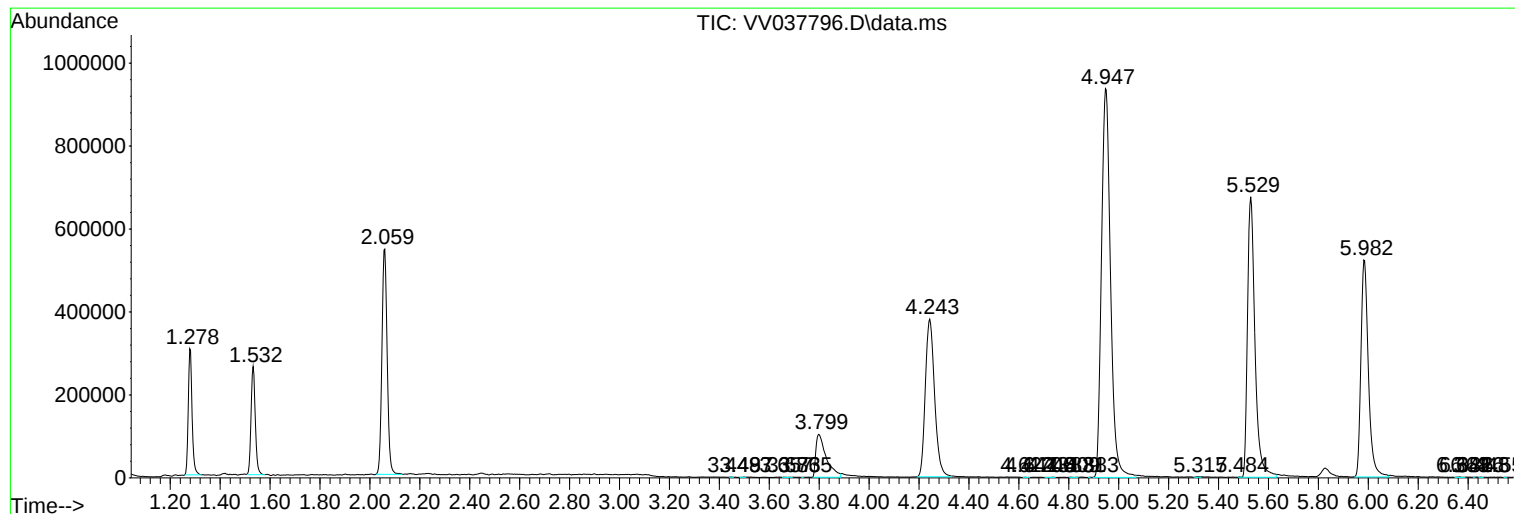

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037796.D
Acq On : 10 Oct 2024 11:50
Operator : SY/MD
Sample : P4363-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037796.D
Acq On : 10 Oct 2024 11:50
Operator : SY/MD
Sample : P4363-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAY5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc