

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037800.D
 Acq On : 10 Oct 2024 13:16
 Operator : SY/MD
 Sample : P4379-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	35	43	45	rBV2	6533	7934	0.37%	0.054%
2	1.281	67	75	89	rBV	268568	289885	13.69%	1.978%
3	1.532	145	153	170	rVB	245322	282695	13.35%	1.929%
4	2.059	307	317	331	rBV	489187	700768	33.10%	4.782%
5	3.567	780	786	789	rBV5	1033	1070	0.05%	0.007%
6	3.616	797	801	804	rBV3	1093	835	0.04%	0.006%
7	3.738	837	839	842	rVB2	725	446	0.02%	0.003%
8	3.802	848	859	889	rBV	90837	266382	12.58%	1.818%
9	4.124	956	959	962	rBV3	632	434	0.02%	0.003%
10	4.185	975	978	979	rBV2	710	420	0.02%	0.003%
11	4.243	979	996	1021	rVV	339936	866715	40.94%	5.914%
12	4.420	1047	1051	1053	rBV3	850	742	0.04%	0.005%
13	4.542	1084	1089	1095	rVB8	905	915	0.04%	0.006%
14	4.577	1095	1100	1103	rVB4	980	734	0.03%	0.005%
15	4.950	1199	1216	1267	rBV2	834740	2116961	100.00%	14.445%
16	5.317	1325	1330	1333	rBV6	848	787	0.04%	0.005%
17	5.426	1360	1364	1367	rBV3	548	549	0.03%	0.004%
18	5.465	1373	1376	1382	rVB4	991	610	0.03%	0.004%
19	5.529	1382	1396	1427	rBV	513340	1082494	51.13%	7.386%
20	5.731	1457	1459	1461	rVV2	1424	586	0.03%	0.004%
21	5.760	1465	1468	1471	rVB4	1007	564	0.03%	0.004%
22	5.828	1480	1489	1504	rBV6	10371	24388	1.15%	0.166%
23	5.985	1525	1538	1567	rBV	462985	967314	45.69%	6.600%
24	6.439	1677	1679	1685	rVB4	897	647	0.03%	0.004%
25	6.490	1690	1695	1697	rBV2	658	479	0.02%	0.003%
26	6.545	1710	1712	1718	rBV5	576	511	0.02%	0.003%
27	6.670	1749	1751	1757	rBV3	435	433	0.02%	0.003%
28	6.741	1770	1773	1775	rBV3	652	444	0.02%	0.003%
29	6.789	1782	1788	1791	rVB5	1093	1066	0.05%	0.007%
30	6.809	1791	1794	1796	rBV3	806	532	0.03%	0.004%
31	6.911	1816	1826	1855	rBV	227200	444321	20.99%	3.032%
32	7.172	1904	1907	1909	rVB3	1046	491	0.02%	0.003%
33	7.236	1913	1927	1956	rBV	904982	1632380	77.11%	11.139%
34	7.551	2015	2025	2056	rBV	152565	299283	14.14%	2.042%
35	7.889	2126	2130	2134	rVB6	1003	882	0.04%	0.006%
36	7.915	2136	2138	2142	rVB4	645	439	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037800.D
 Acq On : 10 Oct 2024 13:16
 Operator : SY/MD
 Sample : P4379-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.937	2143	2145	2150	rVB4	677	493	0.02%	0.003%
38	7.989	2158	2161	2163	rVB3	769	479	0.02%	0.003%
39	8.027	2163	2173	2218	rBV2	279989	647322	30.58%	4.417%
40	8.368	2270	2279	2288	rBV9	3007	5792	0.27%	0.040%
41	8.506	2320	2322	2327	rBV6	525	543	0.03%	0.004%
42	8.554	2334	2337	2340	rVB4	1112	913	0.04%	0.006%
43	8.651	2365	2367	2370	rVB3	950	489	0.02%	0.003%
44	8.683	2374	2377	2379	rVV2	602	428	0.02%	0.003%
45	8.779	2396	2407	2431	rBV	817696	1377174	65.05%	9.397%
46	9.197	2535	2537	2540	rBV2	903	641	0.03%	0.004%
47	9.217	2540	2543	2545	rVV3	990	632	0.03%	0.004%
48	9.255	2553	2555	2557	rVB2	841	459	0.02%	0.003%
49	9.278	2559	2562	2563	rBV3	879	513	0.02%	0.004%
50	9.339	2576	2581	2584	rBV5	1246	1187	0.06%	0.008%
51	9.419	2604	2606	2609	rVB2	1011	500	0.02%	0.003%
52	9.445	2609	2614	2618	rBV5	871	854	0.04%	0.006%
53	9.487	2622	2627	2633	rBV7	1129	1142	0.05%	0.008%
54	9.522	2633	2638	2641	rBV3	725	569	0.03%	0.004%
55	9.689	2686	2690	2694	rBV4	835	696	0.03%	0.005%
56	9.783	2716	2719	2724	rBV4	751	631	0.03%	0.004%
57	9.921	2758	2762	2764	rBV3	560	443	0.02%	0.003%
58	9.969	2774	2777	2782	rBV4	587	661	0.03%	0.005%
59	10.146	2820	2832	2854	rBV	551832	876246	41.39%	5.979%
60	10.381	2903	2905	2908	rVB4	1025	440	0.02%	0.003%
61	10.397	2908	2910	2914	rBV2	793	463	0.02%	0.003%
62	10.416	2914	2916	2919	rBV	779	614	0.03%	0.004%
63	10.551	2955	2958	2959	rBV2	754	447	0.02%	0.003%
64	10.638	2982	2985	2990	rBV5	526	531	0.03%	0.004%
65	10.673	2993	2996	2998	rVB3	948	559	0.03%	0.004%
66	10.995	3091	3096	3098	rBV2	758	700	0.03%	0.005%
67	11.011	3098	3101	3103	rVV5	866	575	0.03%	0.004%
68	11.024	3103	3105	3109	rVB2	707	470	0.02%	0.003%
69	11.053	3109	3114	3119	rBV5	758	798	0.04%	0.005%
70	11.107	3126	3131	3133	rBV3	723	575	0.03%	0.004%
71	11.178	3143	3153	3190	rBV	747206	1234953	58.34%	8.427%
72	11.554	3252	3270	3292	rBV	914107	1478177	69.83%	10.086%
73	11.792	3340	3344	3348	rVV5	1199	929	0.04%	0.006%
74	11.876	3367	3370	3371	rBV	828	503	0.02%	0.003%
75	11.902	3376	3378	3381	rBV5	761	569	0.03%	0.004%
76	11.947	3389	3392	3398	rVB7	1148	1102	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037800.D
 Acq On : 10 Oct 2024 13:16
 Operator : SY/MD
 Sample : P4379-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.992	3402	3406	3410	rBV3	1011	769	0.04%	0.005%
78	12.139	3448	3452	3457	rVV3	925	785	0.04%	0.005%
79	12.184	3465	3466	3470	rVB2	758	490	0.02%	0.003%
80	12.207	3470	3473	3474	rBV2	863	515	0.02%	0.004%
81	12.252	3482	3487	3489	rBV4	751	615	0.03%	0.004%
82	12.365	3518	3522	3530	rVB5	838	964	0.05%	0.007%
83	12.529	3570	3573	3577	rBV2	881	576	0.03%	0.004%
84	12.738	3634	3638	3639	rBV3	855	609	0.03%	0.004%
85	12.840	3665	3670	3672	rBV2	747	693	0.03%	0.005%
86	12.879	3679	3682	3685	rBV4	652	484	0.02%	0.003%
87	12.898	3685	3688	3690	rVV3	763	499	0.02%	0.003%
88	12.992	3713	3717	3719	rBV4	690	555	0.03%	0.004%
89	13.220	3783	3788	3791	rBV3	1596	1327	0.06%	0.009%
90	13.271	3800	3804	3808	rBV4	667	501	0.02%	0.003%
91	13.519	3878	3881	3883	rVB4	986	592	0.03%	0.004%
92	13.754	3950	3954	3958	rBV4	1121	945	0.04%	0.006%
93	13.885	3991	3995	3997	rBV2	997	735	0.03%	0.005%
94	13.982	4021	4025	4030	rBV4	1359	1460	0.07%	0.010%
95	14.255	4108	4110	4114	rVB2	1080	668	0.03%	0.005%
96	14.284	4114	4119	4122	rBV5	942	940	0.04%	0.006%
97	14.336	4130	4135	4136	rBV3	1033	818	0.04%	0.006%
98	14.406	4154	4157	4159	rVB4	1070	595	0.03%	0.004%
99	14.866	4298	4300	4307	rVB6	1030	724	0.03%	0.005%
100	15.033	4350	4352	4357	rBV5	1220	957	0.05%	0.007%




Sum of corrected areas: 14655164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037800.D
Acq On : 10 Oct 2024 13:16
Operator : SY/MD
Sample : P4379-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

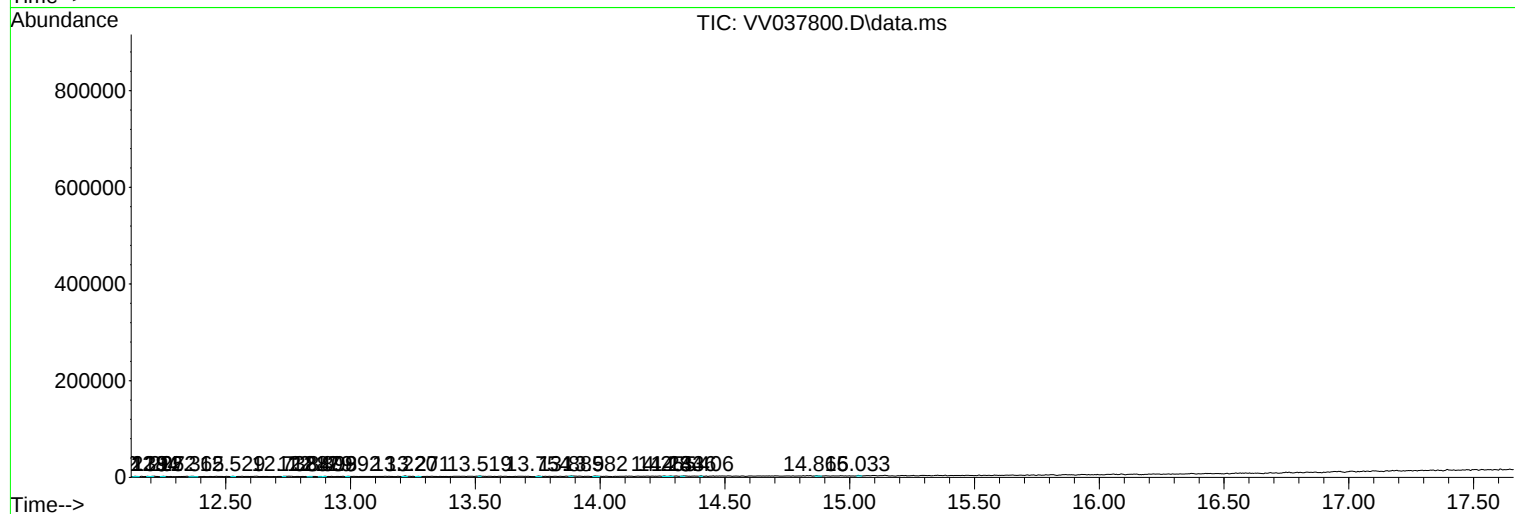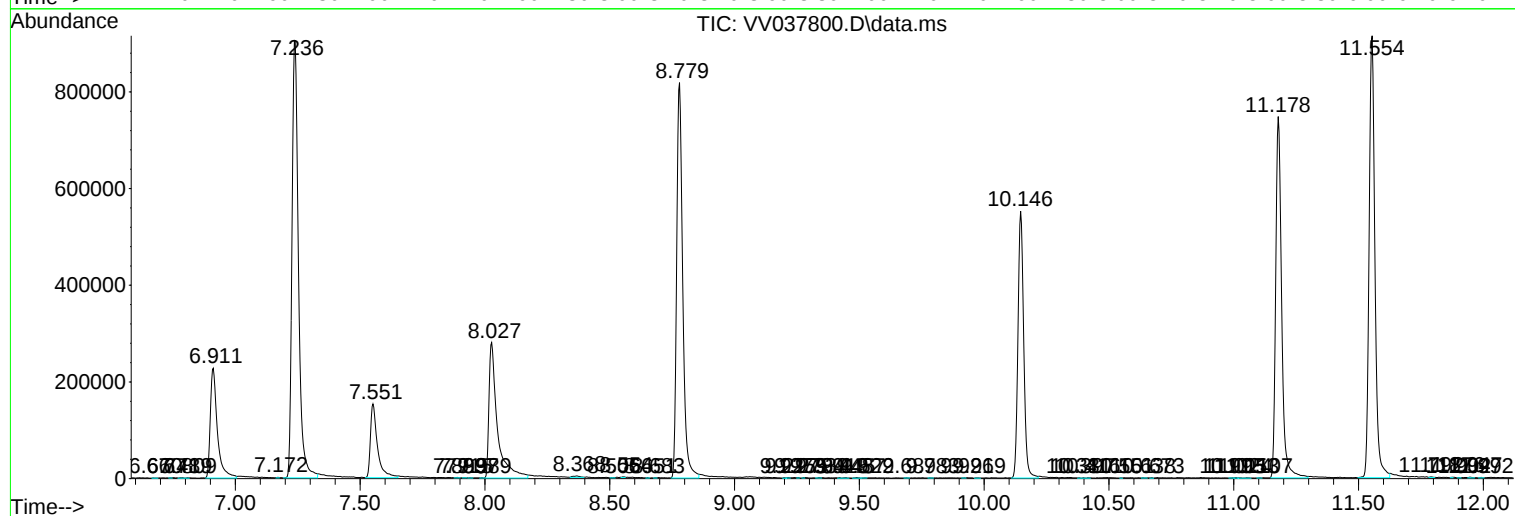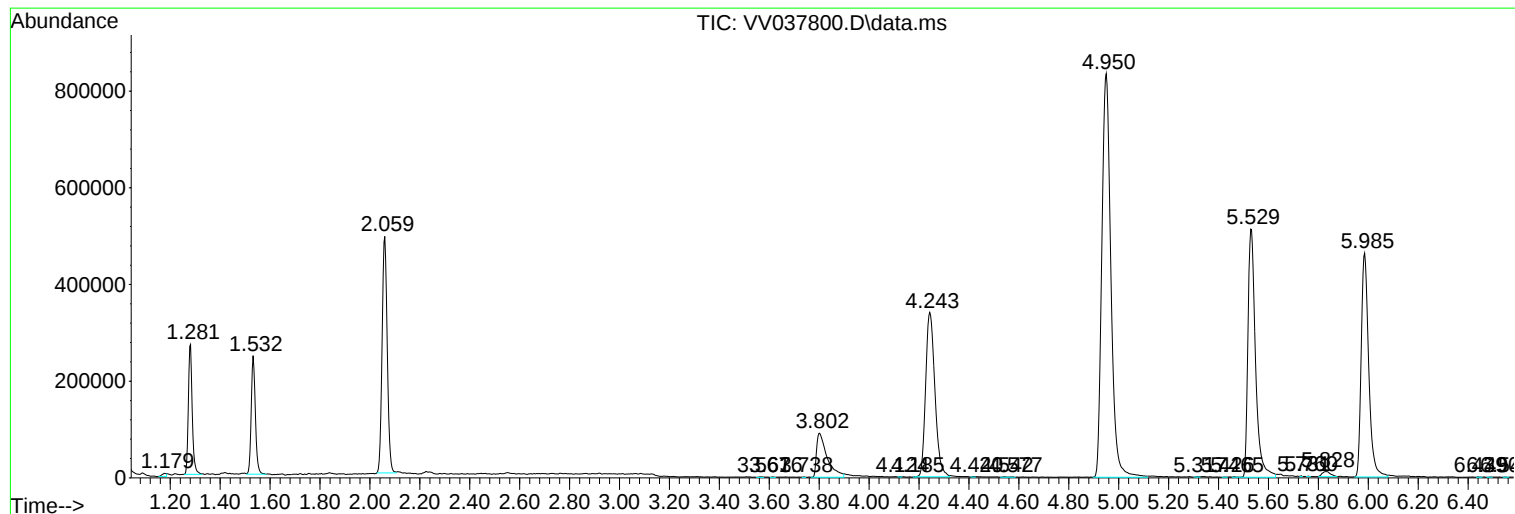

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037800.D
Acq On : 10 Oct 2024 13:16
Operator : SY/MD
Sample : P4379-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037800.D
Acq On : 10 Oct 2024 13:16
Operator : SY/MD
Sample : P4379-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------