

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037801.D
 Acq On : 10 Oct 2024 13:38
 Operator : SY/MD
 Sample : P4379-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037801.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	271333	285862	13.44%	1.934%
2	1.532	146	153	169	rVB	235524	281259	13.22%	1.903%
3	2.060	308	317	331	rVB	488703	697744	32.80%	4.720%
4	3.388	728	730	732	rBV2	554	377	0.02%	0.003%
5	3.478	756	758	761	rBV2	365	238	0.01%	0.002%
6	3.571	785	787	791	rBV2	865	670	0.03%	0.005%
7	3.619	798	802	807	rBV6	695	602	0.03%	0.004%
8	3.728	834	836	838	rBV2	461	196	0.01%	0.001%
9	3.767	845	848	849	rBV	478	233	0.01%	0.002%
10	3.799	850	858	891	rBV	94735	288025	13.54%	1.949%
11	4.243	981	996	1025	rBV2	345327	876065	41.18%	5.927%
12	4.494	1066	1074	1075	rBV2	669	682	0.03%	0.005%
13	4.542	1086	1089	1091	rBV2	659	447	0.02%	0.003%
14	4.674	1126	1130	1132	rBV2	307	283	0.01%	0.002%
15	4.715	1137	1143	1144	rBV2	638	494	0.02%	0.003%
16	4.754	1154	1155	1156	rBV2	506	194	0.01%	0.001%
17	4.789	1162	1166	1168	rBV3	173	126	0.01%	0.001%
18	4.802	1168	1170	1172	rBV2	562	322	0.02%	0.002%
19	4.851	1184	1185	1187	rBV	558	236	0.01%	0.002%
20	4.947	1201	1215	1248	rBV2	848987	2127546	100.00%	14.394%
21	5.410	1357	1359	1361	rVB3	695	290	0.01%	0.002%
22	5.529	1385	1396	1430	rBV	526654	1112782	52.30%	7.528%
23	5.986	1526	1538	1577	rBV	470248	972201	45.70%	6.577%
24	6.352	1650	1652	1653	rBV2	591	207	0.01%	0.001%
25	6.365	1653	1656	1659	rVV2	475	300	0.01%	0.002%
26	6.445	1678	1681	1683	rBV4	1184	608	0.03%	0.004%
27	6.471	1687	1689	1691	rBV2	395	162	0.01%	0.001%
28	6.481	1691	1692	1694	rBV	506	260	0.01%	0.002%
29	6.510	1699	1701	1703	rBV2	738	306	0.01%	0.002%
30	6.529	1704	1707	1711	rBV4	573	447	0.02%	0.003%
31	6.613	1731	1733	1735	rBV2	275	188	0.01%	0.001%
32	6.625	1735	1737	1742	rVB4	517	274	0.01%	0.002%
33	6.670	1747	1751	1752	rBV2	868	498	0.02%	0.003%
34	6.693	1756	1758	1761	rBV3	874	458	0.02%	0.003%
35	6.722	1763	1767	1769	rBV2	761	507	0.02%	0.003%
36	6.738	1769	1772	1773	rBV3	486	231	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037801.D
 Acq On : 10 Oct 2024 13:38
 Operator : SY/MD
 Sample : P4379-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.776	1782	1784	1785	rBV	639	238	0.01%	0.002%
38	6.818	1793	1797	1799	rBV3	741	375	0.02%	0.003%
39	6.850	1803	1807	1809	rBV2	728	477	0.02%	0.003%
40	6.908	1815	1825	1862	rBV	226066	454597	21.37%	3.075%
41	7.236	1917	1927	1962	rBV	920943	1657474	77.91%	11.213%
42	7.551	2016	2025	2047	rBV2	158627	295705	13.90%	2.001%
43	7.799	2100	2102	2104	rBV2	710	264	0.01%	0.002%
44	8.024	2164	2172	2215	rBV2	275781	638281	30.00%	4.318%
45	8.600	2350	2351	2356	rVB3	1118	388	0.02%	0.003%
46	8.645	2362	2365	2370	rVB5	1035	795	0.04%	0.005%
47	8.686	2375	2378	2383	rBV4	576	566	0.03%	0.004%
48	8.722	2387	2389	2392	rVB3	503	258	0.01%	0.002%
49	8.780	2392	2407	2442	rBV	834553	1420565	66.77%	9.611%
50	9.175	2527	2530	2533	rBV5	837	572	0.03%	0.004%
51	9.236	2546	2549	2551	rBV3	701	351	0.02%	0.002%
52	9.272	2557	2560	2561	rBV2	515	262	0.01%	0.002%
53	9.323	2573	2576	2577	rBV2	718	448	0.02%	0.003%
54	9.413	2602	2604	2607	rBV3	587	260	0.01%	0.002%
55	9.448	2612	2615	2618	rBV3	798	488	0.02%	0.003%
56	9.535	2641	2642	2643	rBV	462	138	0.01%	0.001%
57	9.545	2643	2645	2652	rVB6	735	525	0.02%	0.004%
58	9.574	2652	2654	2657	rBV	228	107	0.01%	0.001%
59	9.593	2657	2660	2662	rBV3	662	452	0.02%	0.003%
60	9.664	2680	2682	2685	rVB2	528	232	0.01%	0.002%
61	9.735	2699	2704	2709	rVB2	1163	1045	0.05%	0.007%
62	9.764	2709	2713	2716	rBV2	678	475	0.02%	0.003%
63	9.831	2732	2734	2737	rVB3	684	251	0.01%	0.002%
64	9.882	2748	2750	2752	rBV	484	230	0.01%	0.002%
65	9.911	2757	2759	2763	rVB2	787	420	0.02%	0.003%
66	9.931	2763	2765	2769	rVB2	892	460	0.02%	0.003%
67	9.947	2769	2770	2772	rBV2	269	112	0.01%	0.001%
68	9.973	2772	2778	2779	rBV3	567	481	0.02%	0.003%
69	10.018	2790	2792	2793	rBV2	578	221	0.01%	0.001%
70	10.053	2801	2803	2805	rBV2	342	124	0.01%	0.001%
71	10.079	2808	2811	2813	rBV2	356	249	0.01%	0.002%
72	10.104	2816	2819	2820	rBV3	524	260	0.01%	0.002%
73	10.146	2821	2832	2854	rBV	565757	891928	41.92%	6.034%
74	10.387	2901	2907	2912	rBV5	767	1198	0.06%	0.008%
75	10.464	2924	2931	2934	rBV4	710	853	0.04%	0.006%
76	10.519	2945	2948	2950	rBV3	720	426	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037801.D
 Acq On : 10 Oct 2024 13:38
 Operator : SY/MD
 Sample : P4379-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.561	2953	2961	2964	rVB5	831	1095	0.05%	0.007%
78	10.583	2964	2968	2975	rVB4	629	606	0.03%	0.004%
79	10.619	2975	2979	2984	rBV3	699	669	0.03%	0.005%
80	10.654	2984	2990	2991	rBV2	443	359	0.02%	0.002%
81	10.709	3004	3007	3009	rBV3	483	351	0.02%	0.002%
82	10.744	3013	3018	3020	rBV2	663	512	0.02%	0.003%
83	10.786	3029	3031	3032	rBV2	322	120	0.01%	0.001%
84	10.821	3040	3042	3044	rBV2	639	359	0.02%	0.002%
85	10.837	3044	3047	3050	rVV3	508	338	0.02%	0.002%
86	10.854	3050	3052	3054	rBV2	894	435	0.02%	0.003%
87	10.879	3059	3060	3064	rVB3	528	251	0.01%	0.002%
88	10.899	3064	3066	3068	rBV2	409	191	0.01%	0.001%
89	10.934	3073	3077	3080	rBV3	937	956	0.04%	0.006%
90	11.011	3096	3101	3104	rBV3	838	796	0.04%	0.005%
91	11.059	3110	3116	3120	rBV4	749	859	0.04%	0.006%
92	11.085	3122	3124	3127	rBV	363	232	0.01%	0.002%
93	11.136	3138	3140	3141	rBV2	817	296	0.01%	0.002%
94	11.178	3143	3153	3177	rBV	770011	1247306	58.63%	8.438%
95	11.554	3258	3270	3299	rBV	919671	1499019	70.46%	10.141%
96	11.924	3381	3385	3386	rVB2	637	394	0.02%	0.003%
97	12.050	3422	3424	3430	rBV4	929	765	0.04%	0.005%
98	12.275	3490	3494	3496	rBV2	973	902	0.04%	0.006%
99	12.548	3577	3579	3580	rBV	626	238	0.01%	0.002%
100	13.400	3841	3844	3846	rBV3	557	351	0.02%	0.002%




Sum of corrected areas: 14781271

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037801.D
Acq On : 10 Oct 2024 13:38
Operator : SY/MD
Sample : P4379-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

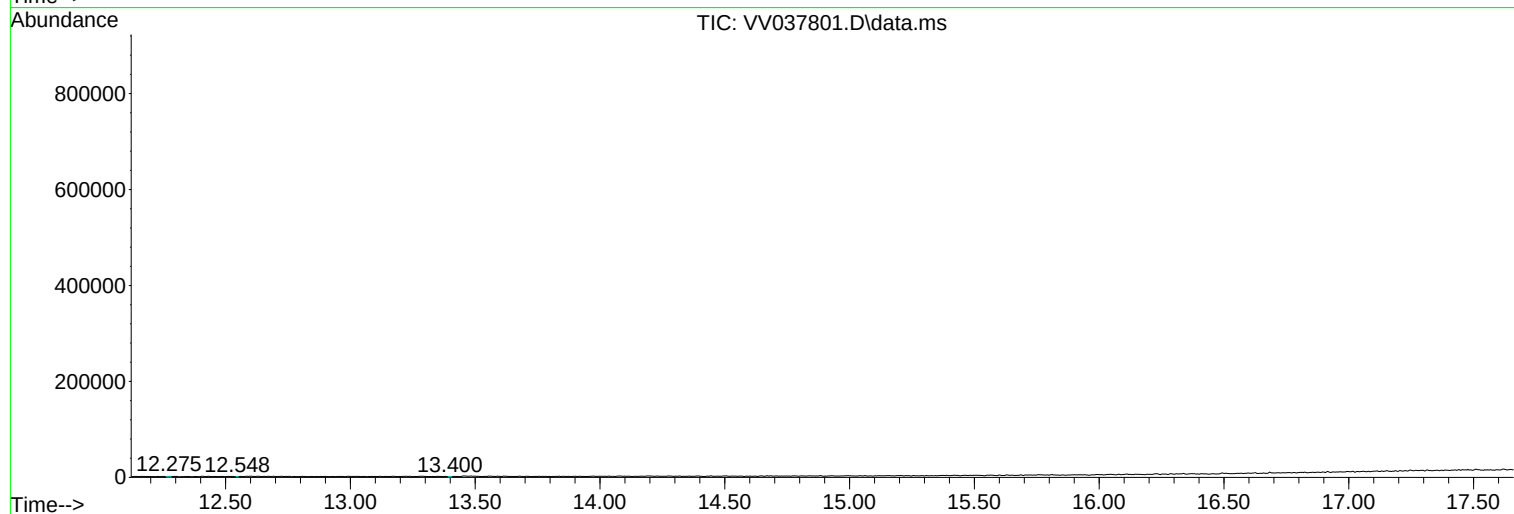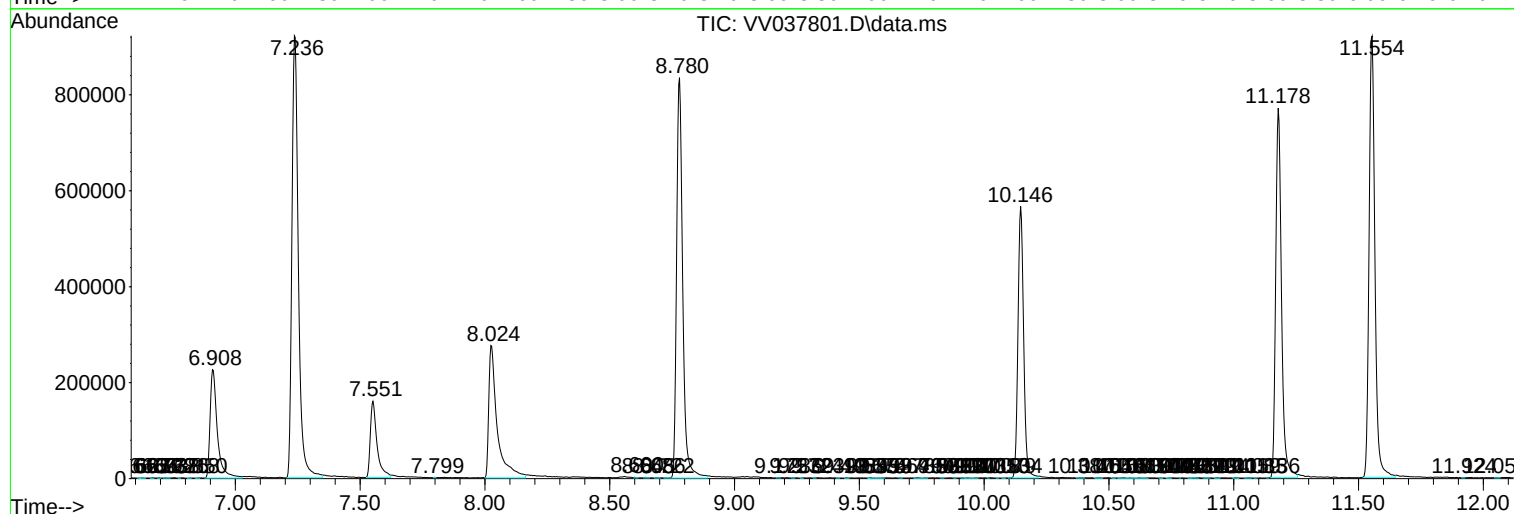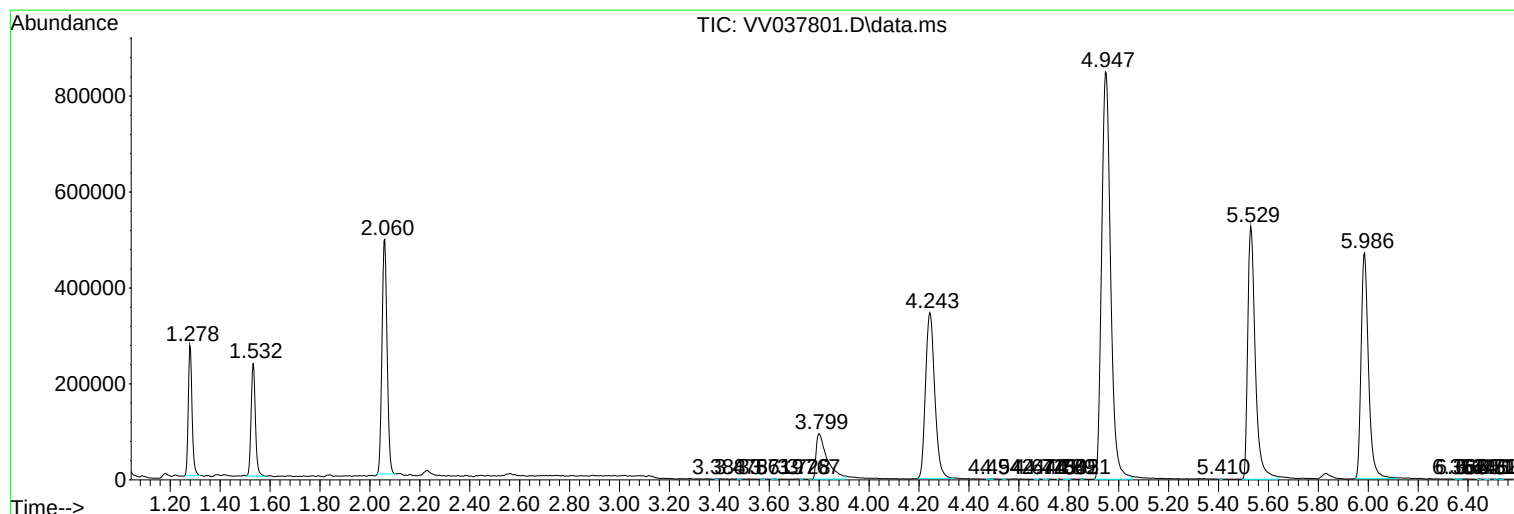

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037801.D
Acq On : 10 Oct 2024 13:38
Operator : SY/MD
Sample : P4379-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037801.D
Acq On : 10 Oct 2024 13:38
Operator : SY/MD
Sample : P4379-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc