

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037802.D
 Acq On : 10 Oct 2024 13:59
 Operator : SY/MD
 Sample : P4379-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	52	rBV	8543	14783	0.72%	0.099%
2	1.281	67	75	88	rBV	264472	282029	13.74%	1.883%
3	1.532	145	153	165	rVB	230309	270462	13.17%	1.806%
4	2.060	307	317	332	rBV	479747	688277	33.52%	4.596%
5	3.375	722	726	730	rBV4	637	445	0.02%	0.003%
6	3.468	753	755	759	rBV2	457	409	0.02%	0.003%
7	3.690	821	824	829	rBV3	768	750	0.04%	0.005%
8	3.799	850	858	894	rBV	86674	268509	13.08%	1.793%
9	4.018	924	926	929	rBV3	1007	572	0.03%	0.004%
10	4.243	979	996	1028	rBV2	337347	861878	41.97%	5.755%
11	4.526	1078	1084	1087	rBV4	884	1003	0.05%	0.007%
12	4.616	1109	1112	1116	rVB3	634	440	0.02%	0.003%
13	4.722	1142	1145	1150	rVB2	872	554	0.03%	0.004%
14	4.757	1153	1156	1159	rBV3	696	492	0.02%	0.003%
15	4.821	1172	1176	1179	rBV3	914	502	0.02%	0.003%
16	4.857	1184	1187	1190	rBV4	1060	836	0.04%	0.006%
17	4.950	1200	1216	1244	rBV2	816291	2053349	100.00%	13.711%
18	5.256	1307	1311	1315	rBV5	1411	1247	0.06%	0.008%
19	5.375	1346	1348	1350	rBV2	784	410	0.02%	0.003%
20	5.529	1385	1396	1430	rBV	604358	1271553	61.93%	8.490%
21	5.831	1482	1490	1501	rVB8	9734	18048	0.88%	0.121%
22	5.985	1525	1538	1565	rBV	452965	943529	45.95%	6.300%
23	6.339	1644	1648	1654	rVB5	938	915	0.04%	0.006%
24	6.410	1666	1670	1673	rBV4	951	894	0.04%	0.006%
25	6.436	1675	1678	1682	rVB5	874	642	0.03%	0.004%
26	6.458	1682	1685	1686	rBV3	772	408	0.02%	0.003%
27	6.493	1693	1696	1699	rVB3	801	605	0.03%	0.004%
28	6.567	1716	1719	1723	rVB	706	454	0.02%	0.003%
29	6.593	1724	1727	1733	rVB6	889	789	0.04%	0.005%
30	6.648	1738	1744	1746	rBV5	1122	1100	0.05%	0.007%
31	6.796	1786	1790	1793	rVB4	806	538	0.03%	0.004%
32	6.908	1815	1825	1862	rBV	217625	437626	21.31%	2.922%
33	7.236	1916	1927	1957	rBV	881533	1589051	77.39%	10.610%
34	7.551	2016	2025	2053	rBV	151037	290906	14.17%	1.942%
35	7.751	2084	2087	2088	rBV3	622	399	0.02%	0.003%
36	8.027	2164	2173	2203	rBV2	254977	572541	27.88%	3.823%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037802.D
 Acq On : 10 Oct 2024 13:59
 Operator : SY/MD
 Sample : P4379-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.458	2305	2307	2310	rVB3	1004	496	0.02%	0.003%
38	8.542	2328	2333	2335	rBV5	1728	1660	0.08%	0.011%
39	8.554	2335	2337	2342	rVB2	1669	1308	0.06%	0.009%
40	8.635	2358	2362	2363	rBV4	683	462	0.02%	0.003%
41	8.780	2396	2407	2437	rBV	968407	1621961	78.99%	10.830%
42	8.995	2472	2474	2476	rBV2	1086	655	0.03%	0.004%
43	9.233	2546	2548	2554	rVB4	1156	680	0.03%	0.005%
44	9.275	2559	2561	2566	rVV3	811	520	0.03%	0.003%
45	9.374	2587	2592	2594	rBV4	665	465	0.02%	0.003%
46	9.432	2608	2610	2613	rVB2	835	436	0.02%	0.003%
47	9.448	2613	2615	2618	rBV4	822	575	0.03%	0.004%
48	9.490	2624	2628	2629	rBV	612	423	0.02%	0.003%
49	9.506	2631	2633	2639	rVB5	806	794	0.04%	0.005%
50	9.641	2672	2675	2678	rBV3	705	563	0.03%	0.004%
51	9.722	2698	2700	2704	rVB3	722	418	0.02%	0.003%
52	9.751	2704	2709	2711	rBV2	910	808	0.04%	0.005%
53	9.873	2744	2747	2749	rBV3	619	474	0.02%	0.003%
54	9.908	2756	2758	2762	rVB4	963	597	0.03%	0.004%
55	9.931	2762	2765	2768	rBV3	654	412	0.02%	0.003%
56	10.146	2819	2832	2859	rBV	537789	856639	41.72%	5.720%
57	10.284	2871	2875	2877	rBV2	967	647	0.03%	0.004%
58	10.471	2929	2933	2934	rBV2	506	401	0.02%	0.003%
59	10.503	2940	2943	2950	rVB5	584	618	0.03%	0.004%
60	10.567	2960	2963	2965	rBV2	873	449	0.02%	0.003%
61	10.786	3027	3031	3034	rVV4	712	618	0.03%	0.004%
62	10.921	3070	3073	3076	rBV2	465	402	0.02%	0.003%
63	11.178	3142	3153	3180	rBV	883781	1424234	69.36%	9.510%
64	11.474	3243	3245	3248	rBV2	1160	615	0.03%	0.004%
65	11.554	3257	3270	3306	rBV	901567	1457732	70.99%	9.733%
66	11.744	3327	3329	3333	rVB4	1097	568	0.03%	0.004%
67	11.763	3333	3335	3340	rBV4	944	885	0.04%	0.006%
68	11.837	3356	3358	3362	rVB4	1181	690	0.03%	0.005%
69	11.869	3366	3368	3371	rVB3	1020	527	0.03%	0.004%
70	12.011	3406	3412	3417	rBV5	1048	978	0.05%	0.007%
71	12.130	3447	3449	3454	rVB5	916	609	0.03%	0.004%
72	12.294	3498	3500	3505	rVB5	615	458	0.02%	0.003%
73	12.365	3520	3522	3526	rBV3	679	661	0.03%	0.004%
74	12.490	3558	3561	3564	rBV2	753	598	0.03%	0.004%
75	12.596	3592	3594	3600	rVB4	1063	823	0.04%	0.005%
76	12.635	3601	3606	3611	rBV5	933	1113	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037802.D
 Acq On : 10 Oct 2024 13:59
 Operator : SY/MD
 Sample : P4379-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL93

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.664	3611	3615	3618	rVV3	764	573	0.03%	0.004%
78	12.721	3631	3633	3637	rVB3	794	416	0.02%	0.003%
79	12.947	3700	3703	3708	rVB3	849	717	0.03%	0.005%
80	12.982	3710	3714	3717	rBV3	892	614	0.03%	0.004%
81	13.049	3730	3735	3737	rBV2	537	424	0.02%	0.003%
82	13.088	3744	3747	3752	rVV5	615	600	0.03%	0.004%
83	13.226	3786	3790	3795	rVB6	1468	1275	0.06%	0.009%
84	13.400	3841	3844	3846	rBV2	748	426	0.02%	0.003%
85	13.416	3846	3849	3853	rVV4	701	520	0.03%	0.003%
86	13.461	3860	3863	3867	rBV4	739	513	0.02%	0.003%
87	13.557	3891	3893	3900	rVB3	925	818	0.04%	0.005%
88	13.602	3901	3907	3909	rBV3	538	601	0.03%	0.004%
89	13.654	3920	3923	3927	rBV3	740	558	0.03%	0.004%
90	13.676	3927	3930	3933	rVV4	1108	631	0.03%	0.004%
91	13.693	3933	3935	3939	rVB2	1053	577	0.03%	0.004%
92	13.873	3987	3991	3992	rBV3	692	488	0.02%	0.003%
93	13.921	4002	4006	4009	rBV4	1080	670	0.03%	0.004%
94	13.995	4026	4029	4034	rBV4	853	913	0.04%	0.006%
95	14.287	4117	4120	4124	rBV4	933	530	0.03%	0.004%
96	14.435	4164	4166	4171	rVB4	992	756	0.04%	0.005%
97	14.802	4276	4280	4283	rBV4	783	869	0.04%	0.006%
98	14.969	4329	4332	4333	rBV3	975	529	0.03%	0.004%
99	15.188	4397	4400	4403	rBV5	1274	874	0.04%	0.006%
100	15.754	4574	4576	4578	rVB2	1613	661	0.03%	0.004%




Sum of corrected areas: 14976470

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037802.D
Acq On : 10 Oct 2024 13:59
Operator : SY/MD
Sample : P4379-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

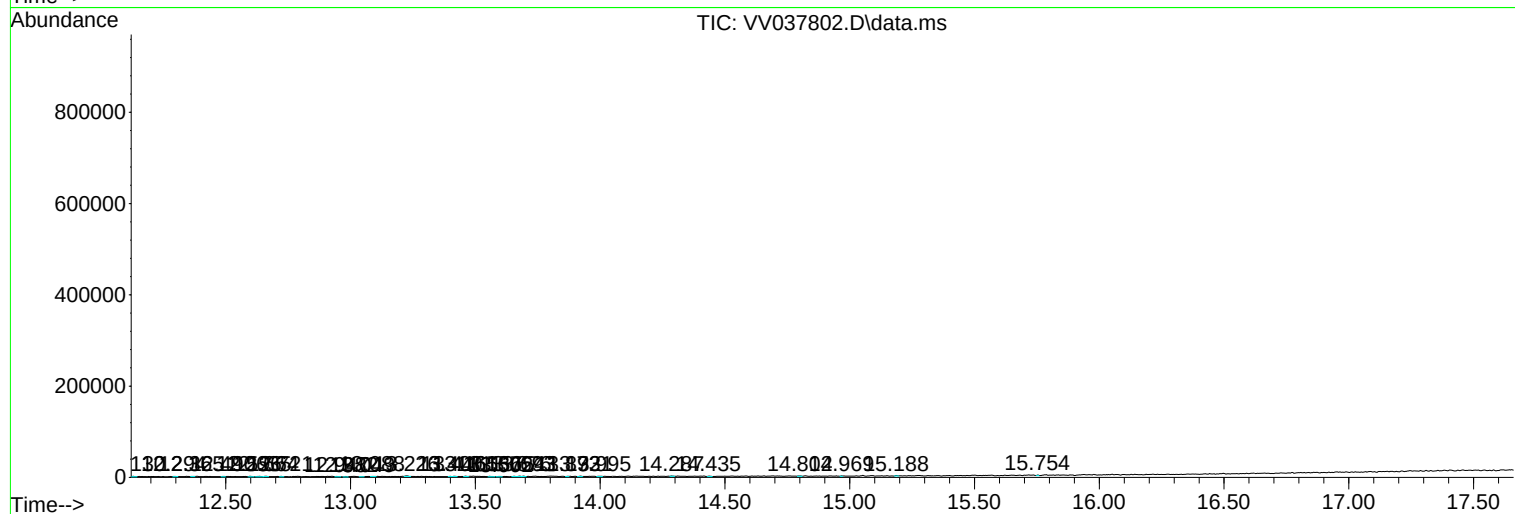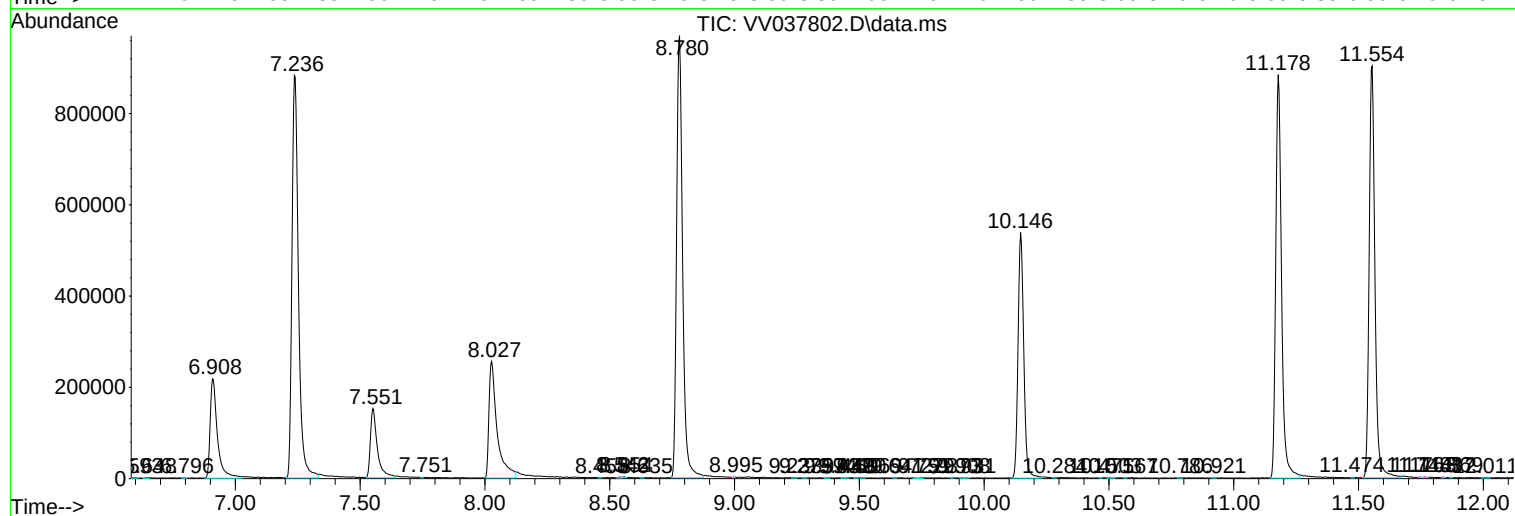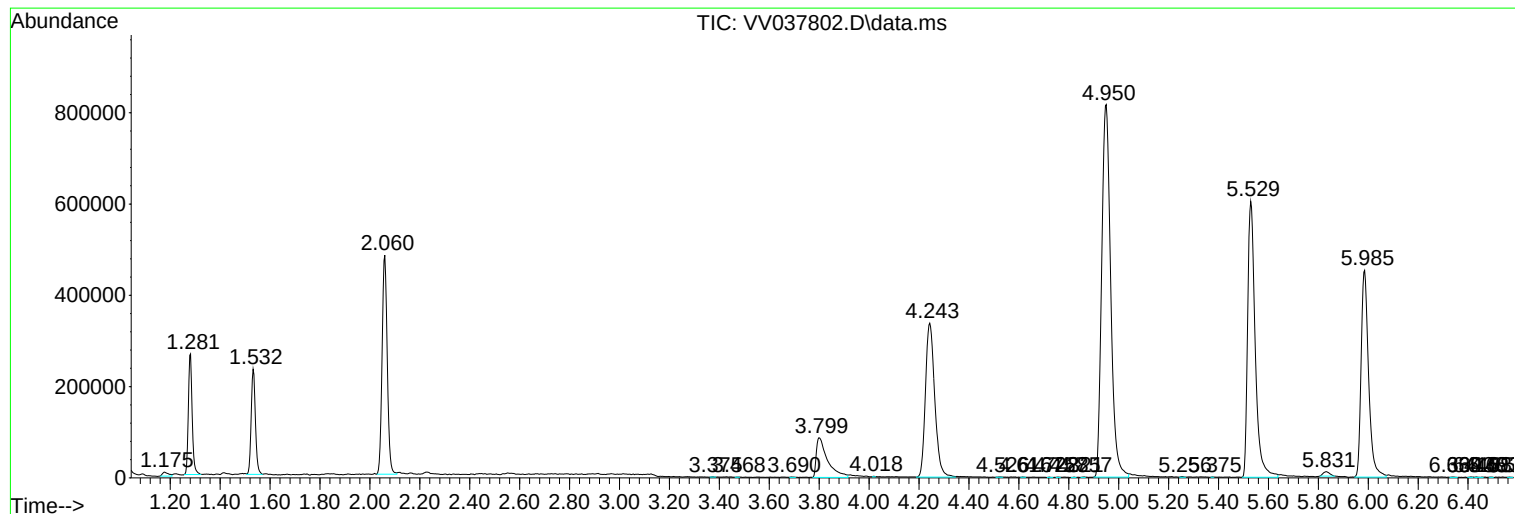

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037802.D
Acq On : 10 Oct 2024 13:59
Operator : SY/MD
Sample : P4379-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037802.D
Acq On : 10 Oct 2024 13:59
Operator : SY/MD
Sample : P4379-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------