

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037803.D
 Acq On : 10 Oct 2024 14:21
 Operator : SY/MD
 Sample : P4379-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	36	44	51	rBV2	13003	24348	1.05%	0.146%
2	1.278	68	74	86	rBV	304713	309067	13.30%	1.851%
3	1.532	145	153	170	rVB	254548	303302	13.05%	1.817%
4	2.060	307	317	332	rBV	533979	768067	33.05%	4.600%
5	3.272	691	694	698	rBV3	1143	928	0.04%	0.006%
6	3.301	698	703	708	rVV5	949	1129	0.05%	0.007%
7	3.326	708	711	715	rVV3	870	642	0.03%	0.004%
8	3.349	715	718	720	rVV3	926	637	0.03%	0.004%
9	3.490	759	762	768	rBV5	545	464	0.02%	0.003%
10	3.548	776	780	783	rBV3	830	557	0.02%	0.003%
11	3.584	787	791	793	rBV3	693	426	0.02%	0.003%
12	3.661	808	815	819	rBV5	840	965	0.04%	0.006%
13	3.799	849	858	890	rBV	101372	291679	12.55%	1.747%
14	4.101	948	952	955	rBV	1043	682	0.03%	0.004%
15	4.143	961	965	967	rVB4	653	466	0.02%	0.003%
16	4.169	967	973	975	rBV5	907	760	0.03%	0.005%
17	4.243	978	996	1029	rBV	381681	968397	41.67%	5.800%
18	4.442	1055	1058	1061	rBV3	664	503	0.02%	0.003%
19	4.780	1158	1163	1165	rBV2	843	641	0.03%	0.004%
20	4.863	1185	1189	1193	rBV3	1062	737	0.03%	0.004%
21	4.947	1200	1215	1251	rBV2	919371	2323764	100.00%	13.918%
22	5.252	1308	1310	1314	rVB4	725	499	0.02%	0.003%
23	5.281	1314	1319	1327	rBV7	1148	1294	0.06%	0.008%
24	5.378	1345	1349	1351	rVV5	723	496	0.02%	0.003%
25	5.420	1357	1362	1363	rBV4	497	456	0.02%	0.003%
26	5.477	1378	1380	1385	rVB4	741	480	0.02%	0.003%
27	5.529	1385	1396	1427	rBV	647602	1349882	58.09%	8.085%
28	5.831	1481	1490	1499	rBV6	9188	17742	0.76%	0.106%
29	5.905	1511	1513	1518	rVB6	813	532	0.02%	0.003%
30	5.982	1524	1537	1571	rBV	513718	1081544	46.54%	6.478%
31	6.265	1622	1625	1631	rVB4	1170	1141	0.05%	0.007%
32	6.297	1631	1635	1637	rBV3	685	636	0.03%	0.004%
33	6.326	1642	1644	1648	rVB3	1084	769	0.03%	0.005%
34	6.394	1662	1665	1667	rBV3	856	538	0.02%	0.003%
35	6.452	1680	1683	1689	rVB3	787	610	0.03%	0.004%
36	6.487	1689	1694	1696	rBV3	541	499	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037803.D
 Acq On : 10 Oct 2024 14:21
 Operator : SY/MD
 Sample : P4379-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.706	1758	1762	1768	rBV5	648	587	0.03%	0.004%
38	6.744	1772	1774	1781	rVB6	997	764	0.03%	0.005%
39	6.847	1801	1806	1808	rBV4	537	466	0.02%	0.003%
40	6.908	1813	1825	1860	rBV	252520	500419	21.53%	2.997%
41	7.236	1916	1927	1957	rBV	1033195	1835854	79.00%	10.996%
42	7.548	2015	2024	2044	rBV	170730	320341	13.79%	1.919%
43	7.934	2140	2144	2148	rBV4	687	509	0.02%	0.003%
44	7.973	2151	2156	2161	rVB5	947	686	0.03%	0.004%
45	8.024	2164	2172	2207	rBV2	301447	674520	29.03%	4.040%
46	8.259	2243	2245	2249	rVB2	1343	733	0.03%	0.004%
47	8.439	2297	2301	2305	rBV6	820	800	0.03%	0.005%
48	8.503	2318	2321	2326	rBV5	1284	975	0.04%	0.006%
49	8.632	2356	2361	2366	rVB5	922	851	0.04%	0.005%
50	8.677	2371	2375	2376	rBV3	763	527	0.02%	0.003%
51	8.780	2396	2407	2440	rBV	1034060	1724586	74.22%	10.329%
52	9.046	2488	2490	2494	rVB5	1390	695	0.03%	0.004%
53	9.288	2561	2565	2567	rBV4	801	517	0.02%	0.003%
54	9.355	2583	2586	2588	rBV4	591	430	0.02%	0.003%
55	9.423	2604	2607	2612	rBV3	1140	947	0.04%	0.006%
56	9.474	2619	2623	2625	rBV2	681	490	0.02%	0.003%
57	9.596	2657	2661	2664	rBV4	596	453	0.02%	0.003%
58	9.683	2686	2688	2694	rBV3	631	427	0.02%	0.003%
59	9.715	2694	2698	2702	rVB3	634	558	0.02%	0.003%
60	9.754	2705	2710	2714	rBV5	596	535	0.02%	0.003%
61	9.924	2760	2763	2768	rVB4	1186	951	0.04%	0.006%
62	9.972	2771	2778	2779	rBV5	441	446	0.02%	0.003%
63	10.146	2820	2832	2855	rBV	617865	976507	42.02%	5.849%
64	10.352	2894	2896	2902	rVB4	613	460	0.02%	0.003%
65	10.390	2905	2908	2911	rBV4	688	462	0.02%	0.003%
66	10.413	2911	2915	2917	rBV3	782	686	0.03%	0.004%
67	10.468	2927	2932	2937	rBV4	471	622	0.03%	0.004%
68	10.538	2948	2954	2957	rBV3	697	698	0.03%	0.004%
69	10.619	2977	2979	2985	rVB2	600	470	0.02%	0.003%
70	10.706	3003	3006	3010	rBV3	630	476	0.02%	0.003%
71	10.789	3027	3032	3039	rBV8	1186	1621	0.07%	0.010%
72	10.824	3040	3043	3046	rVB2	824	492	0.02%	0.003%
73	10.850	3046	3051	3052	rBV2	571	566	0.02%	0.003%
74	10.995	3094	3096	3102	rVV3	415	497	0.02%	0.003%
75	11.178	3142	3153	3186	rBV	929544	1512512	65.09%	9.059%
76	11.551	3257	3269	3298	rBV	1012257	1656603	71.29%	9.922%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037803.D
 Acq On : 10 Oct 2024 14:21
 Operator : SY/MD
 Sample : P4379-04
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.818	3349	3352	3354	rBV3	1058	715	0.03%	0.004%
78	11.857	3363	3364	3367	rVB3	1320	589	0.03%	0.004%
79	11.898	3374	3377	3381	rBV3	726	607	0.03%	0.004%
80	11.927	3384	3386	3390	rVV4	1082	785	0.03%	0.005%
81	12.085	3432	3435	3437	rBV2	649	456	0.02%	0.003%
82	12.175	3457	3463	3467	rVB5	1027	1127	0.05%	0.007%
83	12.204	3467	3472	3474	rBV2	744	602	0.03%	0.004%
84	12.236	3478	3482	3484	rBV2	1044	669	0.03%	0.004%
85	12.603	3590	3596	3600	rBV4	1147	1470	0.06%	0.009%
86	12.638	3604	3607	3611	rVB3	646	539	0.02%	0.003%
87	12.660	3611	3614	3618	rBV2	813	788	0.03%	0.005%
88	12.918	3690	3694	3697	rBV4	814	849	0.04%	0.005%
89	12.998	3716	3719	3724	rBV3	669	502	0.02%	0.003%
90	13.046	3731	3734	3737	rBV3	639	512	0.02%	0.003%
91	13.323	3816	3820	3823	rBV4	691	534	0.02%	0.003%
92	13.471	3859	3866	3870	rBV5	1200	1346	0.06%	0.008%
93	13.667	3923	3927	3929	rBV3	939	686	0.03%	0.004%
94	13.831	3975	3978	3983	rVB4	1015	1027	0.04%	0.006%
95	13.937	4008	4011	4016	rBV6	923	817	0.04%	0.005%
96	13.979	4021	4024	4028	rBV4	975	752	0.03%	0.005%
97	14.094	4057	4060	4063	rVV3	625	441	0.02%	0.003%
98	15.014	4343	4346	4350	rBV2	1159	892	0.04%	0.005%
99	15.181	4393	4398	4399	rBV4	1536	1295	0.06%	0.008%
100	15.442	4477	4479	4482	rBV2	1117	819	0.04%	0.005%




Sum of corrected areas: 16695837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037803.D
Acq On : 10 Oct 2024 14:21
Operator : SY/MD
Sample : P4379-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

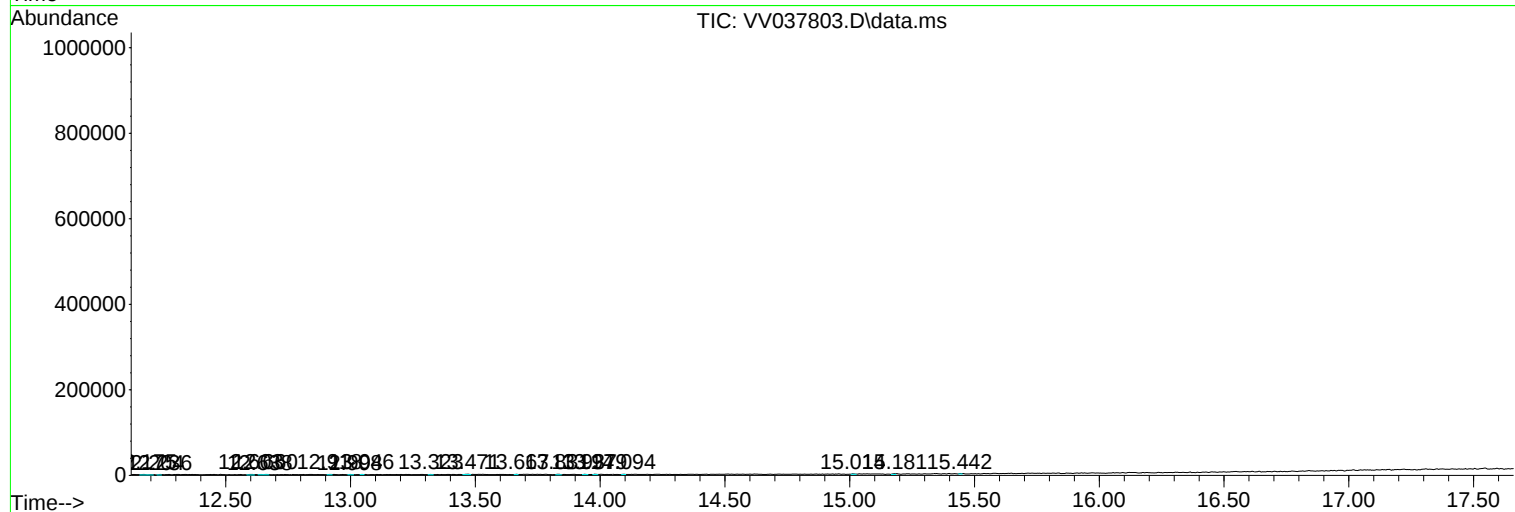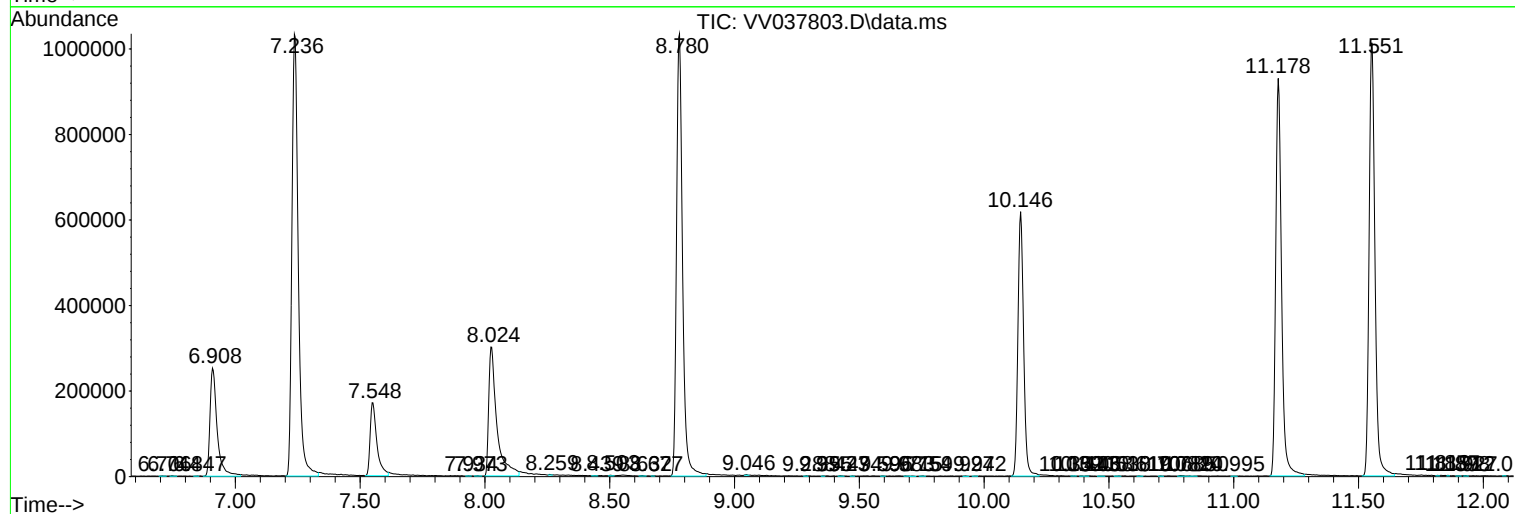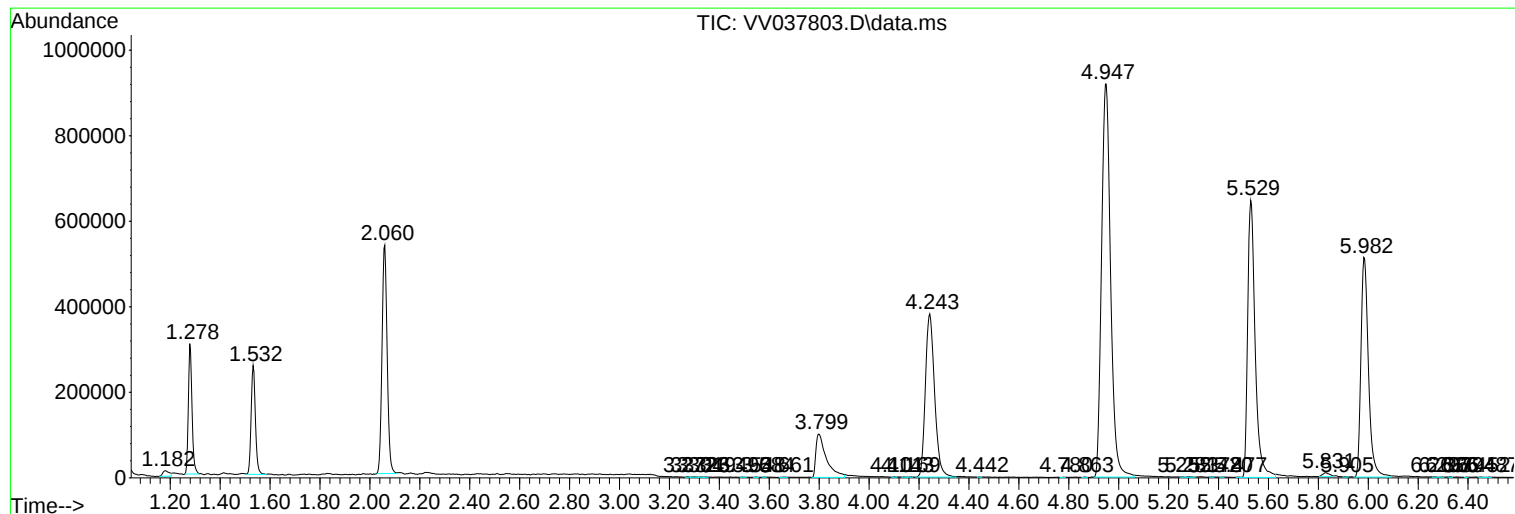

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037803.D
Acq On : 10 Oct 2024 14:21
Operator : SY/MD
Sample : P4379-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037803.D
Acq On : 10 Oct 2024 14:21
Operator : SY/MD
Sample : P4379-04
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------