

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037804.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4379-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037804.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV	14206	24674	1.06%	0.146%
2	1.278	68	74	90	rVB	290075	309245	13.34%	1.832%
3	1.532	146	153	171	rVB	255983	299061	12.90%	1.772%
4	2.060	308	317	331	rVB	523598	746616	32.20%	4.423%
5	3.542	774	778	782	rBV4	960	841	0.04%	0.005%
6	3.622	801	803	806	rBV2	328	199	0.01%	0.001%
7	3.661	813	815	819	rVB3	482	215	0.01%	0.001%
8	3.706	827	829	831	rBV2	489	274	0.01%	0.002%
9	3.754	841	844	846	rBV2	231	114	0.00%	0.001%
10	3.806	848	860	902	rBV3	284161	778805	33.59%	4.613%
11	4.243	978	996	1026	rBV	378355	957017	41.28%	5.669%
12	4.526	1081	1084	1086	rBV2	852	399	0.02%	0.002%
13	4.600	1104	1107	1109	rVB2	542	263	0.01%	0.002%
14	4.648	1119	1122	1123	rBV2	451	146	0.01%	0.001%
15	4.664	1123	1127	1129	rBV3	566	470	0.02%	0.003%
16	4.680	1129	1132	1137	rBV4	470	416	0.02%	0.002%
17	4.715	1142	1143	1145	rBV	297	120	0.01%	0.001%
18	4.728	1145	1147	1152	rBV4	826	737	0.03%	0.004%
19	4.751	1152	1154	1156	rVB	365	156	0.01%	0.001%
20	4.860	1186	1188	1193	rBV4	557	349	0.02%	0.002%
21	4.879	1193	1194	1199	rVB3	522	267	0.01%	0.002%
22	4.947	1200	1215	1260	rBV2	918075	2318336	100.00%	13.733%
23	5.420	1360	1362	1366	rBV3	524	414	0.02%	0.002%
24	5.529	1385	1396	1423	rBV	640208	1319353	56.91%	7.815%
25	5.982	1525	1537	1574	rBV	505439	1061086	45.77%	6.285%
26	6.294	1632	1634	1636	rBV4	606	377	0.02%	0.002%
27	6.413	1669	1671	1672	rBV2	439	176	0.01%	0.001%
28	6.477	1689	1691	1692	rBV	595	193	0.01%	0.001%
29	6.558	1715	1716	1717	rBV	413	132	0.01%	0.001%
30	6.587	1722	1725	1728	rVB3	791	453	0.02%	0.003%
31	6.616	1728	1734	1735	rBV2	875	785	0.03%	0.005%
32	6.645	1742	1743	1747	rBV2	633	403	0.02%	0.002%
33	6.667	1747	1750	1751	rBV2	485	196	0.01%	0.001%
34	6.693	1756	1758	1760	rBV	520	274	0.01%	0.002%
35	6.706	1760	1762	1765	rBV3	378	173	0.01%	0.001%
36	6.725	1765	1768	1771	rBV3	761	681	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037804.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4379-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.754	1775	1777	1780	rBV3	472	280	0.01%	0.002%
38	6.799	1787	1791	1796	rVB4	729	664	0.03%	0.004%
39	6.822	1796	1798	1799	rBV	317	122	0.01%	0.001%
40	6.834	1799	1802	1804	rBV3	867	497	0.02%	0.003%
41	6.847	1804	1806	1808	rVB2	636	231	0.01%	0.001%
42	6.860	1808	1810	1813	rVB2	545	288	0.01%	0.002%
43	6.908	1813	1825	1855	rBV	250291	492665	21.25%	2.918%
44	7.175	1906	1908	1913	rBV4	839	652	0.03%	0.004%
45	7.236	1916	1927	1950	rBV	1012660	1783723	76.94%	10.566%
46	7.551	2016	2025	2055	rBV	169347	318332	13.73%	1.886%
47	7.960	2147	2152	2154	rBV5	1004	896	0.04%	0.005%
48	8.024	2164	2172	2213	rBV2	296390	667826	28.81%	3.956%
49	8.471	2309	2311	2312	rBV	1050	429	0.02%	0.003%
50	8.654	2367	2368	2370	rBV2	446	205	0.01%	0.001%
51	8.735	2390	2393	2395	rBV3	640	365	0.02%	0.002%
52	8.780	2395	2407	2436	rBV	1027685	1703111	73.46%	10.089%
53	9.268	2555	2559	2562	rBV5	714	674	0.03%	0.004%
54	9.362	2586	2588	2590	rVB2	1032	415	0.02%	0.002%
55	9.403	2599	2601	2606	rBV3	659	527	0.02%	0.003%
56	9.477	2622	2624	2627	rVV3	613	373	0.02%	0.002%
57	9.532	2638	2641	2643	rVB2	613	359	0.02%	0.002%
58	9.583	2654	2657	2659	rVB2	819	420	0.02%	0.002%
59	9.606	2659	2664	2671	rBV5	1009	1014	0.04%	0.006%
60	9.638	2671	2674	2678	rBV3	479	490	0.02%	0.003%
61	9.702	2688	2694	2695	rBV3	779	674	0.03%	0.004%
62	9.738	2701	2705	2710	rBV6	919	1169	0.05%	0.007%
63	9.799	2722	2724	2727	rVB3	550	215	0.01%	0.001%
64	9.866	2743	2745	2748	rBV2	587	357	0.02%	0.002%
65	9.998	2784	2786	2788	rBV2	269	147	0.01%	0.001%
66	10.021	2788	2793	2796	rVB4	841	659	0.03%	0.004%
67	10.037	2796	2798	2800	rBV	441	224	0.01%	0.001%
68	10.053	2800	2803	2808	rVV4	782	596	0.03%	0.004%
69	10.101	2816	2818	2820	rBV2	334	171	0.01%	0.001%
70	10.146	2820	2832	2849	rBV	598315	953279	41.12%	5.647%
71	10.477	2930	2935	2936	rBV3	672	556	0.02%	0.003%
72	10.529	2949	2951	2953	rBV	322	126	0.01%	0.001%
73	10.574	2962	2965	2966	rBV3	669	357	0.02%	0.002%
74	10.609	2974	2976	2978	rVB	795	354	0.02%	0.002%
75	10.625	2978	2981	2984	rBV2	696	349	0.02%	0.002%
76	10.702	3003	3005	3010	rVB2	379	170	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037804.D
 Acq On : 10 Oct 2024 14:42
 Operator : SY/MD
 Sample : P4379-05
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOL96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.722	3010	3011	3013	rBV	387	207	0.01%	0.001%
78	10.754	3017	3021	3026	rBV3	621	679	0.03%	0.004%
79	10.818	3039	3041	3046	rBV4	476	339	0.01%	0.002%
80	10.860	3050	3054	3059	rBV5	978	989	0.04%	0.006%
81	10.924	3072	3074	3077	rVB2	577	320	0.01%	0.002%
82	10.944	3077	3080	3081	rBV2	314	133	0.01%	0.001%
83	10.956	3081	3084	3088	rBV3	353	201	0.01%	0.001%
84	11.008	3097	3100	3102	rBV2	534	355	0.02%	0.002%
85	11.127	3134	3137	3139	rBV4	806	511	0.02%	0.003%
86	11.178	3143	3153	3183	rVV	929495	1478300	63.77%	8.757%
87	11.554	3258	3270	3299	rBV	1013175	1635360	70.54%	9.687%
88	12.046	3421	3423	3425	rBV3	697	350	0.02%	0.002%
89	12.162	3456	3459	3463	rBV3	840	547	0.02%	0.003%
90	12.204	3469	3472	3474	rBV3	634	430	0.02%	0.003%
91	12.233	3479	3481	3484	rBV2	633	363	0.02%	0.002%
92	12.323	3505	3509	3512	rBV5	765	671	0.03%	0.004%
93	12.365	3517	3522	3523	rBV4	817	615	0.03%	0.004%
94	12.394	3529	3531	3533	rVB2	958	380	0.02%	0.002%
95	12.882	3680	3683	3684	rBV	613	304	0.01%	0.002%
96	13.085	3743	3746	3749	rBV3	897	659	0.03%	0.004%
97	13.214	3785	3786	3792	rVB3	1022	759	0.03%	0.004%
98	13.287	3806	3809	3811	rBV2	494	301	0.01%	0.002%
99	13.641	3917	3919	3923	rBV3	948	703	0.03%	0.004%
100	13.699	3934	3937	3940	rBV3	807	729	0.03%	0.004%




Sum of corrected areas: 16881582

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037804.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4379-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

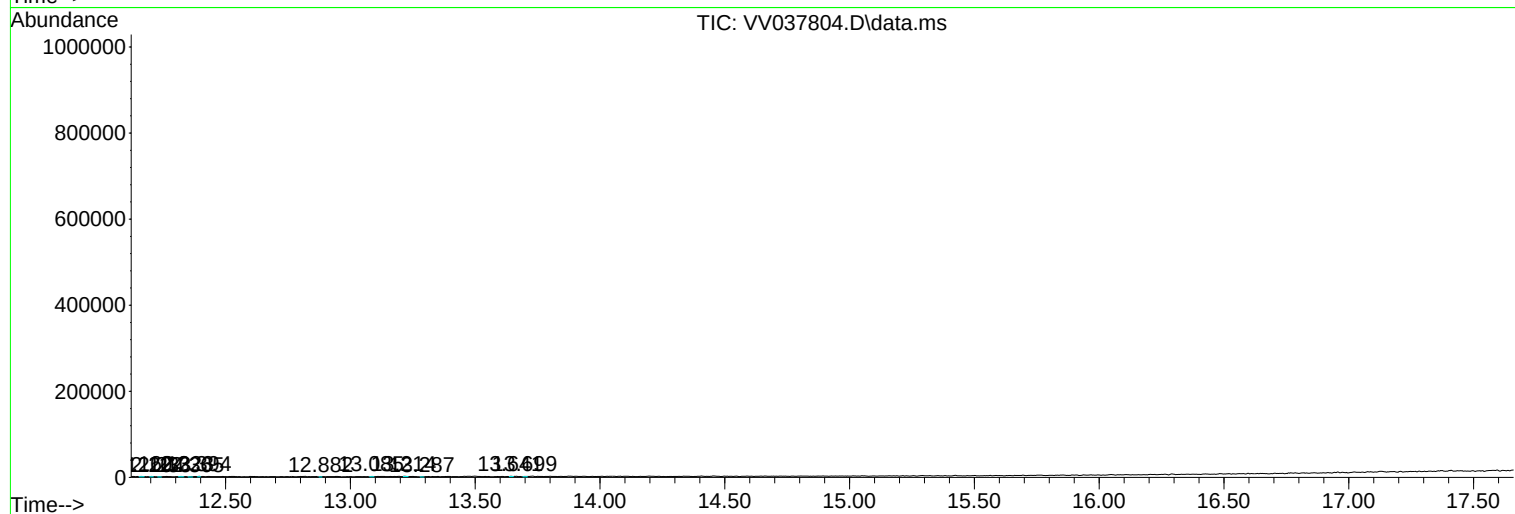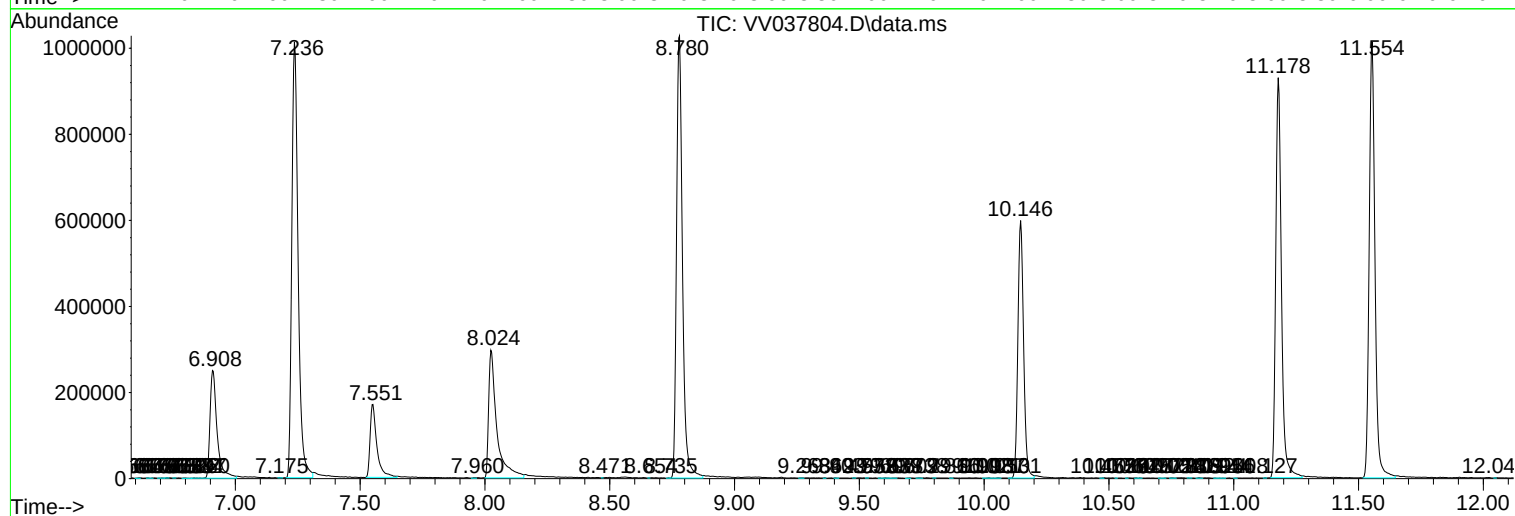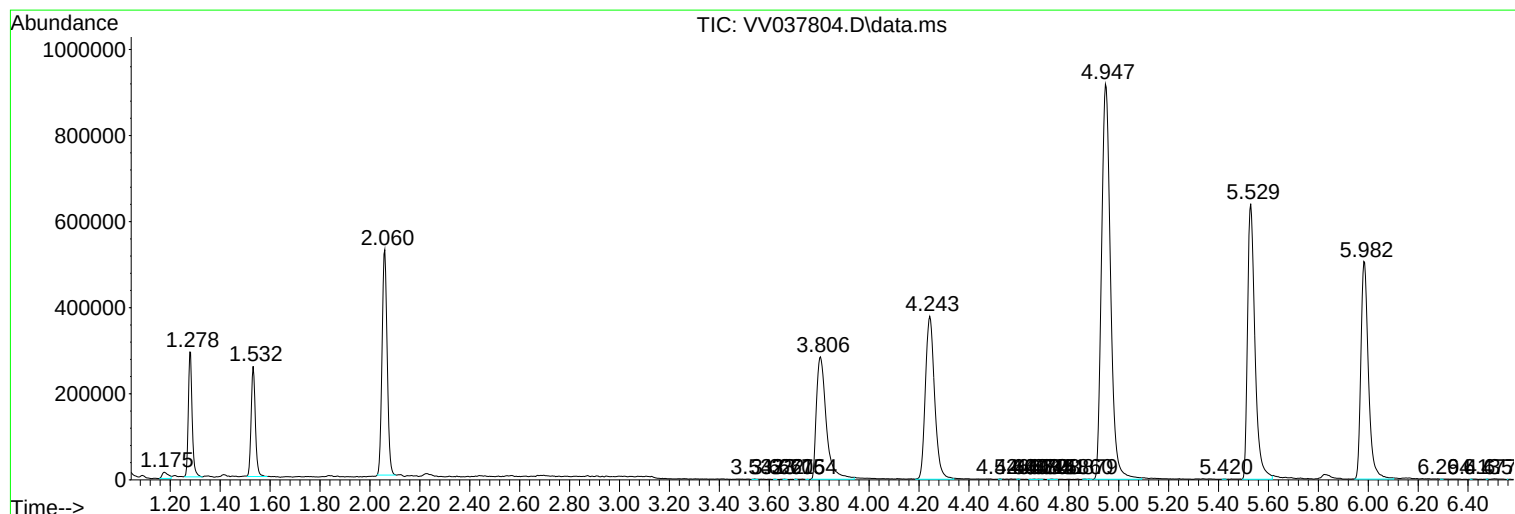

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037804.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4379-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037804.D
Acq On : 10 Oct 2024 14:42
Operator : SY/MD
Sample : P4379-05
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOL96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------