

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037806.D
 Acq On : 10 Oct 2024 15:26
 Operator : SY/MD
 Sample : P4379-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	52	rBV	13388	21684	0.92%	0.129%
2	1.278	68	74	90	rVB	294471	312637	13.33%	1.858%
3	1.532	146	153	168	rVB	259470	306009	13.05%	1.819%
4	2.060	308	317	332	rVB	532050	759582	32.38%	4.515%
5	3.442	744	747	751	rBV3	835	603	0.03%	0.004%
6	3.519	768	771	774	rBV2	852	665	0.03%	0.004%
7	3.574	785	788	791	rVB2	674	349	0.01%	0.002%
8	3.593	791	794	796	rBV2	431	288	0.01%	0.002%
9	3.645	809	810	812	rVB	561	193	0.01%	0.001%
10	3.680	816	821	826	rBV3	622	714	0.03%	0.004%
11	3.799	849	858	888	rBV2	100573	290636	12.39%	1.728%
12	4.243	981	996	1029	rBV	384373	970238	41.37%	5.768%
13	4.455	1060	1062	1064	rBV3	457	314	0.01%	0.002%
14	4.561	1091	1095	1098	rBV3	708	548	0.02%	0.003%
15	4.593	1102	1105	1106	rBV2	537	291	0.01%	0.002%
16	4.658	1122	1125	1127	rBV3	491	291	0.01%	0.002%
17	4.715	1141	1143	1145	rBV2	428	179	0.01%	0.001%
18	4.818	1172	1175	1177	rBV3	412	306	0.01%	0.002%
19	4.889	1194	1197	1200	rBV4	615	450	0.02%	0.003%
20	4.947	1200	1215	1251	rBV2	926220	2345528	100.00%	13.943%
21	5.381	1348	1350	1353	rVB2	1027	501	0.02%	0.003%
22	5.397	1353	1355	1358	rBV	530	360	0.02%	0.002%
23	5.420	1358	1362	1366	rBV4	835	956	0.04%	0.006%
24	5.465	1373	1376	1379	rBV4	498	300	0.01%	0.002%
25	5.529	1385	1396	1431	rBV	660719	1377360	58.72%	8.188%
26	5.982	1526	1537	1570	rBV	517455	1070782	45.65%	6.365%
27	6.230	1613	1614	1616	rBV	687	325	0.01%	0.002%
28	6.297	1631	1635	1638	rBV3	447	452	0.02%	0.003%
29	6.355	1652	1653	1654	rBV3	600	155	0.01%	0.001%
30	6.442	1678	1680	1681	rBV	328	133	0.01%	0.001%
31	6.481	1690	1692	1694	rVV3	418	210	0.01%	0.001%
32	6.503	1697	1699	1700	rBV	518	176	0.01%	0.001%
33	6.539	1707	1710	1712	rVB3	609	356	0.02%	0.002%
34	6.555	1712	1715	1717	rBV	782	436	0.02%	0.003%
35	6.619	1734	1735	1738	rVB3	403	135	0.01%	0.001%
36	6.641	1741	1742	1745	rVB	514	215	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037806.D
 Acq On : 10 Oct 2024 15:26
 Operator : SY/MD
 Sample : P4379-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.683	1752	1755	1757	rBV2	430	301	0.01%	0.002%
38	6.693	1757	1758	1761	rVB2	687	256	0.01%	0.002%
39	6.731	1761	1770	1771	rBV6	1133	1152	0.05%	0.007%
40	6.805	1790	1793	1796	rVB3	797	468	0.02%	0.003%
41	6.854	1804	1808	1810	rBV3	463	330	0.01%	0.002%
42	6.908	1815	1825	1861	rBV	254512	498409	21.25%	2.963%
43	7.236	1916	1927	1959	rBV	1032638	1839462	78.42%	10.935%
44	7.548	2016	2024	2052	rBV	170689	324193	13.82%	1.927%
45	7.918	2137	2139	2142	rVB3	1089	542	0.02%	0.003%
46	7.950	2146	2149	2151	rBV	637	401	0.02%	0.002%
47	7.973	2154	2156	2159	rVB4	646	325	0.01%	0.002%
48	8.024	2164	2172	2209	rBV2	302352	677542	28.89%	4.028%
49	8.558	2330	2338	2341	rBV6	2646	3338	0.14%	0.020%
50	8.719	2385	2388	2396	rVB8	915	1044	0.04%	0.006%
51	8.780	2396	2407	2439	rBV	1064503	1773461	75.61%	10.542%
52	9.182	2530	2532	2534	rBV	563	326	0.01%	0.002%
53	9.236	2548	2549	2551	rBV2	557	203	0.01%	0.001%
54	9.297	2564	2568	2569	rBV3	514	359	0.02%	0.002%
55	9.323	2574	2576	2577	rBV	480	230	0.01%	0.001%
56	9.355	2583	2586	2588	rBV3	355	227	0.01%	0.001%
57	9.378	2588	2593	2594	rBV3	793	569	0.02%	0.003%
58	9.432	2606	2610	2614	rVB3	392	324	0.01%	0.002%
59	9.545	2642	2645	2647	rBV2	609	489	0.02%	0.003%
60	9.580	2653	2656	2660	rBV2	735	580	0.02%	0.003%
61	9.638	2672	2674	2676	rBV	593	373	0.02%	0.002%
62	9.686	2685	2689	2692	rVB4	557	333	0.01%	0.002%
63	9.786	2718	2720	2722	rVB	408	176	0.01%	0.001%
64	9.809	2724	2727	2729	rVB2	347	157	0.01%	0.001%
65	9.834	2733	2735	2736	rVV2	550	135	0.01%	0.001%
66	9.866	2741	2745	2747	rBV3	427	344	0.01%	0.002%
67	9.966	2772	2776	2780	rVV3	885	696	0.03%	0.004%
68	9.989	2780	2783	2787	rVB2	678	406	0.02%	0.002%
69	10.011	2787	2790	2792	rBV2	832	444	0.02%	0.003%
70	10.053	2801	2803	2805	rBV	343	162	0.01%	0.001%
71	10.066	2805	2807	2809	rVV2	617	311	0.01%	0.002%
72	10.146	2820	2832	2859	rBV	613657	976885	41.65%	5.807%
73	10.339	2890	2892	2896	rVB4	789	512	0.02%	0.003%
74	10.362	2896	2899	2902	rBV2	695	553	0.02%	0.003%
75	10.509	2944	2945	2947	rBV	470	221	0.01%	0.001%
76	10.532	2950	2952	2954	rBV	561	296	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037806.D
 Acq On : 10 Oct 2024 15:26
 Operator : SY/MD
 Sample : P4379-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.593	2969	2971	2973	rBV3	530	307	0.01%	0.002%
78	10.622	2978	2980	2983	rVB2	497	250	0.01%	0.001%
79	10.641	2984	2986	2988	rVV3	404	216	0.01%	0.001%
80	10.693	2999	3002	3006	rVB2	373	240	0.01%	0.001%
81	10.731	3011	3014	3017	rBV2	863	474	0.02%	0.003%
82	10.747	3017	3019	3021	rBV2	347	179	0.01%	0.001%
83	10.780	3026	3029	3031	rBV4	617	345	0.01%	0.002%
84	10.834	3042	3046	3049	rBV4	487	403	0.02%	0.002%
85	11.011	3096	3101	3104	rBV4	470	514	0.02%	0.003%
86	11.053	3110	3114	3116	rBV	599	464	0.02%	0.003%
87	11.082	3121	3123	3125	rVV	371	202	0.01%	0.001%
88	11.133	3135	3139	3142	rBV3	717	675	0.03%	0.004%
89	11.178	3142	3153	3186	rBV	980121	1559605	66.49%	9.271%
90	11.554	3258	3270	3298	rBV	1022706	1682345	71.73%	10.001%
91	11.992	3404	3406	3410	rVB3	1217	682	0.03%	0.004%
92	12.339	3512	3514	3516	rBV	419	185	0.01%	0.001%
93	12.378	3524	3526	3529	rBV	655	359	0.02%	0.002%
94	12.390	3529	3530	3533	rBV3	670	289	0.01%	0.002%
95	12.484	3557	3559	3563	rVB3	1287	811	0.03%	0.005%
96	12.513	3564	3568	3572	rBV4	720	783	0.03%	0.005%
97	12.609	3596	3598	3602	rBV4	725	484	0.02%	0.003%
98	12.902	3687	3689	3691	rBV	470	249	0.01%	0.001%
99	12.924	3691	3696	3698	rVV3	631	607	0.03%	0.004%
100	13.509	3876	3878	3880	rBV3	894	496	0.02%	0.003%




Sum of corrected areas: 16822056

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037806.D
Acq On : 10 Oct 2024 15:26
Operator : SY/MD
Sample : P4379-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

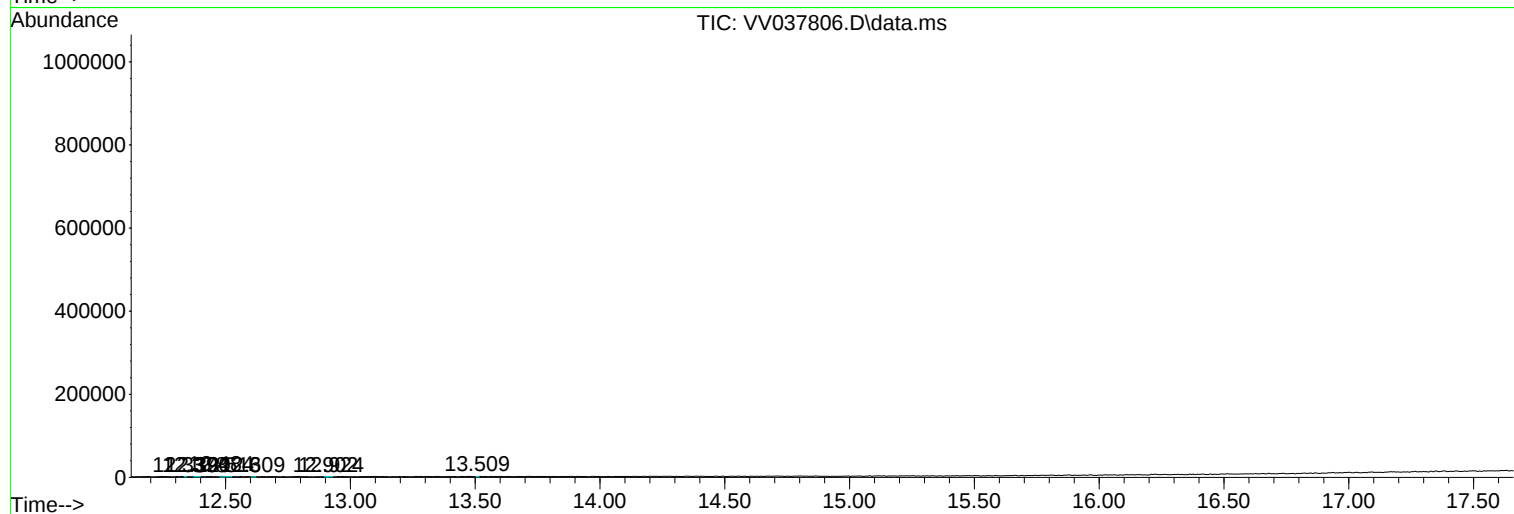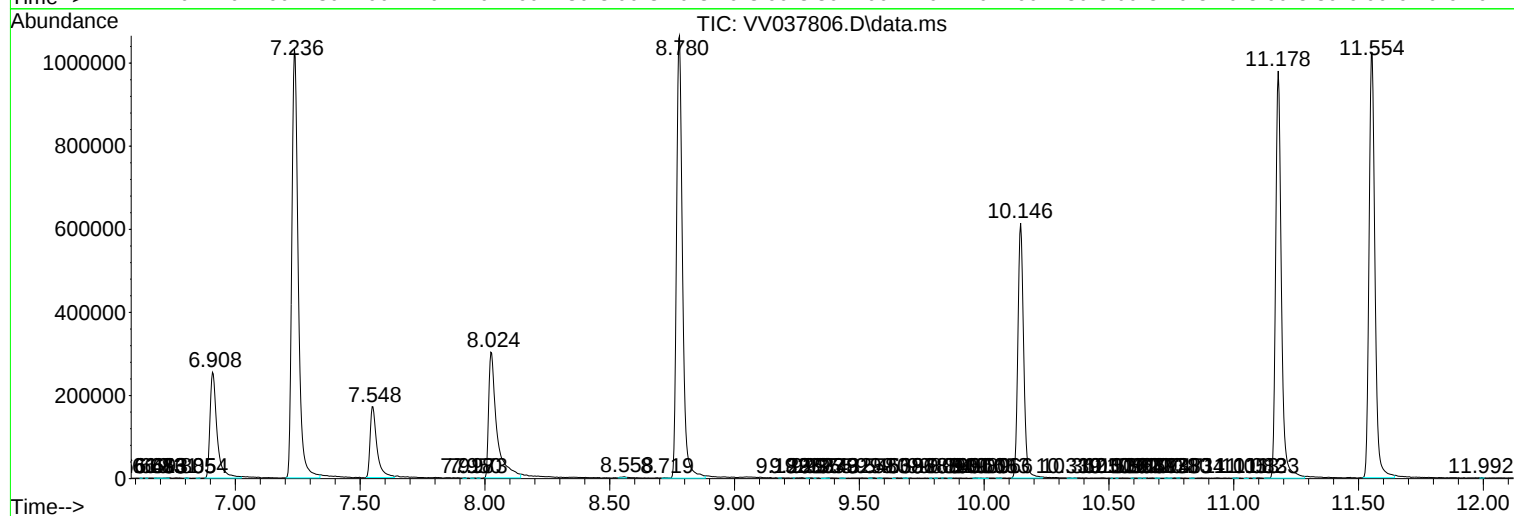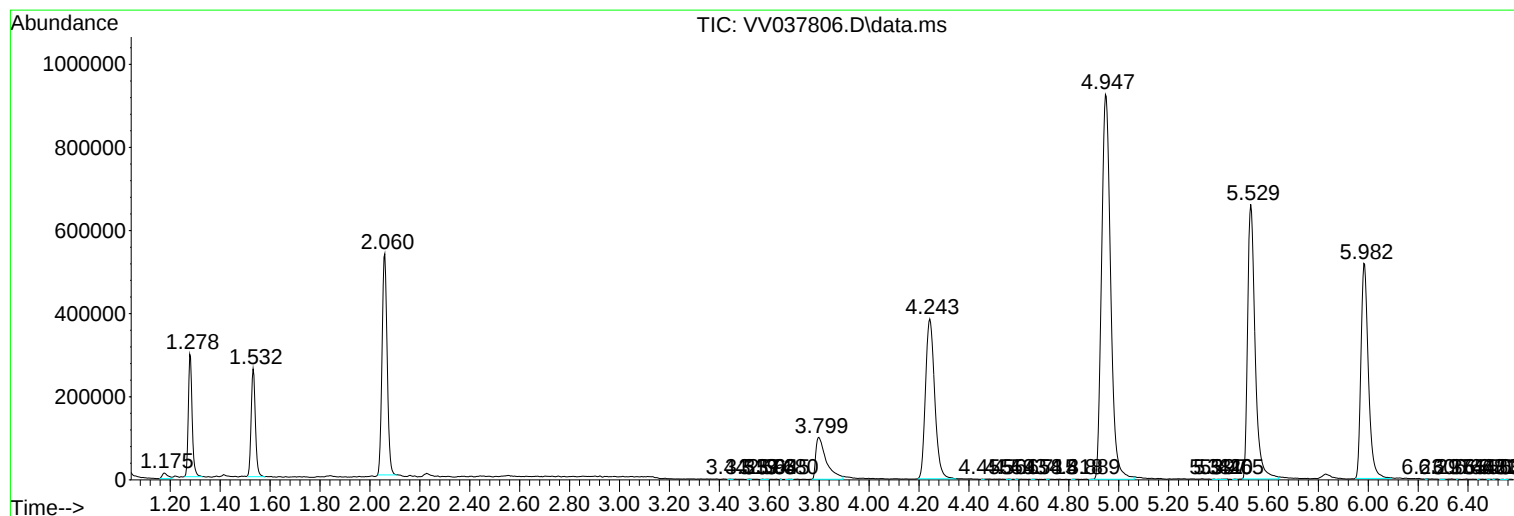

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037806.D
Acq On : 10 Oct 2024 15:26
Operator : SY/MD
Sample : P4379-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037806.D
Acq On : 10 Oct 2024 15:26
Operator : SY/MD
Sample : P4379-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------