

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037807.D
 Acq On : 10 Oct 2024 15:47
 Operator : SY/MD
 Sample : P4379-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	52	rBV	11249	17748	0.75%	0.105%
2	1.278	68	74	91	rVB	288801	311127	13.13%	1.838%
3	1.532	146	153	169	rVB	260229	311800	13.15%	1.842%
4	2.060	308	317	332	rBV	540268	769628	32.47%	4.547%
5	3.243	682	685	688	rBV4	692	498	0.02%	0.003%
6	3.445	746	748	751	rVB	854	465	0.02%	0.003%
7	3.539	775	777	778	rBV	448	137	0.01%	0.001%
8	3.574	786	788	790	rBV2	367	228	0.01%	0.001%
9	3.590	790	793	796	rVV4	812	645	0.03%	0.004%
10	3.799	849	858	894	rBV	102942	301486	12.72%	1.781%
11	4.243	979	996	1025	rBV	393263	991184	41.82%	5.856%
12	4.667	1126	1128	1129	rBV	697	289	0.01%	0.002%
13	4.696	1135	1137	1139	rBV	450	295	0.01%	0.002%
14	4.728	1144	1147	1150	rBV2	504	377	0.02%	0.002%
15	4.748	1150	1153	1154	rVV2	560	268	0.01%	0.002%
16	4.770	1158	1160	1161	rVV	317	88	0.00%	0.001%
17	4.796	1167	1168	1172	rBV3	340	214	0.01%	0.001%
18	4.825	1172	1177	1178	rBV4	631	410	0.02%	0.002%
19	4.950	1195	1216	1251	rBV2	938324	2370393	100.00%	14.005%
20	5.484	1380	1382	1384	rBV2	466	243	0.01%	0.001%
21	5.529	1385	1396	1428	rBV	662964	1384846	58.42%	8.182%
22	5.982	1524	1537	1568	rBV	527734	1098081	46.32%	6.488%
23	6.294	1631	1634	1636	rBV2	786	539	0.02%	0.003%
24	6.333	1644	1646	1647	rBV2	521	273	0.01%	0.002%
25	6.490	1693	1695	1698	rBV3	545	396	0.02%	0.002%
26	6.506	1698	1700	1702	rVB2	840	403	0.02%	0.002%
27	6.571	1718	1720	1725	rVB4	587	477	0.02%	0.003%
28	6.600	1725	1729	1732	rBV4	572	482	0.02%	0.003%
29	6.616	1732	1734	1736	rVV2	515	210	0.01%	0.001%
30	6.651	1739	1745	1748	rBV4	620	569	0.02%	0.003%
31	6.674	1748	1752	1753	rBV3	765	441	0.02%	0.003%
32	6.712	1760	1764	1766	rBV2	452	361	0.02%	0.002%
33	6.838	1800	1803	1809	rBV4	794	794	0.03%	0.005%
34	6.860	1809	1810	1811	rBV4	246	74	0.00%	0.000%
35	6.870	1811	1813	1814	rVB	601	171	0.01%	0.001%
36	6.908	1814	1825	1854	rBV	252995	497808	21.00%	2.941%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037807.D
 Acq On : 10 Oct 2024 15:47
 Operator : SY/MD
 Sample : P4379-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.236	1916	1927	1956	rBV	1046769	1855377	78.27%	10.962%
38	7.551	2016	2025	2053	rBV2	169824	330444	13.94%	1.952%
39	7.940	2143	2146	2149	rBV3	507	405	0.02%	0.002%
40	8.024	2164	2172	2211	rBV2	303849	678732	28.63%	4.010%
41	8.709	2383	2385	2388	rBV3	827	378	0.02%	0.002%
42	8.725	2388	2390	2394	rVB2	461	267	0.01%	0.002%
43	8.776	2396	2406	2429	rBV	1060470	1758442	74.18%	10.389%
44	9.191	2531	2535	2542	rBV6	840	1029	0.04%	0.006%
45	9.223	2542	2545	2548	rBV2	664	480	0.02%	0.003%
46	9.252	2552	2554	2556	rBV2	670	349	0.01%	0.002%
47	9.291	2563	2566	2568	rBV4	505	323	0.01%	0.002%
48	9.561	2649	2650	2651	rBV4	258	99	0.00%	0.001%
49	9.571	2651	2653	2656	rVV3	448	254	0.01%	0.002%
50	9.641	2673	2675	2677	rBV	316	173	0.01%	0.001%
51	9.709	2692	2696	2697	rBV	830	472	0.02%	0.003%
52	9.754	2708	2710	2714	rVB2	652	306	0.01%	0.002%
53	9.776	2714	2717	2718	rBV	389	204	0.01%	0.001%
54	9.847	2738	2739	2740	rBV	384	91	0.00%	0.001%
55	9.895	2752	2754	2758	rVB2	532	257	0.01%	0.002%
56	9.921	2760	2762	2764	rBV	395	160	0.01%	0.001%
57	9.976	2774	2779	2780	rBV2	591	438	0.02%	0.003%
58	10.030	2794	2796	2799	rBV2	491	313	0.01%	0.002%
59	10.053	2801	2803	2808	rVB4	583	328	0.01%	0.002%
60	10.075	2808	2810	2812	rBV	329	183	0.01%	0.001%
61	10.085	2812	2813	2816	rVB2	723	274	0.01%	0.002%
62	10.146	2820	2832	2852	rBV	603946	974825	41.13%	5.759%
63	10.397	2906	2910	2912	rBV3	353	333	0.01%	0.002%
64	10.480	2932	2936	2939	rBV5	713	618	0.03%	0.004%
65	10.558	2957	2960	2963	rBV3	614	419	0.02%	0.002%
66	10.632	2981	2983	2986	rBV	610	392	0.02%	0.002%
67	10.706	3003	3006	3008	rBV2	382	233	0.01%	0.001%
68	10.741	3014	3017	3020	rBV3	660	505	0.02%	0.003%
69	10.853	3050	3052	3054	rBV3	643	380	0.02%	0.002%
70	10.940	3076	3079	3080	rBV	371	238	0.01%	0.001%
71	11.001	3096	3098	3100	rBV2	491	194	0.01%	0.001%
72	11.014	3100	3102	3106	rVV4	627	367	0.02%	0.002%
73	11.033	3106	3108	3112	rVB2	526	297	0.01%	0.002%
74	11.059	3112	3116	3117	rVB3	448	261	0.01%	0.002%
75	11.072	3117	3120	3123	rBV2	718	357	0.02%	0.002%
76	11.098	3126	3128	3134	rBV3	576	560	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037807.D
Acq On : 10 Oct 2024 15:47
Operator : SY/MD
Sample : P4379-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	11.178	3142	3153	3185	rBV	970685	1555169	65.61%	9.188%
78	11.551	3256	3269	3303	rBV	1048949	1690398	71.31%	9.987%
79	11.863	3363	3366	3369	rBV3	698	591	0.02%	0.003%
80	11.947	3390	3392	3394	rBV2	1083	595	0.03%	0.004%
81	12.078	3431	3433	3435	rBV2	434	206	0.01%	0.001%
82	12.149	3452	3455	3458	rBV3	998	684	0.03%	0.004%
83	12.262	3488	3490	3495	rBV2	646	590	0.02%	0.003%
84	12.304	3500	3503	3507	rBV2	749	692	0.03%	0.004%
85	12.336	3511	3513	3515	rBV2	635	262	0.01%	0.002%
86	12.419	3537	3539	3543	rBV2	442	265	0.01%	0.002%
87	12.439	3543	3545	3546	rBV2	519	178	0.01%	0.001%
88	12.612	3598	3599	3600	rBV	356	103	0.00%	0.001%
89	12.702	3625	3627	3632	rVB4	844	586	0.02%	0.003%
90	12.844	3668	3671	3672	rBV	924	524	0.02%	0.003%
91	12.885	3682	3684	3687	rBV3	621	402	0.02%	0.002%
92	13.262	3797	3801	3804	rBV3	1185	1068	0.05%	0.006%
93	14.069	4050	4052	4054	rBV2	721	361	0.02%	0.002%




Sum of corrected areas: 16925879

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037807.D
Acq On : 10 Oct 2024 15:47
Operator : SY/MD
Sample : P4379-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

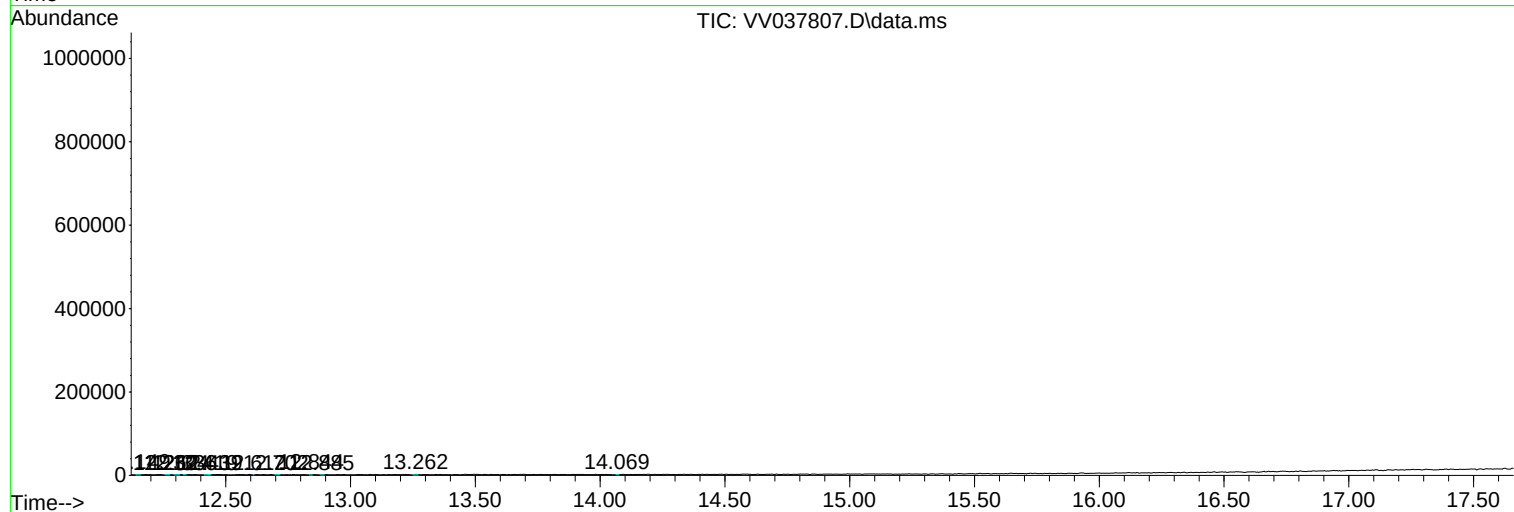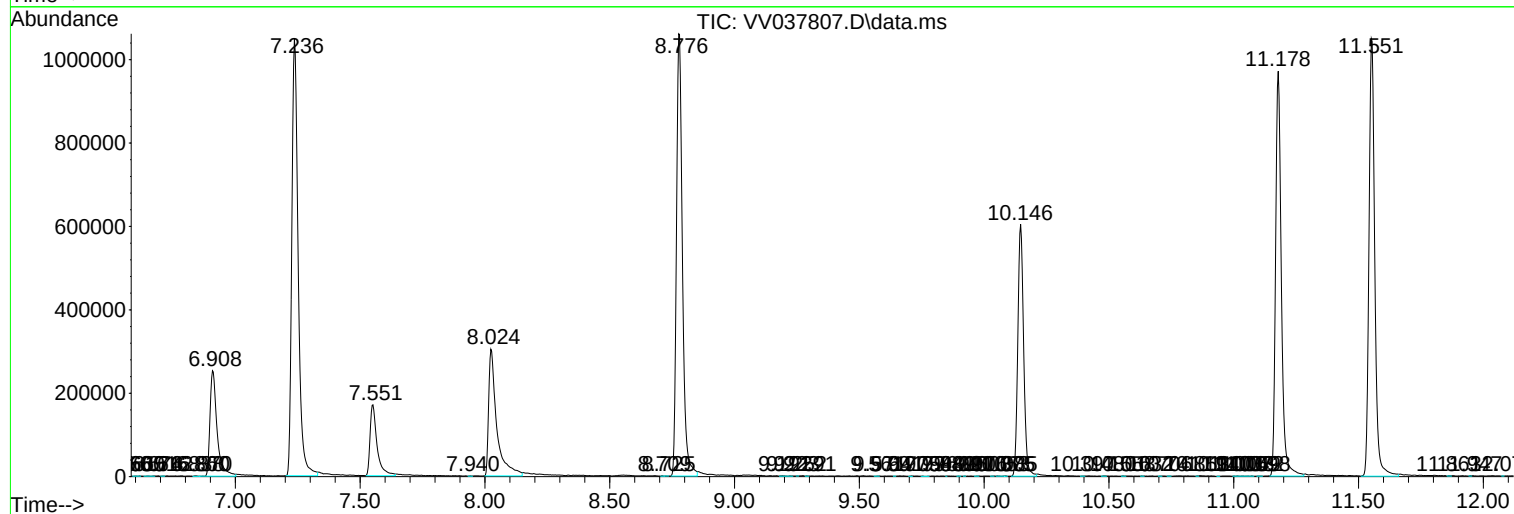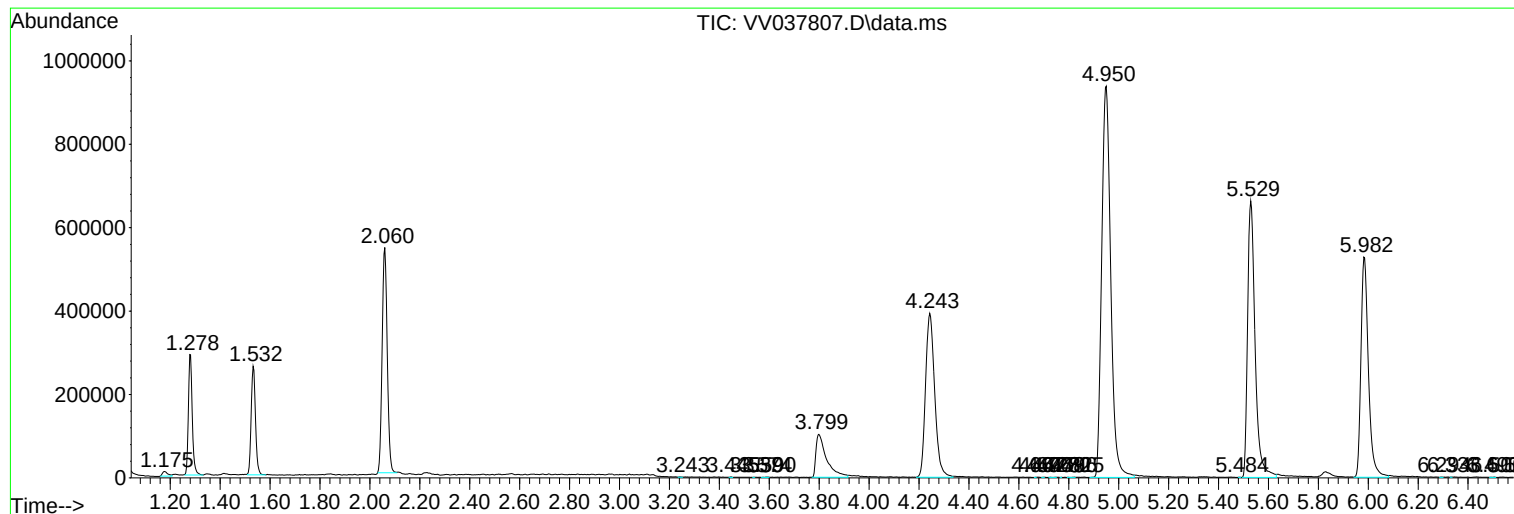

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037807.D
Acq On : 10 Oct 2024 15:47
Operator : SY/MD
Sample : P4379-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037807.D
Acq On : 10 Oct 2024 15:47
Operator : SY/MD
Sample : P4379-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc