

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037808.D
 Acq On : 10 Oct 2024 16:09
 Operator : SY/MD
 Sample : P4379-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.178	37	43	51	rBV	12103	18705	0.75%	0.098%
2	1.281	68	75	91	rVB2	350694	382384	15.40%	1.999%
3	1.532	146	153	168	rVB	257596	302996	12.21%	1.584%
4	2.059	308	317	333	rVB	535267	771076	31.06%	4.032%
5	3.281	694	697	699	rBV2	851	571	0.02%	0.003%
6	3.455	748	751	754	rBV3	664	500	0.02%	0.003%
7	3.493	761	763	764	rBV	598	218	0.01%	0.001%
8	3.526	769	773	775	rBV3	528	309	0.01%	0.002%
9	3.596	793	795	798	rBV3	507	351	0.01%	0.002%
10	3.645	806	810	812	rBV3	356	294	0.01%	0.002%
11	3.686	818	823	826	rBV	378	358	0.01%	0.002%
12	3.805	846	860	900	rBV2	1015570	2482535	100.00%	12.981%
13	4.243	981	996	1032	rVB	379815	966566	38.93%	5.054%
14	4.661	1122	1126	1128	rBV3	735	505	0.02%	0.003%
15	4.696	1132	1137	1141	rBV4	686	715	0.03%	0.004%
16	4.796	1165	1168	1173	rBV6	704	808	0.03%	0.004%
17	4.863	1186	1189	1191	rBV2	539	378	0.02%	0.002%
18	4.950	1199	1216	1249	rBV2	936676	2356807	94.94%	12.323%
19	5.400	1354	1356	1358	rVB2	724	251	0.01%	0.001%
20	5.455	1369	1373	1374	rBV	862	520	0.02%	0.003%
21	5.529	1385	1396	1440	rBV	653105	1386803	55.86%	7.251%
22	5.982	1525	1537	1572	rBV	522777	1083018	43.63%	5.663%
23	6.307	1636	1638	1643	rVB4	709	399	0.02%	0.002%
24	6.442	1678	1680	1681	rBV	587	285	0.01%	0.001%
25	6.480	1689	1692	1694	rBV3	689	530	0.02%	0.003%
26	6.590	1723	1726	1727	rBV2	705	299	0.01%	0.002%
27	6.606	1727	1731	1734	rVV4	760	664	0.03%	0.003%
28	6.619	1734	1735	1737	rVV	698	268	0.01%	0.001%
29	6.635	1737	1740	1742	rVB3	504	260	0.01%	0.001%
30	6.670	1749	1751	1753	rBV	571	234	0.01%	0.001%
31	6.689	1755	1757	1759	rBV2	512	289	0.01%	0.002%
32	6.728	1767	1769	1772	rVB3	497	318	0.01%	0.002%
33	6.751	1772	1776	1779	rBV2	826	788	0.03%	0.004%
34	6.763	1779	1780	1786	rVB5	631	520	0.02%	0.003%
35	6.802	1789	1792	1797	rVB4	1073	811	0.03%	0.004%
36	6.828	1797	1800	1804	rBV3	518	353	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037808.D
 Acq On : 10 Oct 2024 16:09
 Operator : SY/MD
 Sample : P4379-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.853	1804	1808	1810	rBV2	505	409	0.02%	0.002%
38	6.908	1813	1825	1861	rBV	254189	499267	20.11%	2.611%
39	7.236	1917	1927	1963	rBV	1031369	1853735	74.67%	9.693%
40	7.551	2016	2025	2054	rBV	170728	320851	12.92%	1.678%
41	7.837	2111	2114	2116	rBV2	1019	551	0.02%	0.003%
42	7.863	2119	2122	2123	rBV	1021	561	0.02%	0.003%
43	7.931	2140	2143	2146	rBV2	758	576	0.02%	0.003%
44	7.979	2153	2158	2160	rBV4	678	594	0.02%	0.003%
45	8.024	2164	2172	2213	rBV2	300242	684561	27.58%	3.579%
46	8.522	2323	2327	2328	rBV3	985	696	0.03%	0.004%
47	8.779	2395	2407	2441	rBV	1049445	1760195	70.90%	9.204%
48	9.223	2542	2545	2548	rBV3	720	594	0.02%	0.003%
49	9.278	2559	2562	2563	rBV3	554	294	0.01%	0.002%
50	9.371	2589	2591	2593	rBV2	544	280	0.01%	0.001%
51	9.387	2593	2596	2598	rVV3	739	527	0.02%	0.003%
52	9.461	2616	2619	2623	rBV5	547	451	0.02%	0.002%
53	9.532	2634	2641	2642	rBV4	858	935	0.04%	0.005%
54	9.564	2647	2651	2655	rVV4	628	600	0.02%	0.003%
55	9.583	2655	2657	2660	rVB2	537	272	0.01%	0.001%
56	9.654	2678	2679	2682	rBV2	549	210	0.01%	0.001%
57	9.718	2694	2699	2702	rBV4	605	531	0.02%	0.003%
58	9.750	2705	2709	2710	rBV3	413	280	0.01%	0.001%
59	9.795	2720	2723	2724	rBV2	511	306	0.01%	0.002%
60	9.889	2748	2752	2755	rVB2	620	381	0.02%	0.002%
61	9.950	2768	2771	2775	rBV5	454	376	0.02%	0.002%
62	10.066	2805	2807	2809	rBV	598	286	0.01%	0.001%
63	10.146	2821	2832	2857	rBV	619031	987020	39.76%	5.161%
64	10.429	2917	2920	2921	rBV	387	228	0.01%	0.001%
65	10.439	2921	2923	2925	rVV2	634	356	0.01%	0.002%
66	10.455	2926	2928	2932	rVB2	975	528	0.02%	0.003%
67	10.503	2939	2943	2946	rBV3	467	389	0.02%	0.002%
68	10.586	2966	2969	2970	rBV3	521	242	0.01%	0.001%
69	10.622	2977	2980	2982	rBV2	611	381	0.02%	0.002%
70	10.660	2987	2992	2996	rVV4	495	538	0.02%	0.003%
71	10.705	3004	3006	3010	rBV2	464	321	0.01%	0.002%
72	10.750	3017	3020	3023	rVB2	762	405	0.02%	0.002%
73	10.786	3023	3031	3033	rBV4	924	847	0.03%	0.004%
74	10.818	3039	3041	3045	rVB3	762	345	0.01%	0.002%
75	10.844	3045	3049	3051	rBV2	536	308	0.01%	0.002%
76	10.866	3053	3056	3057	rBV	734	399	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037808.D
 Acq On : 10 Oct 2024 16:09
 Operator : SY/MD
 Sample : P4379-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.898	3064	3066	3070	rVB2	614	252	0.01%	0.001%
78	11.075	3119	3121	3123	rVB2	584	248	0.01%	0.001%
79	11.130	3136	3138	3141	rBV3	474	246	0.01%	0.001%
80	11.178	3142	3153	3185	rBV	957814	1544178	62.20%	8.074%
81	11.496	3250	3252	3257	rBV3	678	461	0.02%	0.002%
82	11.554	3257	3270	3302	rBV	1031126	1685161	67.88%	8.811%
83	11.918	3380	3383	3385	rBV2	1095	813	0.03%	0.004%
84	12.008	3409	3411	3415	rBV3	369	271	0.01%	0.001%
85	12.085	3432	3435	3436	rBV	608	252	0.01%	0.001%
86	12.213	3470	3475	3477	rBV5	801	852	0.03%	0.004%
87	12.249	3483	3486	3489	rBV4	903	668	0.03%	0.003%
88	12.291	3495	3499	3501	rBV3	814	546	0.02%	0.003%
89	12.403	3530	3534	3536	rBV3	838	667	0.03%	0.003%
90	12.792	3654	3655	3657	rBV	478	273	0.01%	0.001%
91	12.963	3703	3708	3710	rBV4	895	717	0.03%	0.004%
92	12.988	3714	3716	3720	rBV2	811	503	0.02%	0.003%
93	13.020	3723	3726	3729	rVB3	915	641	0.03%	0.003%
94	13.078	3742	3744	3748	rBV3	542	293	0.01%	0.002%
95	13.175	3770	3774	3776	rBV2	1033	708	0.03%	0.004%
96	13.217	3782	3787	3790	rBV3	1101	1016	0.04%	0.005%
97	13.429	3851	3853	3861	rBV6	852	1074	0.04%	0.006%
98	13.580	3896	3900	3902	rBV4	808	506	0.02%	0.003%
99	14.175	4083	4085	4088	rBV3	767	585	0.02%	0.003%
100	14.284	4117	4119	4122	rBV3	1200	811	0.03%	0.004%




Sum of corrected areas: 19125054

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037808.D
Acq On : 10 Oct 2024 16:09
Operator : SY/MD
Sample : P4379-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

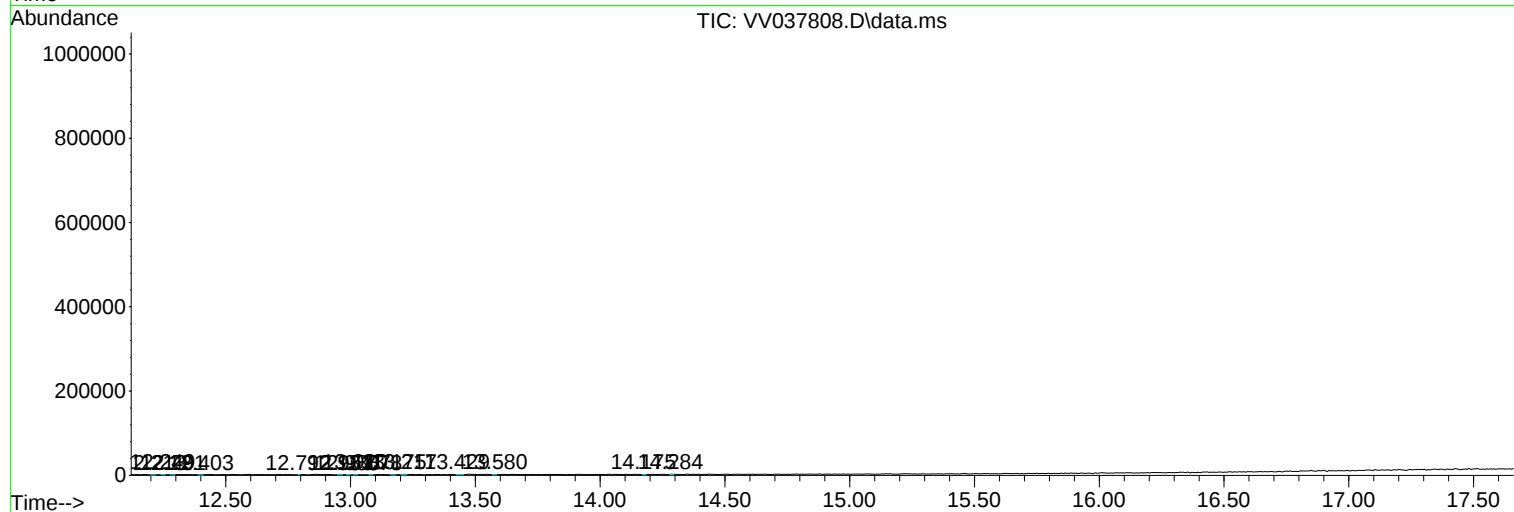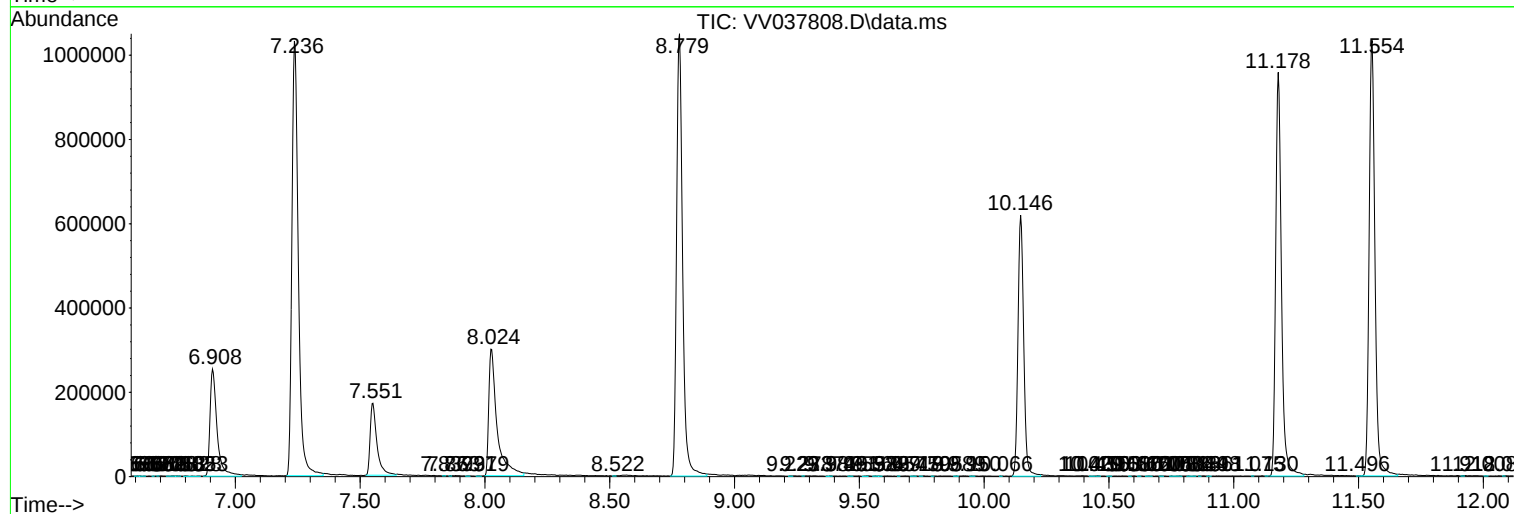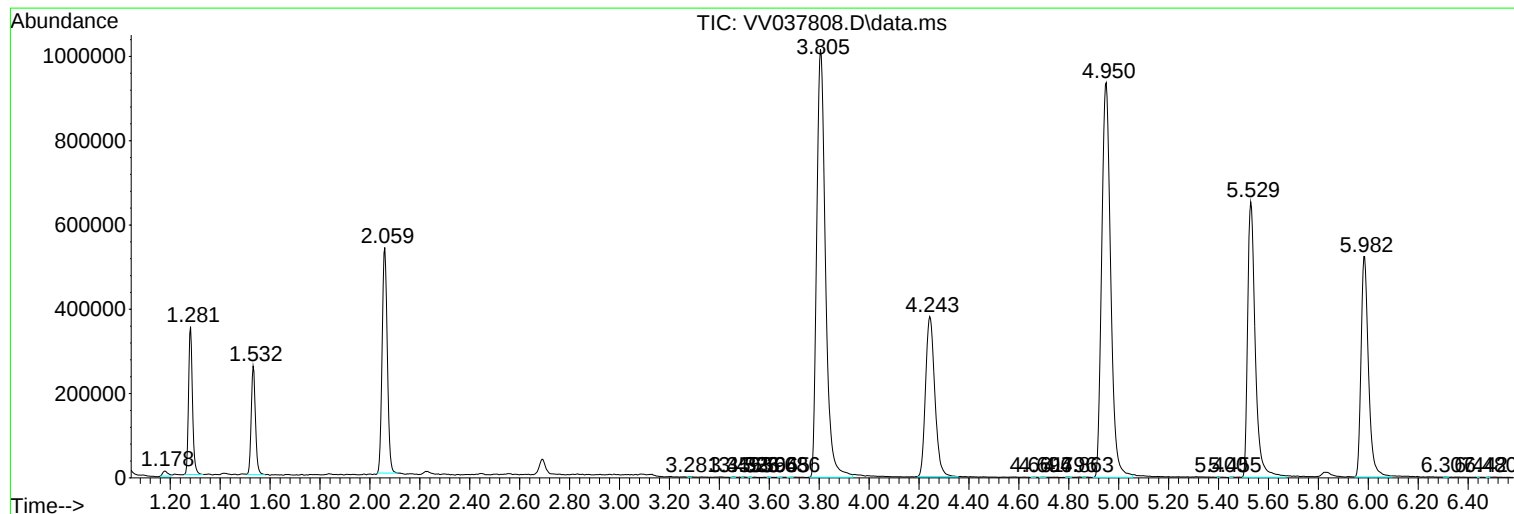

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037808.D
Acq On : 10 Oct 2024 16:09
Operator : SY/MD
Sample : P4379-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037808.D
Acq On : 10 Oct 2024 16:09
Operator : SY/MD
Sample : P4379-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc