
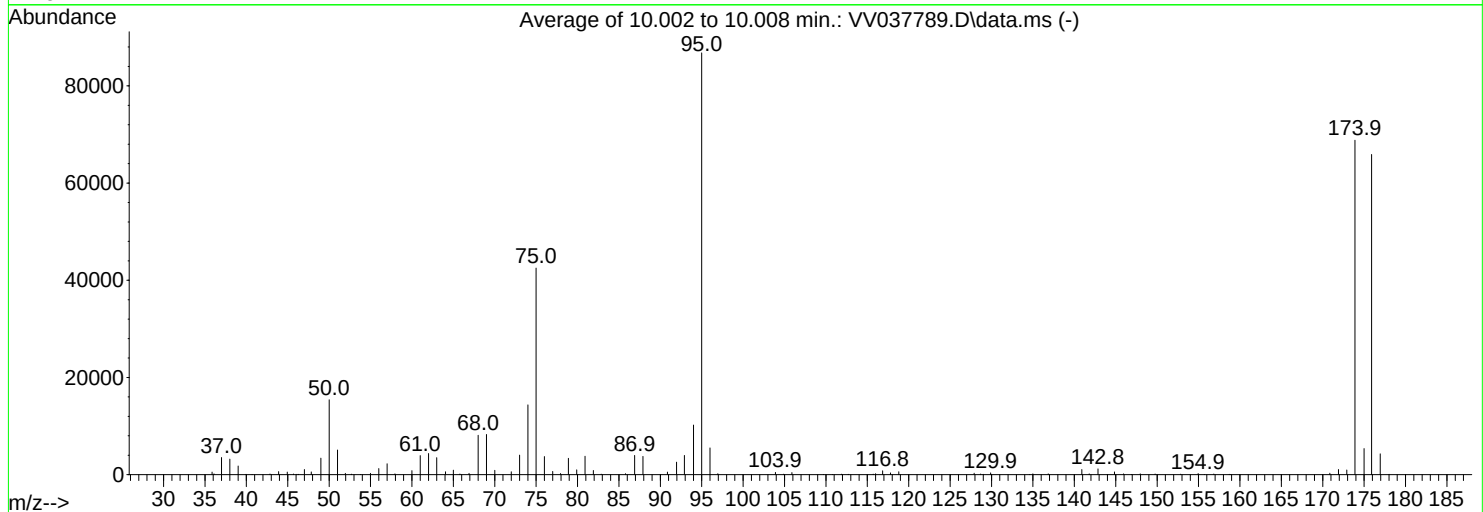


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037789.D
Acq On : 10 Oct 2024 08:44
Operator : SY/MD
Sample : BFB391
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB391

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Fri Oct 11 05:10:27 2024

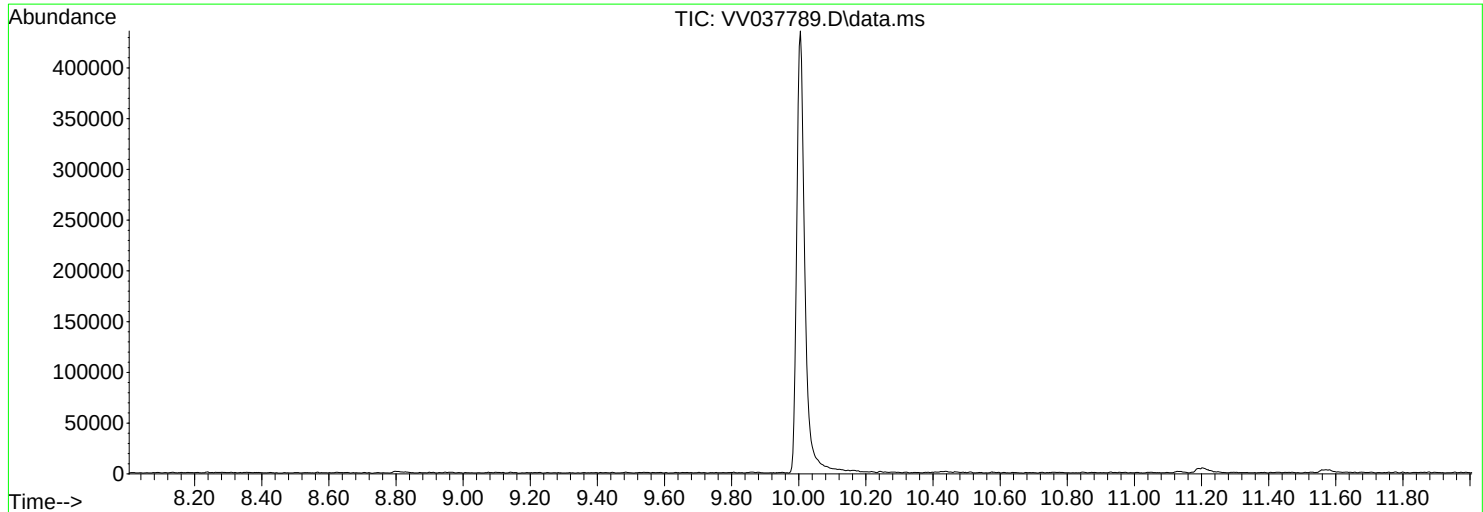

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	15417	PASS
75	95	30	80	49.0	42496	PASS
95	95	100	100	100.0	86800	PASS
96	95	5	9	6.3	5487	PASS
173	174	0.00	2	1.4	942	PASS
174	95	50	120	79.3	68811	PASS
175	174	5	9	7.8	5366	PASS
176	174	95	105	95.7	65880	PASS
177	176	5	10	6.5	4289	PASS

m/z	Abundance
39.90	246.0
41.10	122.0
43.00	121.0
44.00	585.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.90	510.0
37.00	3545.0
38.00	3365.0
39.00	1785.0
40.00	313.0
42.90	104.0
43.10	110.0
43.90	1114.0
45.00	540.0
46.10	207.0
47.00	1027.0
47.80	554.0
49.00	3426.0
50.00	15892.0
51.00	5016.0
52.00	326.0
52.70	109.0
55.00	289.0
56.00	1373.0
57.00	2373.0
57.90	140.0
60.00	838.0
61.00	3996.0
62.00	4370.0
63.00	3610.0
64.10	623.0
65.00	910.0
65.90	148.0
66.90	295.0
68.00	8284.0
69.00	8313.0
70.00	827.0
72.00	565.0
73.00	4394.0
74.00	14251.0
75.00	43568.0
76.00	4002.0
76.90	721.0
78.90	3421.0
79.90	830.0
80.90	3637.0
81.90	834.0
85.80	163.0
86.90	4183.0
87.90	3723.0
90.90	477.0
92.00	2681.0
92.90	3889.0
94.00	10383.0
95.00	87424.0
96.00	5663.0
97.00	189.0
103.90	438.0
104.90	157.0
105.90	362.0
109.70	128.0
112.70	121.0
115.70	257.0
116.90	715.0
117.80	318.0
118.80	543.0
127.90	293.0
128.70	163.0
129.90	411.0
135.00	121.0
136.90	101.0
140.90	1016.0
141.80	165.0
142.90	1149.0
144.80	616.0
146.00	169.0
148.00	246.0
149.80	131.0
152.80	104.0
154.90	262.0
156.90	153.0
158.70	102.0
170.80	288.0
171.90	1034.0
172.90	966.0
173.90	67232.0
175.00	5249.0
175.90	64472.0
176.90	4535.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.80	507.0
36.10	503.0
37.00	3666.0
38.00	3309.0
39.00	1861.0
40.10	331.0
42.80	128.0
43.90	1238.0
44.90	532.0
45.70	196.0
46.30	194.0
47.00	1110.0
47.90	579.0
49.00	3509.0
50.00	15955.0
51.00	5292.0
51.90	283.0
52.70	116.0
55.00	268.0
56.00	1280.0
57.00	2282.0
58.00	182.0
60.00	863.0
61.00	3993.0
62.00	4474.0
63.00	3629.0
64.00	620.0
65.00	980.0
65.80	136.0
66.90	276.0
68.00	8303.0
69.00	8588.0
70.00	957.0
72.00	610.0
73.00	4168.0
74.00	14855.0
75.00	43880.0
76.00	3880.0
77.00	651.0
78.00	405.0
78.90	3429.0
79.90	1007.0
80.90	3997.0
81.90	898.0
82.90	153.0
85.80	200.0
86.90	4050.0
87.90	3873.0
90.90	555.0
92.00	2685.0
92.90	4174.0
94.00	10523.0
95.00	89712.0
96.00	5634.0
96.90	199.0
103.90	492.0
104.90	128.0
105.90	457.0
111.90	155.0
112.70	118.0
116.00	268.0
116.80	820.0
117.80	367.0
118.80	598.0
127.90	332.0
128.70	197.0
129.90	381.0
134.60	118.0
135.00	167.0
136.80	170.0
140.90	1112.0
141.80	163.0
142.80	1205.0
144.80	608.0
145.90	170.0
147.90	169.0
149.70	147.0
152.90	117.0
154.90	242.0
156.80	131.0
158.70	125.0
170.80	310.0
171.90	1099.0
172.90	969.0
173.90	71232.0
175.00	5518.0
175.90	68168.0
177.00	4346.0
178.00	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.90	535.0
37.00	3400.0
38.00	2947.0
39.00	1702.0
40.10	291.0
40.70	144.0
42.80	135.0
43.90	1242.0
44.90	537.0
45.70	165.0
47.00	1010.0
47.90	530.0
49.00	3272.0
50.00	14404.0
51.00	4883.0
51.90	211.0
52.70	114.0
53.80	124.0
55.00	232.0
56.00	1106.0
57.00	2059.0
58.00	158.0
60.00	804.0
61.00	3732.0
62.00	4235.0
63.00	3271.0
64.00	575.0
65.00	835.0
65.70	156.0
66.90	200.0
68.00	7763.0
69.00	7883.0
70.00	911.0
72.00	617.0
73.00	3510.0
74.00	14011.0
75.00	40040.0
76.00	3328.0
77.10	597.0
77.90	333.0
78.90	3212.0
79.90	1101.0
80.90	3717.0
81.90	880.0
82.80	191.0
85.80	241.0
86.90	3615.0
87.90	3680.0
90.80	517.0
91.90	2359.0
92.90	3817.0
94.00	9751.0
95.00	83264.0
96.00	5163.0
96.90	181.0
103.90	478.0
105.90	440.0
110.80	117.0
111.90	190.0
116.00	300.0
116.80	804.0
117.80	377.0
118.80	668.0
127.90	300.0
129.00	189.0
129.90	304.0
135.00	197.0
136.80	221.0
140.90	1023.0
141.80	152.0
142.80	1220.0
144.00	107.0
144.90	492.0
145.90	185.0
146.90	103.0
147.90	119.0
149.70	126.0
152.90	106.0
155.00	205.0
155.70	115.0
156.80	102.0
158.90	107.0
170.90	296.0
171.90	1036.0
172.90	892.0
173.90	67968.0
175.00	5330.0
175.90	65000.0
177.00	3987.0
178.00	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391