

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037728.D
 Acq On : 11 Oct 2024 14:05
 Operator : SY/MD
 Sample : P4346-07ME
 Misc : 3.76G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 14 06:18:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 06:04:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	932927	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	902482	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	443884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	316648	38.665	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	77.320%	
7) Chloroethane-d5	1.503	69	147958	23.275	ug/L	-0.03
Spiked Amount	50.000	Range 70 - 130	Recovery	=	46.560%#	
11) 1,1-Dichloroethene-d2	2.043	65	154361	45.115	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.220%	
21) 2-Butanone-d5	3.802	46	327980	112.438	ug/L	0.01
Spiked Amount	100.000	Range 40 - 130	Recovery	=	112.440%	
24) Chloroform-d	4.236	84	725230	49.775	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.540%	
26) 1,2-Dichloroethane-d4	4.934	65	449272	52.680	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.360%	
32) Benzene-d6	4.947	84	1443849	51.127	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.260%	
36) 1,2-Dichloropropane-d6	5.982	67	464681	51.674	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.340%	
41) Toluene-d8	7.236	98	1303276	50.894	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.780%	
43) trans-1,3-Dichloroprop...	7.548	79	210057	50.284	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	100.560%	
47) 2-Hexanone-d5	8.027	63	241098	126.969	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	126.970%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	551479	52.779	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	105.560%	
66) 1,2-Dichlorobenzene-d4	11.554	152	534941	57.191	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	114.380%	
Target Compounds						
					Qvalue	
39) cis-1,3-Dichloropropene	6.905	75	12660	1.128	ug/L #	62
48) 2-Hexanone	8.027	43	30394	6.830	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037728.D
Acq On : 11 Oct 2024 14:05
Operator : SY/MD
Sample : P4346-07ME
Misc : 3.76G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 14 06:18:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 06:04:26 2024
Response via : Initial Calibration

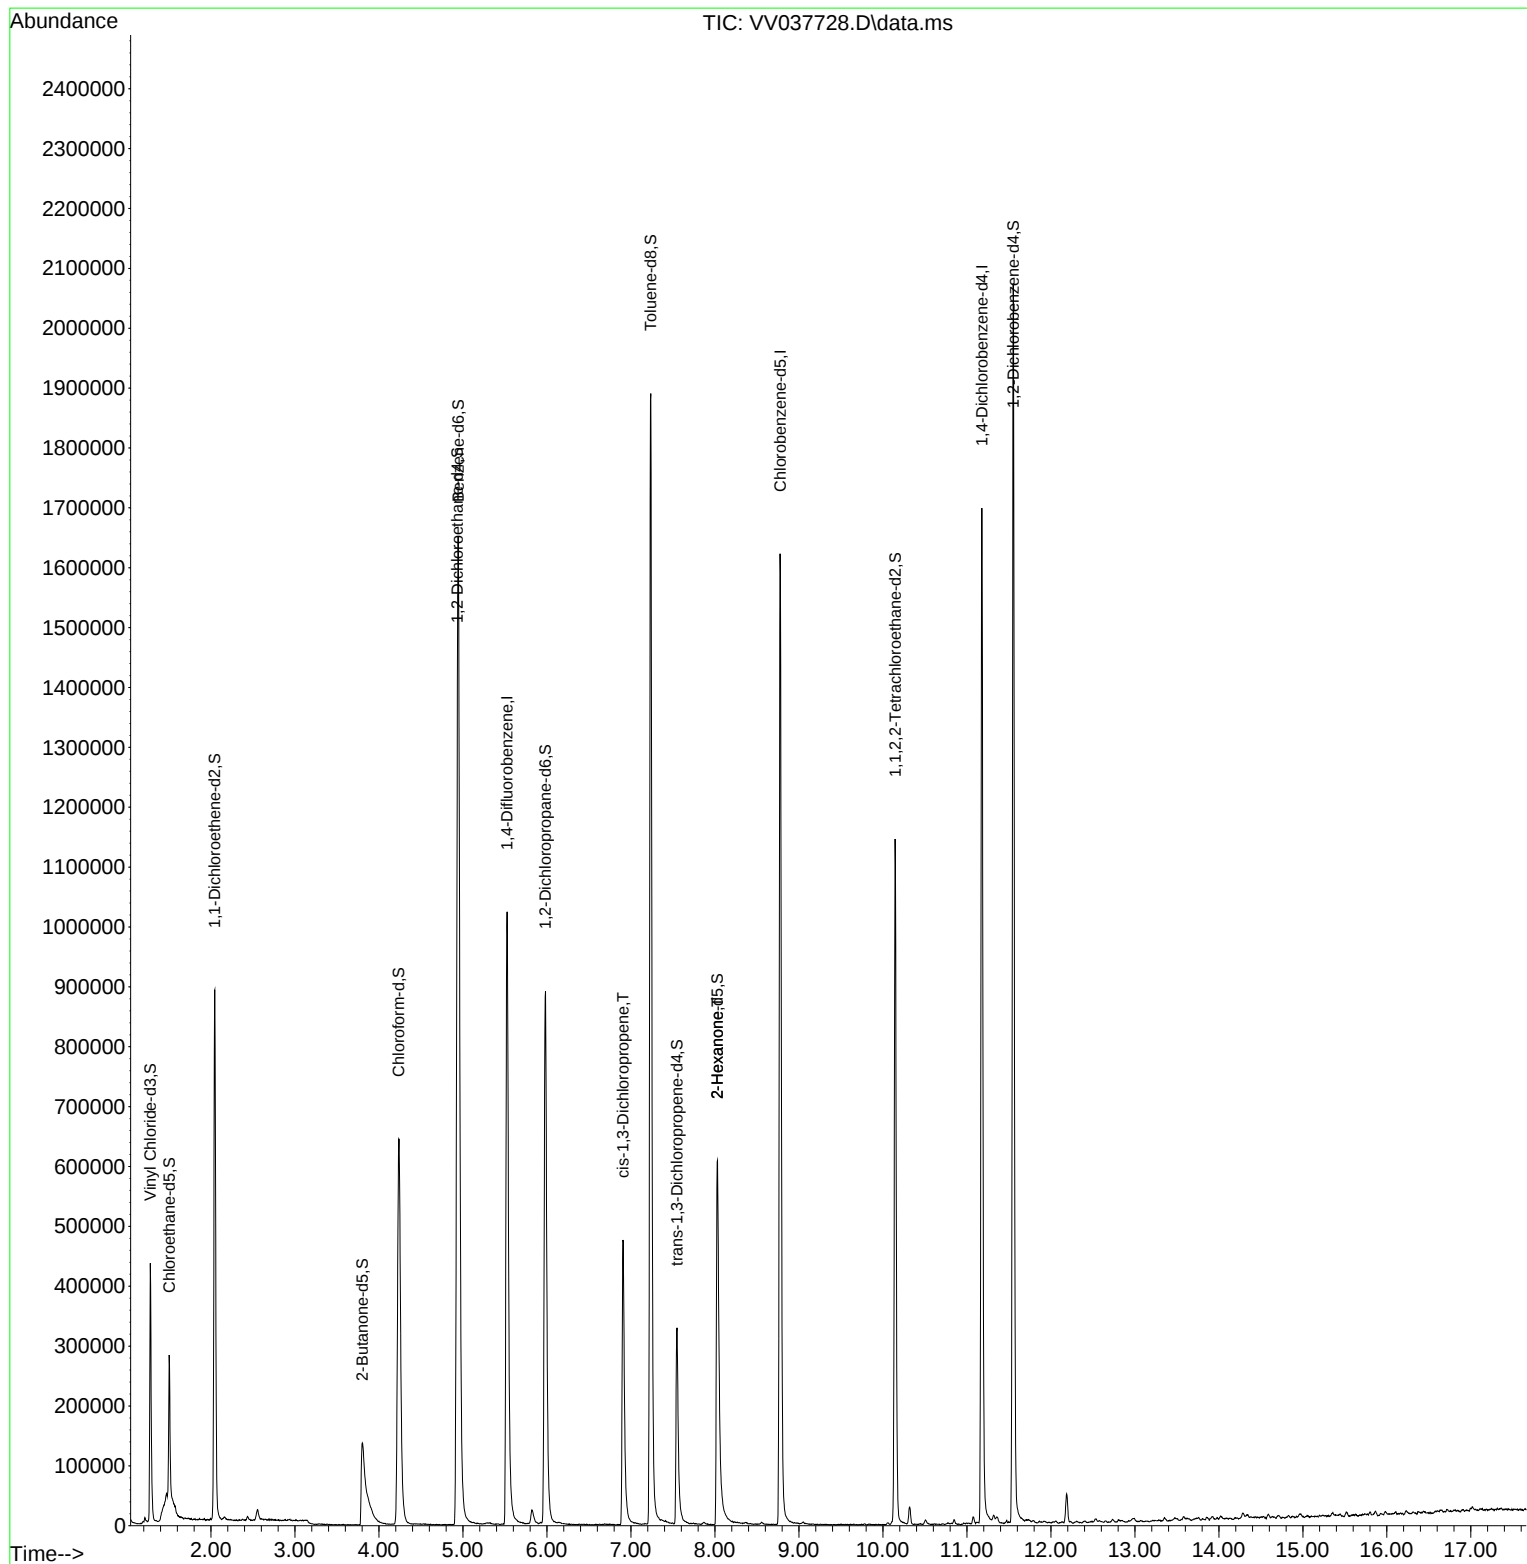

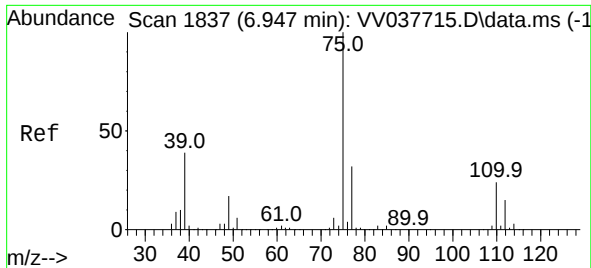

#39

cis-1,3-Dichloropropene

Concen: 1.128 ug/L

RT: 6.905 min Scan# 11

Delta R.T. -0.042 min

Lab File: VV037728.D

Acq: 11 Oct 2024 14:05

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 75 Resp: 12660

Ion Ratio Lower Upper

75 100

77 51.8 21.8 40.4#

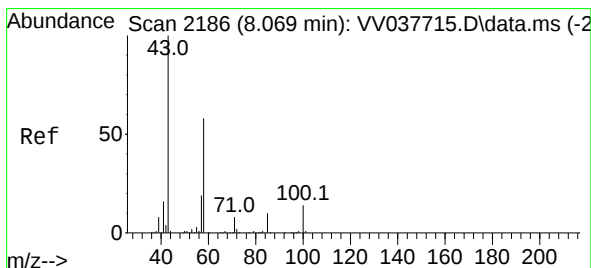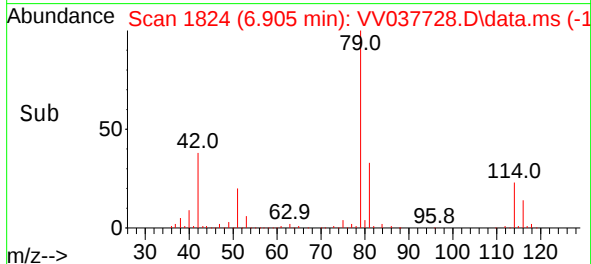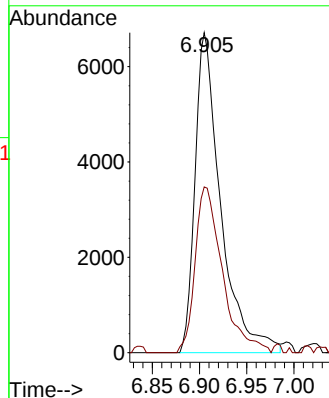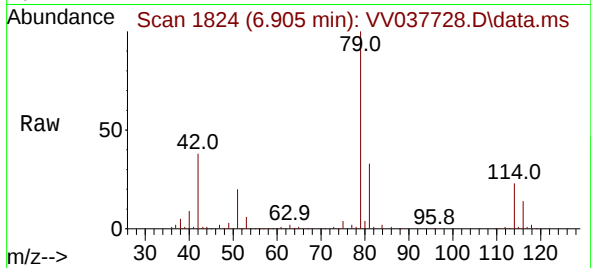

#48

2-Hexanone

Concen: 6.830 ug/L

RT: 8.027 min Scan# 2173

Delta R.T. -0.042 min

Lab File: VV037728.D

Acq: 11 Oct 2024 14:05

Tgt Ion: 43 Resp: 30394

Ion Ratio Lower Upper

43 100

58 39.9 46.5 69.7#

57 33.2 15.1 22.7#

100 1.7 10.7 16.1#

