




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037826.D
Acq On : 11 Oct 2024 13:22
Operator : SY/MD
Sample : P4346-11ME
Misc : 3.28G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAX1ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/14/2024
Supervised By :Mahesh Dadoda 10/14/2024

Quant Time: Oct 14 06:17:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 06:04:26 2024
Response via : Initial Calibration

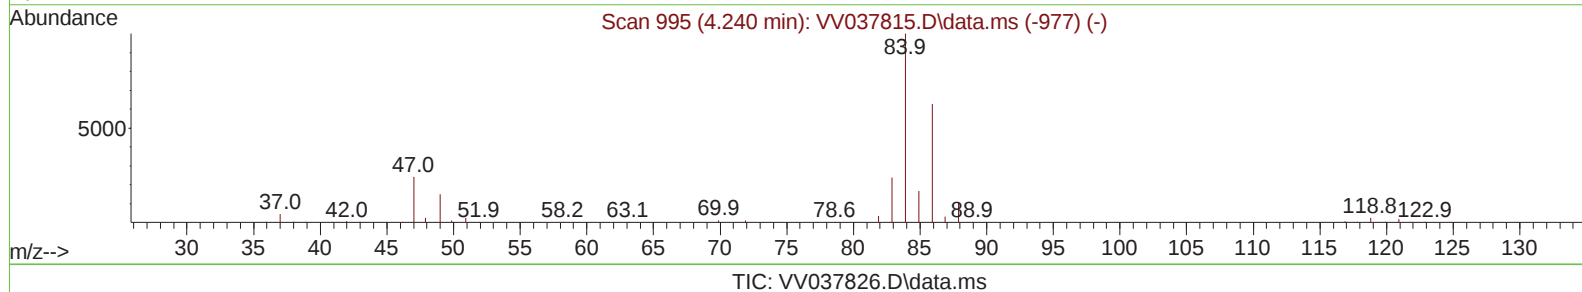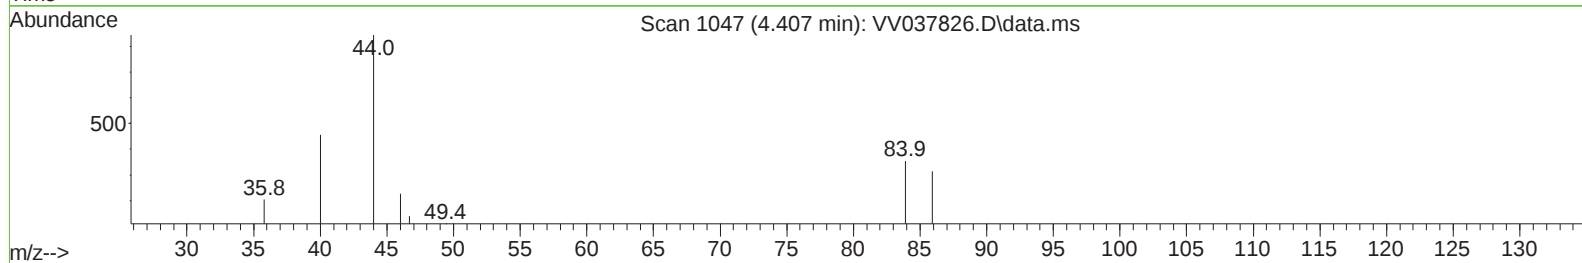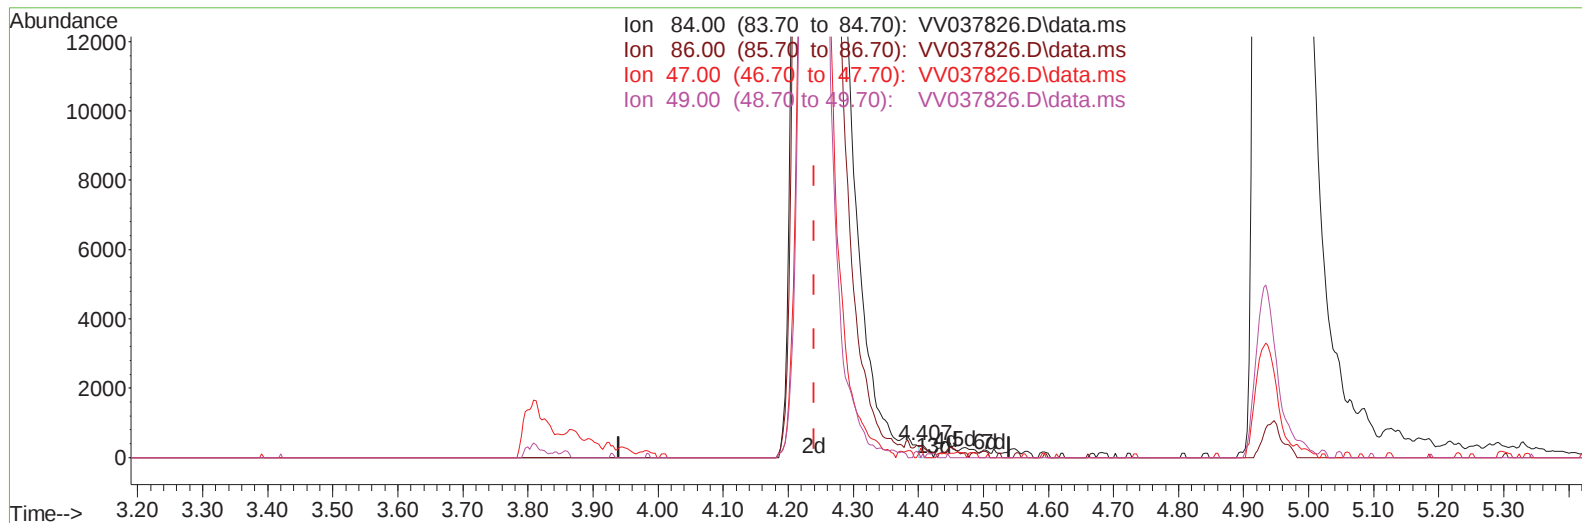

(24) Chloroform-d (S)

4.407min (+ 0.167) 0.03 ug/L

response 293

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	79.18
47.00	36.40	34.81
49.00	22.70	29.35




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037826.D
 Acq On : 11 Oct 2024 13:22
 Operator : SY/MD
 Sample : P4346-11ME
 Misc : 3.28G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAX1ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/14/2024
 Supervised By :Mahesh Dadoda 10/14/2024

Quant Time: Oct 14 06:17:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 06:04:26 2024
 Response via : Initial Calibration

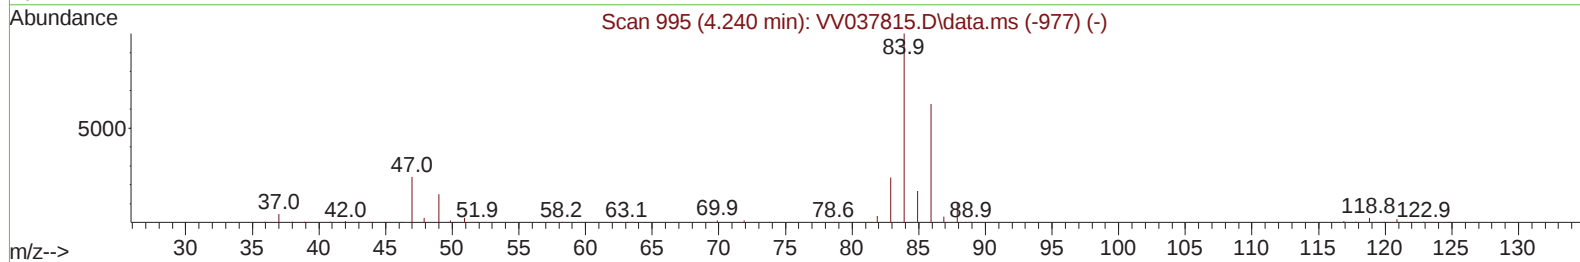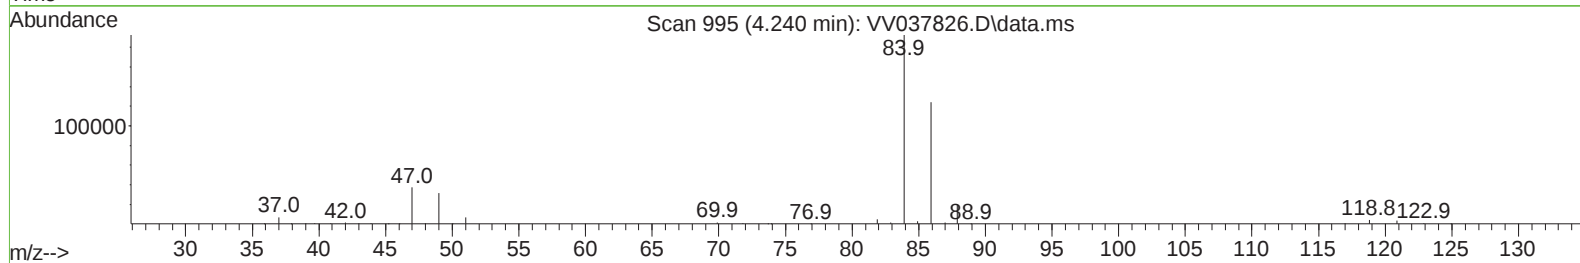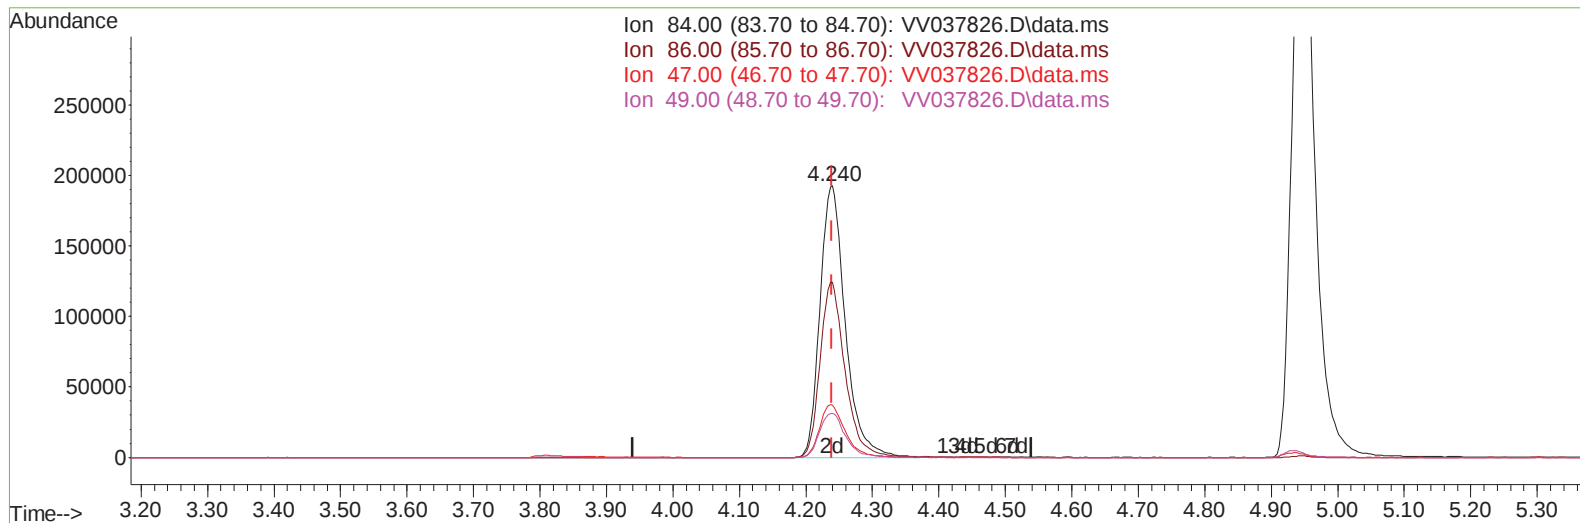

TIC: VV037826.D\data.ms

(24) Chloroform-d (S)

4.240min (-0.000) 56.37 ug/L m

response 508256

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.60	0.05#
47.00	36.40	0.02#
49.00	22.70	0.02#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037826.D
 Acq On : 11 Oct 2024 13:22
 Operator : SY/MD
 Sample : P4346-11ME
 Misc : 3.28G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAX1ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/14/2024
 Supervised By :Mahesh Dadoda 10/14/2024

Quant Time: Oct 14 06:17:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 06:04:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	577325	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	572082	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	276106	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	230388	45.459	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	90.920%	
7) Chloroethane-d5	1.503	69	93925	23.876	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130	Recovery	=	47.760%#	
11) 1,1-Dichloroethene-d2	2.044	65	108743	51.358	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	102.720%	
21) 2-Butanone-d5	3.806	46	191575	106.129	ug/L	0.02
Spiked Amount 100.000	Range 40	- 130	Recovery	=	106.130%	
24) Chloroform-d	4.240	84	508256m	56.369	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	112.740%	
26) 1,2-Dichloroethane-d4	4.931	65	318580	60.364	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	120.720%	
32) Benzene-d6	4.947	84	1015203	56.710	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	113.420%	
36) 1,2-Dichloropropane-d6	5.982	67	329560	57.814	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	115.620%	
41) Toluene-d8	7.236	98	900695	55.487	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	110.980%	
43) trans-1,3-Dichloroprop...	7.548	79	141918	53.593	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	107.180%	
47) 2-Hexanone-d5	8.030	63	166093	137.987	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	137.990%#	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	397678	60.041	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	120.080%#	
66) 1,2-Dichlorobenzene-d4	11.554	152	375474	64.535	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	129.080%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037826.D
Acq On : 11 Oct 2024 13:22
Operator : SY/MD
Sample : P4346-11ME
Misc : 3.28G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAX1ME

Manual IntegrationsAPPROVED

Quant Time: Oct 14 06:17:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 06:04:26 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/14/2024
Supervised By :Mahesh Dadoda 10/14/2024

