

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037820.D
 Acq On : 11 Oct 2024 11:13
 Operator : SY/MD
 Sample : P4352-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE0

Quant Time: Oct 14 06:16:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 06:04:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	606665	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	603167	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	273471	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	183602	34.476	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.960%		
7) Chloroethane-d5	1.532	69	163162	39.471	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.940%		
11) 1,1-Dichloroethene-d2	2.060	65	86534	38.892	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	77.780%		
21) 2-Butanone-d5	3.796	46	157267	82.909	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.910%		
24) Chloroform-d	4.243	84	409092	43.177	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.360%		
26) 1,2-Dichloroethane-d4	4.937	65	245676	44.299	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.600%		
32) Benzene-d6	4.953	84	784778	41.579	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.160%		
36) 1,2-Dichloropropane-d6	5.982	67	253973	42.257	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.520%		
41) Toluene-d8	7.236	98	685893	40.076	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	80.160%		
43) trans-1,3-Dichloroprop...	7.551	79	104671	37.490	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.980%		
47) 2-Hexanone-d5	8.024	63	93558	73.720	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	73.720%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	286371	41.008	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.020%		
66) 1,2-Dichlorobenzene-d4	11.551	152	274754	47.679	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.360%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	63145	33.958	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037820.D
Acq On : 11 Oct 2024 11:13
Operator : SY/MD
Sample : P4352-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE0

Quant Time: Oct 14 06:16:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 06:04:26 2024
Response via : Initial Calibration

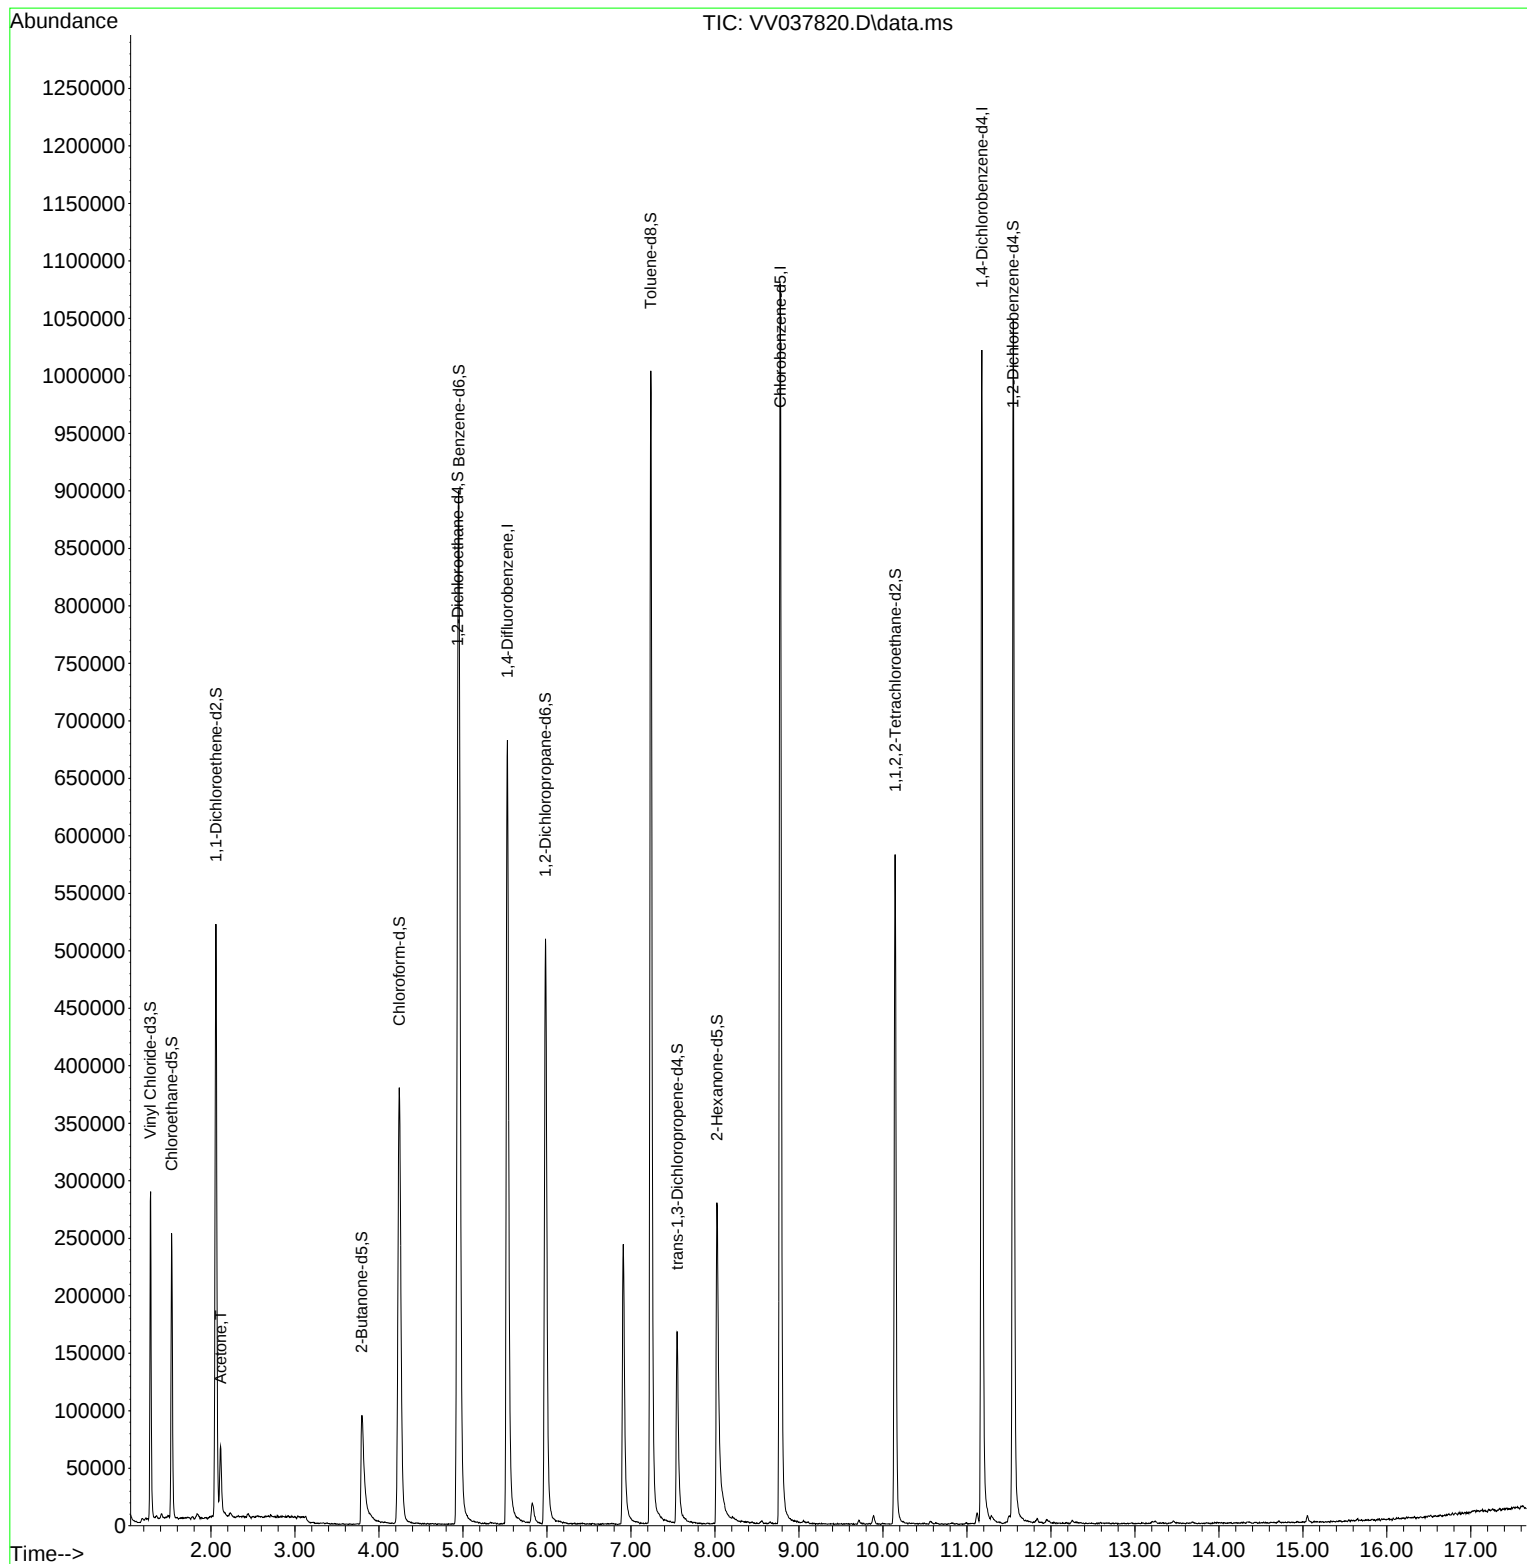

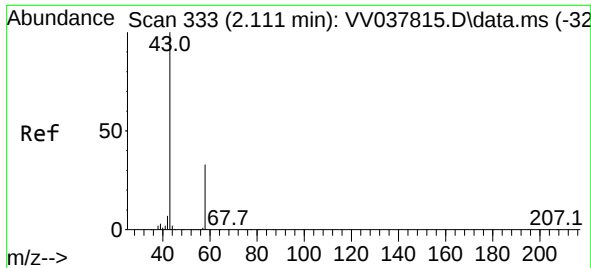

#13

Acetone

Concen: 33.958 ug/L

RT: 2.114 min Scan# 31

Delta R.T. 0.003 min

Lab File: VV037820.D


Acq: 11 Oct 2024 11:13

Instrument :

MSVOA_V

ClientSampleId :

A4FE0

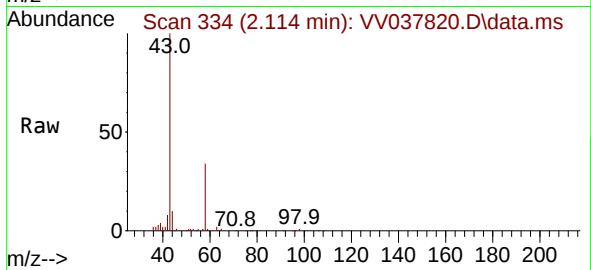

Tgt Ion: 43 Resp: 63145

Ion Ratio Lower Upper

43 100

58 33.8 0.0 66.6

