

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037817.D
 Acq On : 11 Oct 2024 10:00
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	91	rBV	302344	314892	13.17%	1.874%
2	1.532	146	153	171	rVB	279070	318920	13.34%	1.898%
3	2.060	308	317	341	rVB	547306	798771	33.42%	4.754%
4	3.491	761	762	763	rBV	425	131	0.01%	0.001%
5	3.568	784	786	791	rBV3	490	380	0.02%	0.002%
6	3.680	819	821	822	rBV	460	125	0.01%	0.001%
7	3.696	822	826	827	rVV	491	288	0.01%	0.002%
8	3.732	832	837	840	rBV2	789	629	0.03%	0.004%
9	3.796	849	857	893	rBV	99602	291674	12.20%	1.736%
10	4.243	976	996	1025	rBV	393130	1016651	42.53%	6.051%
11	4.561	1090	1095	1097	rBV2	917	839	0.04%	0.005%
12	4.645	1119	1121	1125	rBV3	622	405	0.02%	0.002%
13	4.667	1125	1128	1130	rBV	760	291	0.01%	0.002%
14	4.680	1130	1132	1133	rBV2	535	224	0.01%	0.001%
15	4.789	1163	1166	1168	rBV2	585	379	0.02%	0.002%
16	4.876	1191	1193	1197	rBV2	263	143	0.01%	0.001%
17	4.950	1197	1216	1250	rBV2	939898	2390430	100.00%	14.228%
18	5.272	1314	1316	1319	rBV2	964	549	0.02%	0.003%
19	5.465	1371	1376	1378	rBV5	592	563	0.02%	0.003%
20	5.529	1385	1396	1431	rBV	624488	1307686	54.71%	7.783%
21	5.982	1523	1537	1569	rBV	536869	1123145	46.99%	6.685%
22	6.230	1611	1614	1622	rVB4	1254	998	0.04%	0.006%
23	6.320	1639	1642	1646	rBV4	745	533	0.02%	0.003%
24	6.342	1646	1649	1654	rBV4	750	722	0.03%	0.004%
25	6.387	1659	1663	1664	rBV3	674	469	0.02%	0.003%
26	6.442	1675	1680	1683	rBV4	742	708	0.03%	0.004%
27	6.523	1703	1705	1708	rBV2	946	556	0.02%	0.003%
28	6.590	1722	1726	1729	rBV3	666	662	0.03%	0.004%
29	6.619	1733	1735	1738	rVB2	384	142	0.01%	0.001%
30	6.635	1738	1740	1742	rBV3	745	386	0.02%	0.002%
31	6.696	1756	1759	1763	rBV4	812	640	0.03%	0.004%
32	6.773	1780	1783	1787	rBV4	851	659	0.03%	0.004%
33	6.812	1792	1795	1799	rVB5	507	506	0.02%	0.003%
34	6.834	1799	1802	1806	rBV2	503	376	0.02%	0.002%
35	6.860	1809	1810	1811	rVB2	281	54	0.00%	0.000%
36	6.870	1811	1813	1814	rBV	616	181	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037817.D
 Acq On : 11 Oct 2024 10:00
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1815	1825	1850	rBV	255199	492947	20.62%	2.934%
38	7.236	1916	1927	1957	rBV	1040126	1831336	76.61%	10.900%
39	7.548	2016	2024	2042	rBV	171693	316852	13.26%	1.886%
40	7.908	2133	2136	2137	rBV3	1168	717	0.03%	0.004%
41	7.992	2160	2162	2164	rBV3	660	261	0.01%	0.002%
42	8.024	2164	2172	2204	rBV2	280637	623970	26.10%	3.714%
43	8.776	2394	2406	2436	rBV	1001423	1672450	69.96%	9.954%
44	9.220	2543	2544	2545	rBV2	621	205	0.01%	0.001%
45	9.272	2555	2560	2566	rBV3	879	1183	0.05%	0.007%
46	9.294	2566	2567	2572	rVV4	632	408	0.02%	0.002%
47	9.320	2572	2575	2580	rBV3	507	522	0.02%	0.003%
48	9.375	2588	2592	2593	rBV2	502	281	0.01%	0.002%
49	9.429	2605	2609	2612	rBV3	669	451	0.02%	0.003%
50	9.445	2612	2614	2617	rVB2	447	300	0.01%	0.002%
51	9.542	2640	2644	2646	rBV4	647	382	0.02%	0.002%
52	9.657	2678	2680	2683	rVB3	601	352	0.01%	0.002%
53	9.677	2683	2686	2689	rBV	605	398	0.02%	0.002%
54	9.702	2692	2694	2697	rVB2	862	334	0.01%	0.002%
55	9.744	2697	2707	2713	rVB5	838	998	0.04%	0.006%
56	9.770	2713	2715	2717	rBV2	230	129	0.01%	0.001%
57	9.793	2720	2722	2724	rBV2	303	117	0.00%	0.001%
58	9.805	2724	2726	2728	rBV	716	413	0.02%	0.002%
59	9.866	2741	2745	2747	rBV2	1041	687	0.03%	0.004%
60	9.924	2760	2763	2766	rBV3	738	599	0.03%	0.004%
61	9.979	2778	2780	2781	rBV3	150	41	0.00%	0.000%
62	10.085	2811	2813	2814	rVB	424	106	0.00%	0.001%
63	10.095	2814	2816	2817	rBV	230	100	0.00%	0.001%
64	10.146	2818	2832	2853	rBV	618460	985410	41.22%	5.865%
65	10.429	2919	2920	2922	rVB	219	60	0.00%	0.000%
66	10.445	2922	2925	2928	rBV2	695	506	0.02%	0.003%
67	10.490	2930	2939	2942	rBV5	1281	1488	0.06%	0.009%
68	10.538	2949	2954	2956	rBV4	852	633	0.03%	0.004%
69	10.619	2977	2979	2982	rBV3	621	366	0.02%	0.002%
70	10.661	2988	2992	2994	rBV3	570	300	0.01%	0.002%
71	10.744	3015	3018	3021	rBV2	466	459	0.02%	0.003%
72	10.818	3038	3041	3043	rBV2	548	377	0.02%	0.002%
73	10.921	3070	3073	3076	rVB3	811	542	0.02%	0.003%
74	10.982	3091	3092	3096	rVB	367	165	0.01%	0.001%
75	10.998	3096	3097	3100	rVB	308	124	0.01%	0.001%
76	11.018	3100	3103	3105	rBV2	549	323	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037817.D
 Acq On : 11 Oct 2024 10:00
 Operator : SY/MD
 Sample : VV1011WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK241

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.056	3112	3115	3116	rBV	425	241	0.01%	0.001%
78	11.098	3126	3128	3130	rBV2	402	216	0.01%	0.001%
79	11.127	3131	3137	3139	rBV5	1867	1769	0.07%	0.011%
80	11.178	3142	3153	3187	rVV	941070	1528434	63.94%	9.097%
81	11.551	3258	3269	3301	rBV	1072896	1729148	72.34%	10.292%
82	11.837	3355	3358	3360	rBV5	1263	739	0.03%	0.004%
83	12.124	3444	3447	3451	rVB3	928	574	0.02%	0.003%
84	12.140	3451	3452	3456	rBV	490	309	0.01%	0.002%
85	12.317	3504	3507	3509	rBV2	545	313	0.01%	0.002%
86	12.458	3548	3551	3554	rVB3	728	403	0.02%	0.002%
87	12.590	3587	3592	3594	rBV4	2058	1914	0.08%	0.011%
88	12.860	3674	3676	3679	rBV	673	361	0.02%	0.002%
89	12.886	3682	3684	3686	rBV2	541	281	0.01%	0.002%
90	13.210	3779	3785	3786	rBV4	3242	3193	0.13%	0.019%
91	13.448	3853	3859	3871	rBV5	6475	12290	0.51%	0.073%
92	13.683	3926	3932	3947	rVB9	4762	8933	0.37%	0.053%




Sum of corrected areas: 16801117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037817.D
Acq On : 11 Oct 2024 10:00
Operator : SY/MD
Sample : VV1011WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

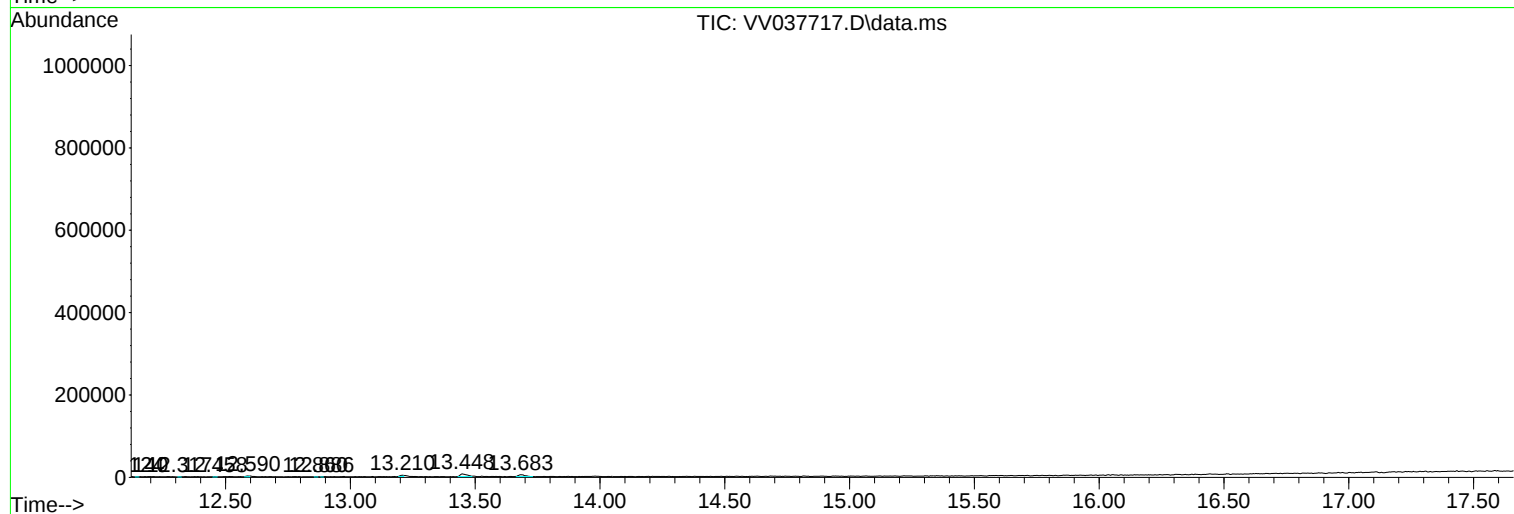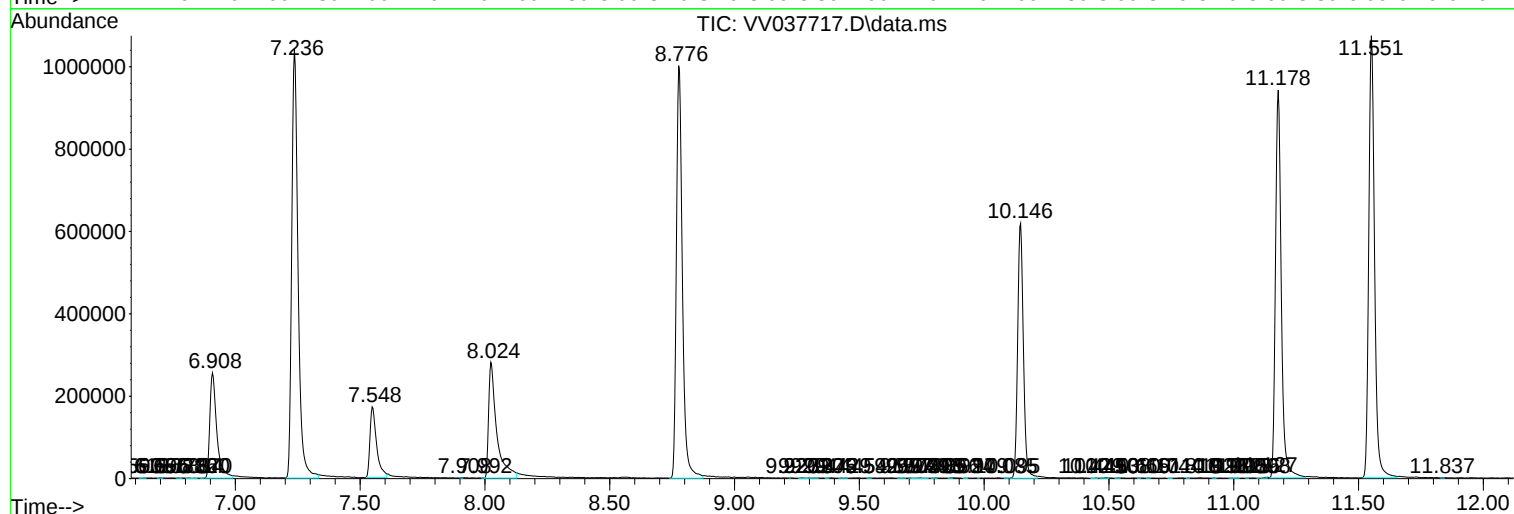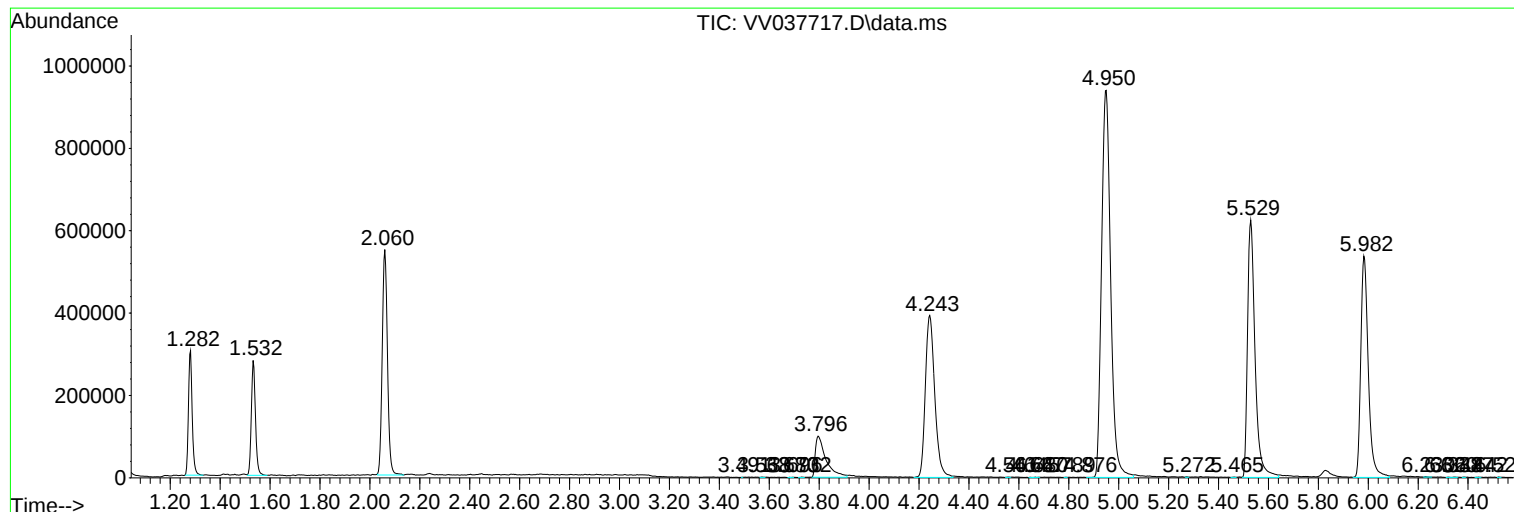

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037817.D
Acq On : 11 Oct 2024 10:00
Operator : SY/MD
Sample : VV1011WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037817.D
Acq On : 11 Oct 2024 10:00
Operator : SY/MD
Sample : VV1011WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK241

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc