

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037819.D
 Acq On : 11 Oct 2024 10:51
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037719.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.221	50	56	64	rBV	36236	37876	1.79%	0.254%
2	1.278	68	74	88	rVB	262903	280267	13.24%	1.877%
3	1.532	146	153	169	rVB	244600	282498	13.35%	1.892%
4	2.060	308	317	327	rBV	487652	693111	32.74%	4.643%
5	3.468	752	755	758	rBV2	603	372	0.02%	0.002%
6	3.487	758	761	765	rBV2	626	642	0.03%	0.004%
7	3.542	776	778	780	rVB2	462	225	0.01%	0.002%
8	3.568	780	786	787	rBV2	627	483	0.02%	0.003%
9	3.667	815	817	819	rBV	524	350	0.02%	0.002%
10	3.690	822	824	826	rBV	268	141	0.01%	0.001%
11	3.745	838	841	846	rVB3	488	389	0.02%	0.003%
12	3.799	849	858	899	rBV	87259	278349	13.15%	1.864%
13	4.240	978	995	1028	rBV	351240	895130	42.29%	5.996%
14	4.571	1096	1098	1100	rBV	330	149	0.01%	0.001%
15	4.581	1100	1101	1105	rVB2	612	346	0.02%	0.002%
16	4.619	1111	1113	1116	rVB3	434	234	0.01%	0.002%
17	4.648	1120	1122	1125	rVV	426	247	0.01%	0.002%
18	4.667	1125	1128	1132	rVB3	958	701	0.03%	0.005%
19	4.690	1132	1135	1137	rBV2	374	257	0.01%	0.002%
20	4.725	1143	1146	1151	rBV4	541	592	0.03%	0.004%
21	4.745	1151	1152	1156	rVB2	414	243	0.01%	0.002%
22	4.812	1171	1173	1180	rBV4	757	693	0.03%	0.005%
23	4.863	1180	1189	1194	rBV4	801	1123	0.05%	0.008%
24	4.896	1197	1199	1200	rBV2	543	252	0.01%	0.002%
25	4.947	1200	1215	1248	rBV2	836214	2116727	100.00%	14.178%
26	5.455	1370	1373	1375	rBV3	631	394	0.02%	0.003%
27	5.490	1379	1384	1385	rBV4	1261	913	0.04%	0.006%
28	5.529	1385	1396	1431	rBV	563188	1173228	55.43%	7.858%
29	5.982	1522	1537	1568	rBV	472896	980913	46.34%	6.570%
30	6.397	1663	1666	1670	rBV4	1323	1086	0.05%	0.007%
31	6.416	1670	1672	1675	rVV2	614	374	0.02%	0.003%
32	6.452	1681	1683	1685	rVB3	604	245	0.01%	0.002%
33	6.490	1694	1695	1697	rVB	435	102	0.00%	0.001%
34	6.507	1697	1700	1702	rBV5	801	547	0.03%	0.004%
35	6.519	1702	1704	1707	rVB	702	432	0.02%	0.003%
36	6.616	1733	1734	1736	rBV2	417	229	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037819.D
 Acq On : 11 Oct 2024 10:51
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.703	1759	1761	1762	rBV	344	155	0.01%	0.001%
38	6.722	1765	1767	1769	rVB	348	132	0.01%	0.001%
39	6.735	1769	1771	1774	rBV3	531	271	0.01%	0.002%
40	6.770	1779	1782	1786	rBV3	775	522	0.02%	0.003%
41	6.908	1813	1825	1860	rBV	228614	455567	21.52%	3.051%
42	7.236	1917	1927	1958	rBV	923013	1635756	77.28%	10.957%
43	7.548	2016	2024	2052	rBV	150792	290828	13.74%	1.948%
44	8.024	2164	2172	2209	rBV2	254817	584018	27.59%	3.912%
45	8.625	2355	2359	2361	rBV3	818	659	0.03%	0.004%
46	8.699	2381	2382	2384	rBV	483	178	0.01%	0.001%
47	8.777	2396	2406	2440	rBV	889533	1492655	70.52%	9.998%
48	9.182	2530	2532	2535	rBV4	563	346	0.02%	0.002%
49	9.201	2536	2538	2541	rVB2	743	334	0.02%	0.002%
50	9.301	2567	2569	2572	rVB3	746	422	0.02%	0.003%
51	9.362	2585	2588	2589	rBV3	615	296	0.01%	0.002%
52	9.404	2595	2601	2603	rBV4	898	801	0.04%	0.005%
53	9.445	2610	2614	2615	rBV	681	446	0.02%	0.003%
54	9.452	2615	2616	2618	rVB2	811	266	0.01%	0.002%
55	9.555	2642	2648	2649	rBV5	515	427	0.02%	0.003%
56	9.613	2663	2666	2669	rVB3	642	416	0.02%	0.003%
57	9.629	2669	2671	2672	rBV	282	100	0.00%	0.001%
58	9.719	2693	2699	2702	rBV6	2409	2887	0.14%	0.019%
59	9.995	2779	2785	2788	rBV4	1336	1531	0.07%	0.010%
60	10.047	2797	2801	2803	rBV4	598	371	0.02%	0.002%
61	10.066	2803	2807	2809	rVB2	599	461	0.02%	0.003%
62	10.104	2817	2819	2821	rBV3	885	447	0.02%	0.003%
63	10.146	2821	2832	2857	rVV	531997	848205	40.07%	5.681%
64	10.429	2917	2920	2925	rBV5	597	505	0.02%	0.003%
65	10.545	2952	2956	2958	rBV3	646	504	0.02%	0.003%
66	10.638	2981	2985	2989	rVB5	1120	895	0.04%	0.006%
67	10.748	3016	3019	3022	rBV3	643	424	0.02%	0.003%
68	10.857	3050	3053	3057	rBV4	860	684	0.03%	0.005%
69	10.918	3069	3072	3075	rBV2	782	557	0.03%	0.004%
70	10.937	3075	3078	3082	rVB4	789	619	0.03%	0.004%
71	10.963	3082	3086	3088	rBV2	613	425	0.02%	0.003%
72	11.178	3143	3153	3184	rBV	828461	1343044	63.45%	8.996%
73	11.551	3259	3269	3293	rVB	956794	1506916	71.19%	10.094%
74	12.159	3451	3458	3462	rBV6	1101	1569	0.07%	0.011%
75	12.796	3654	3656	3660	rBV4	781	538	0.03%	0.004%
76	12.998	3717	3719	3721	rBV	597	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037819.D
Acq On : 11 Oct 2024 10:51
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	13.043	3731	3733	3735	rBV2	928	518	0.02%	0.003%
78	13.294	3808	3811	3816	rBV5	861	1032	0.05%	0.007%
79	13.342	3824	3826	3827	rBV	555	220	0.01%	0.001%
80	14.275	4112	4116	4118	rBV3	1671	1498	0.07%	0.010%
81	14.329	4130	4133	4135	rBV2	1356	950	0.04%	0.006%




Sum of corrected areas: 14929480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037819.D
Acq On : 11 Oct 2024 10:51
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

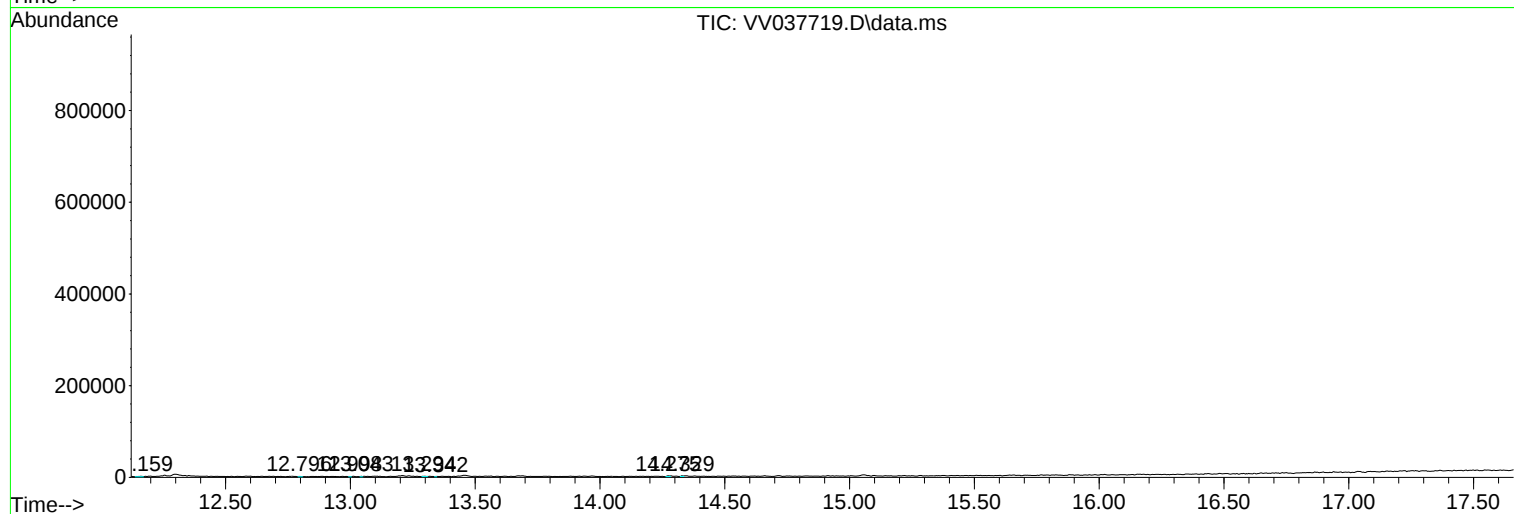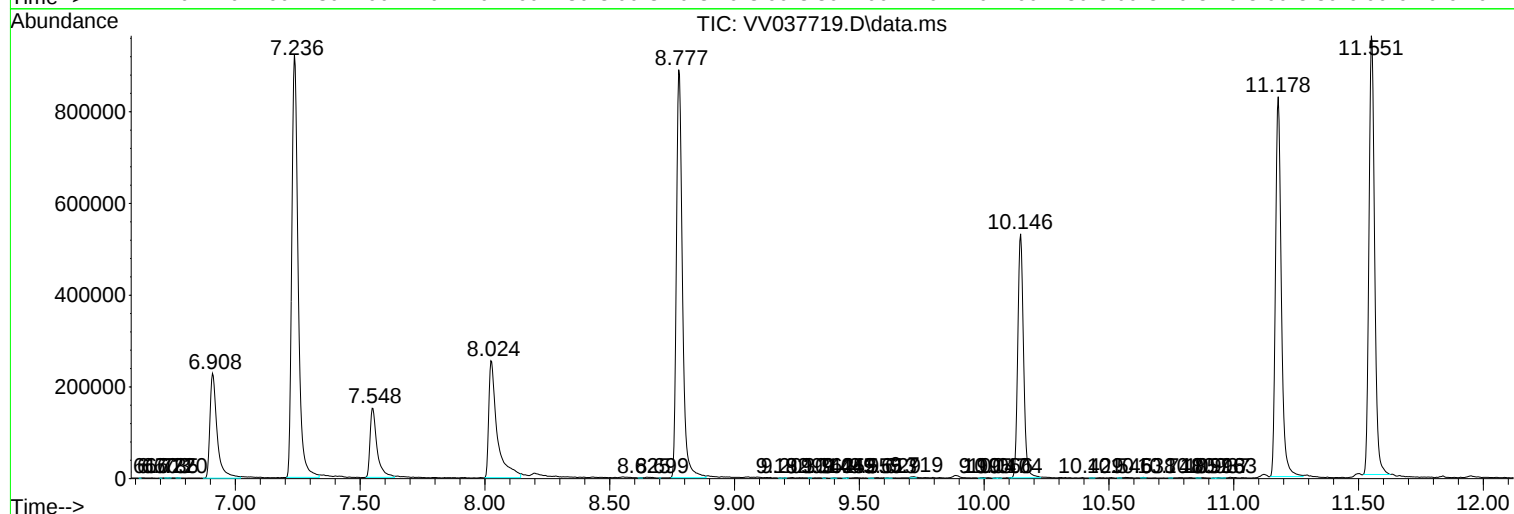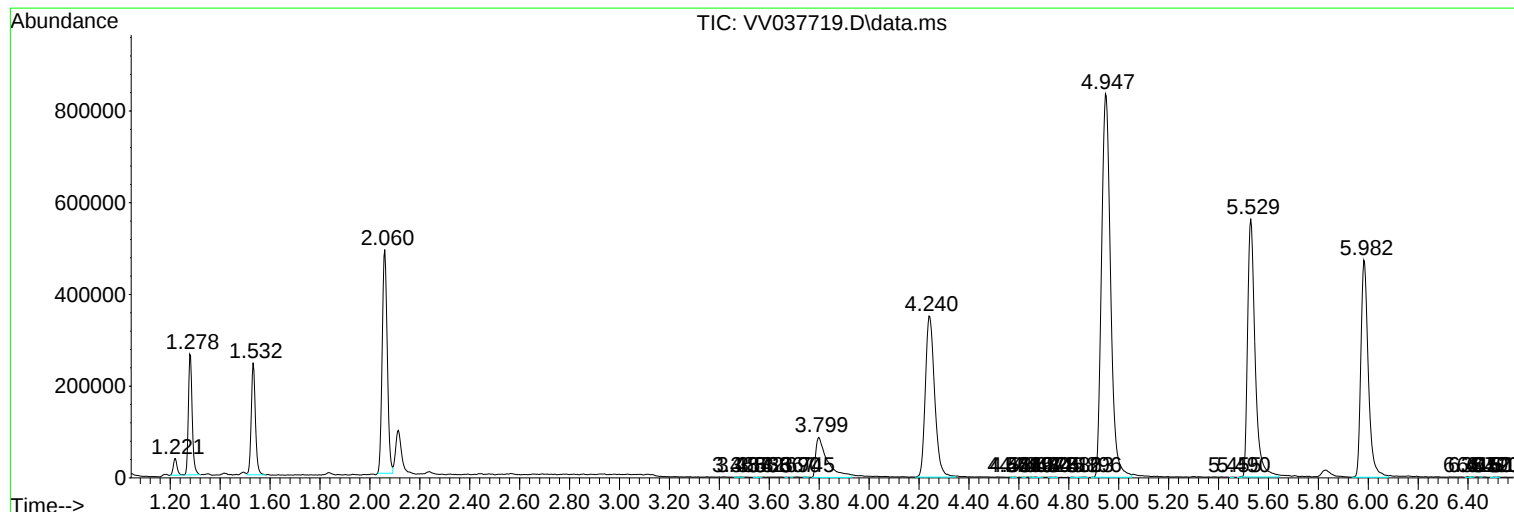

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037819.D
Acq On : 11 Oct 2024 10:51
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037819.D
Acq On : 11 Oct 2024 10:51
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc