

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037820.D
 Acq On : 11 Oct 2024 11:13
 Operator : SY/MD
 Sample : P4352-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rBV	284316	296029	13.01%	1.778%
2	1.532	146	153	168	rVB	247454	289849	12.74%	1.741%
3	2.060	308	317	327	rBV	512502	730462	32.11%	4.388%
4	3.468	753	755	757	rBV	635	282	0.01%	0.002%
5	3.529	772	774	778	rVB3	379	172	0.01%	0.001%
6	3.648	808	811	814	rBV3	758	580	0.03%	0.003%
7	3.796	849	857	886	rBV	94420	269933	11.87%	1.622%
8	4.243	981	996	1026	rBV	377951	951431	41.83%	5.715%
9	4.516	1079	1081	1084	rBV2	813	545	0.02%	0.003%
10	4.542	1087	1089	1093	rVV4	700	398	0.02%	0.002%
11	4.606	1105	1109	1110	rBV3	438	243	0.01%	0.001%
12	4.632	1115	1117	1118	rBV2	425	193	0.01%	0.001%
13	4.671	1126	1129	1134	rVB4	963	824	0.04%	0.005%
14	4.699	1134	1138	1139	rBV2	445	266	0.01%	0.002%
15	4.716	1139	1143	1146	rVV4	478	387	0.02%	0.002%
16	4.748	1151	1153	1157	rVV2	427	334	0.01%	0.002%
17	4.828	1174	1178	1179	rBV3	613	351	0.02%	0.002%
18	4.867	1188	1190	1192	rBV2	359	194	0.01%	0.001%
19	4.896	1196	1199	1200	rBV2	689	347	0.02%	0.002%
20	4.950	1200	1216	1247	rBV2	898671	2274595	100.00%	13.664%
21	5.294	1321	1323	1327	rVB2	468	248	0.01%	0.001%
22	5.410	1355	1359	1363	rVB3	673	584	0.03%	0.004%
23	5.436	1366	1367	1370	rBV3	463	205	0.01%	0.001%
24	5.452	1370	1372	1373	rBV	564	220	0.01%	0.001%
25	5.462	1373	1375	1378	rBV4	446	215	0.01%	0.001%
26	5.490	1380	1384	1385	rBV3	782	501	0.02%	0.003%
27	5.529	1385	1396	1428	rBV	681271	1409983	61.99%	8.470%
28	5.825	1481	1488	1510	rVB4	17175	40110	1.76%	0.241%
29	5.982	1524	1537	1564	rBV	509006	1059196	46.57%	6.363%
30	6.310	1636	1639	1642	rBV2	926	649	0.03%	0.004%
31	6.368	1655	1657	1660	rBV4	687	458	0.02%	0.003%
32	6.407	1667	1669	1673	rBV4	659	531	0.02%	0.003%
33	6.461	1683	1686	1688	rBV3	371	245	0.01%	0.001%
34	6.542	1707	1711	1716	rBV7	863	1071	0.05%	0.006%
35	6.613	1731	1733	1735	rVB2	547	255	0.01%	0.002%
36	6.638	1740	1741	1744	rBV3	554	290	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037820.D
 Acq On : 11 Oct 2024 11:13
 Operator : SY/MD
 Sample : P4352-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.667	1744	1750	1753	rBV5	828	762	0.03%	0.005%
38	6.693	1753	1758	1760	rBV5	483	440	0.02%	0.003%
39	6.725	1765	1768	1771	rBV3	721	602	0.03%	0.004%
40	6.757	1775	1778	1780	rBV3	387	214	0.01%	0.001%
41	6.773	1780	1783	1786	rVV2	724	429	0.02%	0.003%
42	6.822	1797	1798	1802	rVB3	629	246	0.01%	0.001%
43	6.863	1805	1811	1812	rBV4	627	478	0.02%	0.003%
44	6.908	1815	1825	1859	rBV	243234	481535	21.17%	2.893%
45	7.114	1887	1889	1890	rBV2	769	255	0.01%	0.002%
46	7.236	1917	1927	1956	rBV	1001997	1774711	78.02%	10.661%
47	7.548	2016	2024	2044	rBV	165867	307777	13.53%	1.849%
48	8.024	2164	2172	2218	rBV2	278999	654313	28.77%	3.930%
49	8.725	2388	2390	2392	rBV2	578	203	0.01%	0.001%
50	8.776	2395	2406	2441	rBV	1078721	1809415	79.55%	10.869%
51	9.211	2538	2541	2543	rBV2	551	407	0.02%	0.002%
52	9.243	2547	2551	2554	rVV5	718	561	0.02%	0.003%
53	9.268	2557	2559	2561	rVB2	813	361	0.02%	0.002%
54	9.349	2581	2584	2585	rBV	371	203	0.01%	0.001%
55	9.378	2592	2593	2595	rBV2	461	201	0.01%	0.001%
56	9.410	2601	2603	2605	rVB2	948	407	0.02%	0.002%
57	9.429	2608	2609	2611	rVV	351	149	0.01%	0.001%
58	9.458	2615	2618	2620	rVB2	733	352	0.02%	0.002%
59	9.532	2637	2641	2643	rBV3	742	454	0.02%	0.003%
60	9.548	2644	2646	2649	rVV3	456	260	0.01%	0.002%
61	9.593	2657	2660	2663	rVB3	859	526	0.02%	0.003%
62	9.609	2663	2665	2666	rBV2	430	192	0.01%	0.001%
63	9.648	2675	2677	2680	rVB3	884	463	0.02%	0.003%
64	9.715	2691	2698	2706	rBV8	3766	5772	0.25%	0.035%
65	9.802	2721	2725	2728	rBV4	750	600	0.03%	0.004%
66	9.838	2731	2736	2737	rVV5	878	631	0.03%	0.004%
67	9.889	2741	2752	2763	rBV5	7557	13377	0.59%	0.080%
68	9.957	2771	2773	2774	rBV	337	192	0.01%	0.001%
69	9.985	2779	2782	2784	rBV2	737	511	0.02%	0.003%
70	10.082	2810	2812	2816	rBV3	409	341	0.01%	0.002%
71	10.146	2820	2832	2859	rVV	581999	934633	41.09%	5.614%
72	10.317	2879	2885	2888	rBV6	1074	1354	0.06%	0.008%
73	10.439	2917	2923	2925	rBV4	812	860	0.04%	0.005%
74	10.497	2937	2941	2944	rBV4	917	642	0.03%	0.004%
75	10.564	2956	2962	2965	rBV4	2763	3265	0.14%	0.020%
76	10.690	2998	3001	3003	rBV	642	392	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037820.D
 Acq On : 11 Oct 2024 11:13
 Operator : SY/MD
 Sample : P4352-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.744	3011	3018	3021	rVB4	553	626	0.03%	0.004%
78	10.770	3024	3026	3028	rBV4	408	201	0.01%	0.001%
79	10.780	3028	3029	3034	rBV4	482	360	0.02%	0.002%
80	10.876	3055	3059	3066	rVB5	819	973	0.04%	0.006%
81	10.921	3070	3073	3074	rBV	413	274	0.01%	0.002%
82	10.960	3081	3085	3086	rBV4	472	285	0.01%	0.002%
83	10.992	3092	3095	3096	rBV2	1015	566	0.02%	0.003%
84	11.124	3127	3136	3142	rBV9	9404	15129	0.67%	0.091%
85	11.178	3143	3153	3184	rVV	1018724	1621781	71.30%	9.742%
86	11.551	3259	3269	3299	rVB	1042107	1650078	72.54%	9.912%
87	12.034	3417	3419	3422	rBV4	1005	508	0.02%	0.003%
88	12.214	3473	3475	3479	rVB3	875	540	0.02%	0.003%
89	12.252	3479	3487	3497	rBV3	3157	6003	0.26%	0.036%
90	12.593	3587	3593	3595	rBV5	1404	1468	0.06%	0.009%
91	12.805	3656	3659	3665	rBV3	912	953	0.04%	0.006%
92	12.844	3669	3671	3673	rVB	595	261	0.01%	0.002%
93	13.079	3742	3744	3747	rBV3	769	478	0.02%	0.003%
94	13.130	3758	3760	3764	rVB4	565	289	0.01%	0.002%
95	13.497	3872	3874	3876	rBV3	923	487	0.02%	0.003%
96	13.619	3907	3912	3917	rBV5	1172	1476	0.06%	0.009%
97	13.905	3999	4001	4005	rBV4	752	622	0.03%	0.004%
98	14.059	4046	4049	4056	rBV7	979	1151	0.05%	0.007%
99	14.484	4180	4181	4186	rBV5	858	415	0.02%	0.002%
100	15.053	4353	4358	4375	rVB5	6447	11528	0.51%	0.069%




Sum of corrected areas: 16647114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037820.D
Acq On : 11 Oct 2024 11:13
Operator : SY/MD
Sample : P4352-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

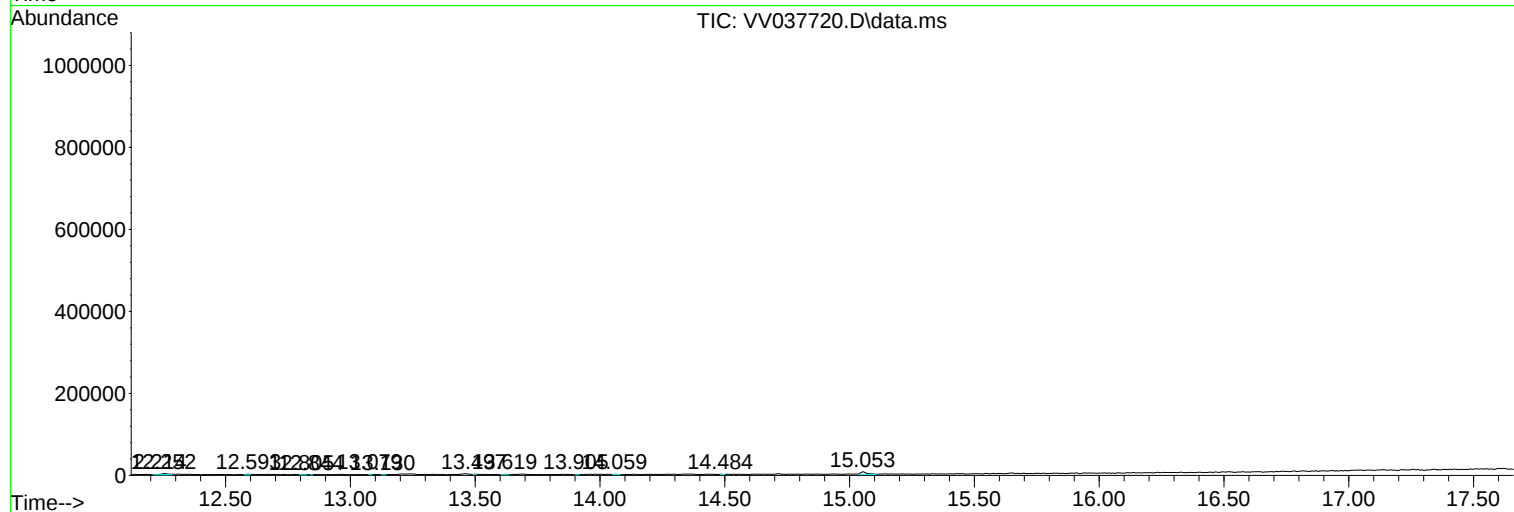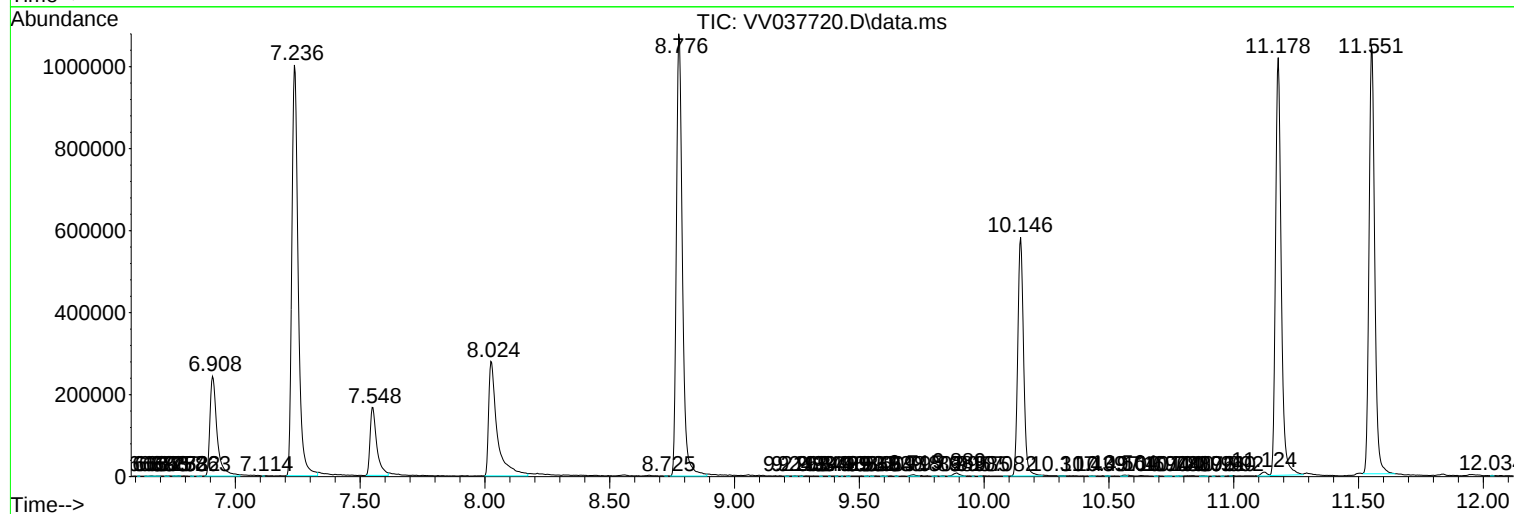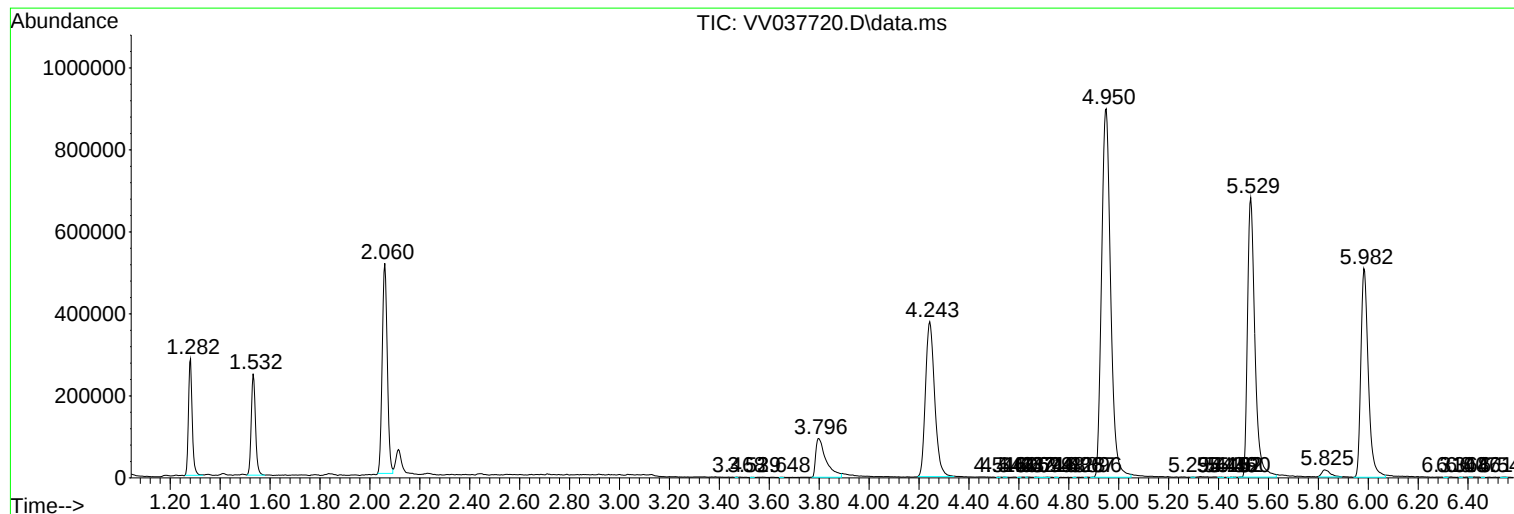

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037820.D
Acq On : 11 Oct 2024 11:13
Operator : SY/MD
Sample : P4352-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037820.D
Acq On : 11 Oct 2024 11:13
Operator : SY/MD
Sample : P4352-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc