

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037821.D
 Acq On : 11 Oct 2024 11:35
 Operator : SY/MD
 Sample : P4379-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	274951	291042	12.77%	1.759%
2	1.532	146	153	169	rVB	246846	292090	12.82%	1.766%
3	2.060	307	317	330	rBV	507918	732197	32.14%	4.426%
4	3.462	749	753	754	rBV2	684	429	0.02%	0.003%
5	3.606	796	798	801	rBV2	324	224	0.01%	0.001%
6	3.796	849	857	899	rBV	96272	292678	12.85%	1.769%
7	4.243	982	996	1027	rVB	367777	932206	40.92%	5.635%
8	4.658	1121	1125	1126	rBV	737	489	0.02%	0.003%
9	4.670	1127	1129	1131	rVV3	544	249	0.01%	0.002%
10	4.709	1139	1141	1142	rBV2	290	69	0.00%	0.000%
11	4.757	1154	1156	1160	rBV3	310	156	0.01%	0.001%
12	4.825	1174	1177	1182	rBV4	677	616	0.03%	0.004%
13	4.844	1182	1183	1186	rVB	290	99	0.00%	0.001%
14	4.860	1186	1188	1189	rBV	258	72	0.00%	0.000%
15	4.870	1189	1191	1197	rVB4	785	805	0.04%	0.005%
16	4.947	1197	1215	1253	rBV2	902774	2278218	100.00%	13.772%
17	5.275	1315	1317	1318	rBV2	601	276	0.01%	0.002%
18	5.529	1385	1396	1430	rBV	691129	1433053	62.90%	8.663%
19	5.982	1525	1537	1565	rBV	503060	1046186	45.92%	6.324%
20	6.304	1632	1637	1638	rBV3	893	670	0.03%	0.004%
21	6.362	1650	1655	1658	rBV3	1360	987	0.04%	0.006%
22	6.445	1678	1681	1682	rBV2	719	270	0.01%	0.002%
23	6.484	1688	1693	1695	rVB5	544	477	0.02%	0.003%
24	6.503	1695	1699	1701	rBV2	758	530	0.02%	0.003%
25	6.532	1705	1708	1709	rBV2	702	359	0.02%	0.002%
26	6.580	1719	1723	1725	rBV3	776	550	0.02%	0.003%
27	6.616	1730	1734	1737	rBV4	588	485	0.02%	0.003%
28	6.632	1737	1739	1743	rVV4	371	178	0.01%	0.001%
29	6.677	1749	1753	1754	rBV	530	321	0.01%	0.002%
30	6.686	1754	1756	1760	rBV4	437	294	0.01%	0.002%
31	6.709	1761	1763	1764	rBV2	952	309	0.01%	0.002%
32	6.735	1769	1771	1773	rBV	661	327	0.01%	0.002%
33	6.841	1802	1804	1809	rBV2	662	534	0.02%	0.003%
34	6.867	1809	1812	1814	rBV4	347	210	0.01%	0.001%
35	6.908	1815	1825	1857	rBV	245228	482678	21.19%	2.918%
36	7.236	1916	1927	1958	rBV	990192	1768361	77.62%	10.690%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037821.D
 Acq On : 11 Oct 2024 11:35
 Operator : SY/MD
 Sample : P4379-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2044	rBV	164862	309294	13.58%	1.870%
38	7.979	2153	2158	2161	rBV4	543	624	0.03%	0.004%
39	8.024	2161	2172	2212	rBV2	286357	660645	29.00%	3.994%
40	8.632	2359	2361	2363	rVB3	285	69	0.00%	0.000%
41	8.670	2371	2373	2374	rBV	529	230	0.01%	0.001%
42	8.690	2376	2379	2382	rVB4	884	568	0.02%	0.003%
43	8.728	2388	2391	2393	rBV2	922	626	0.03%	0.004%
44	8.776	2396	2406	2441	rVV	1079991	1814138	79.63%	10.967%
45	9.275	2559	2561	2564	rBV4	347	151	0.01%	0.001%
46	9.333	2577	2579	2580	rBV2	592	263	0.01%	0.002%
47	9.391	2595	2597	2598	rBV	490	191	0.01%	0.001%
48	9.551	2645	2647	2648	rBV	660	276	0.01%	0.002%
49	9.587	2656	2658	2660	rBV2	342	114	0.01%	0.001%
50	9.728	2699	2702	2704	rBV3	688	479	0.02%	0.003%
51	9.789	2715	2721	2723	rBV3	756	633	0.03%	0.004%
52	9.866	2742	2745	2747	rBV2	681	440	0.02%	0.003%
53	9.889	2749	2752	2755	rVV4	1180	739	0.03%	0.004%
54	9.944	2767	2769	2772	rBV3	483	213	0.01%	0.001%
55	9.985	2780	2782	2785	rVB3	694	299	0.01%	0.002%
56	10.001	2785	2787	2790	rVB2	657	356	0.02%	0.002%
57	10.024	2790	2794	2795	rBV2	645	391	0.02%	0.002%
58	10.050	2799	2802	2810	rBV4	916	943	0.04%	0.006%
59	10.146	2819	2832	2851	rBV	592778	945365	41.50%	5.715%
60	10.358	2895	2898	2905	rVB4	951	997	0.04%	0.006%
61	10.391	2905	2908	2911	rBV3	579	524	0.02%	0.003%
62	10.554	2957	2959	2961	rVB2	205	65	0.00%	0.000%
63	10.567	2961	2963	2967	rVB2	203	119	0.01%	0.001%
64	10.587	2967	2969	2972	rBV4	604	362	0.02%	0.002%
65	10.661	2989	2992	2995	rBV2	504	305	0.01%	0.002%
66	10.690	2998	3001	3007	rBV4	759	760	0.03%	0.005%
67	10.725	3010	3012	3014	rBV2	244	143	0.01%	0.001%
68	10.741	3014	3017	3021	rBV3	507	317	0.01%	0.002%
69	10.773	3025	3027	3030	rBV3	533	347	0.02%	0.002%
70	10.837	3042	3047	3050	rBV6	816	746	0.03%	0.005%
71	10.860	3050	3054	3057	rBV6	829	743	0.03%	0.004%
72	10.966	3085	3087	3088	rBV	270	94	0.00%	0.001%
73	10.985	3091	3093	3096	rVB3	776	386	0.02%	0.002%
74	11.011	3096	3101	3104	rBV2	434	503	0.02%	0.003%
75	11.030	3105	3107	3110	rVV3	798	449	0.02%	0.003%
76	11.050	3110	3113	3116	rVV4	630	329	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037821.D
 Acq On : 11 Oct 2024 11:35
 Operator : SY/MD
 Sample : P4379-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOLH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.069	3116	3119	3121	rVB2	475	200	0.01%	0.001%
78	11.178	3141	3153	3184	rBV	994089	1606972	70.54%	9.714%
79	11.551	3258	3269	3297	rBV	988621	1622760	71.23%	9.810%
80	11.921	3381	3384	3386	rBV4	884	688	0.03%	0.004%
81	12.040	3417	3421	3423	rBV4	860	600	0.03%	0.004%
82	12.178	3461	3464	3468	rBV5	879	752	0.03%	0.005%
83	12.265	3488	3491	3493	rBV2	764	410	0.02%	0.002%
84	12.316	3505	3507	3511	rVB4	819	436	0.02%	0.003%
85	12.448	3546	3548	3550	rBV	489	190	0.01%	0.001%
86	12.587	3586	3591	3593	rBV5	1359	1178	0.05%	0.007%
87	12.712	3628	3630	3633	rBV2	957	479	0.02%	0.003%
88	12.931	3696	3698	3700	rBV3	516	273	0.01%	0.002%
89	13.027	3726	3728	3730	rBV2	638	277	0.01%	0.002%
90	13.615	3909	3911	3914	rBV2	1092	645	0.03%	0.004%
91	13.689	3929	3934	3938	rBV6	1484	1724	0.08%	0.010%
92	14.281	4113	4118	4122	rBV5	1689	1628	0.07%	0.010%




Sum of corrected areas: 16542142

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037821.D
Acq On : 11 Oct 2024 11:35
Operator : SY/MD
Sample : P4379-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

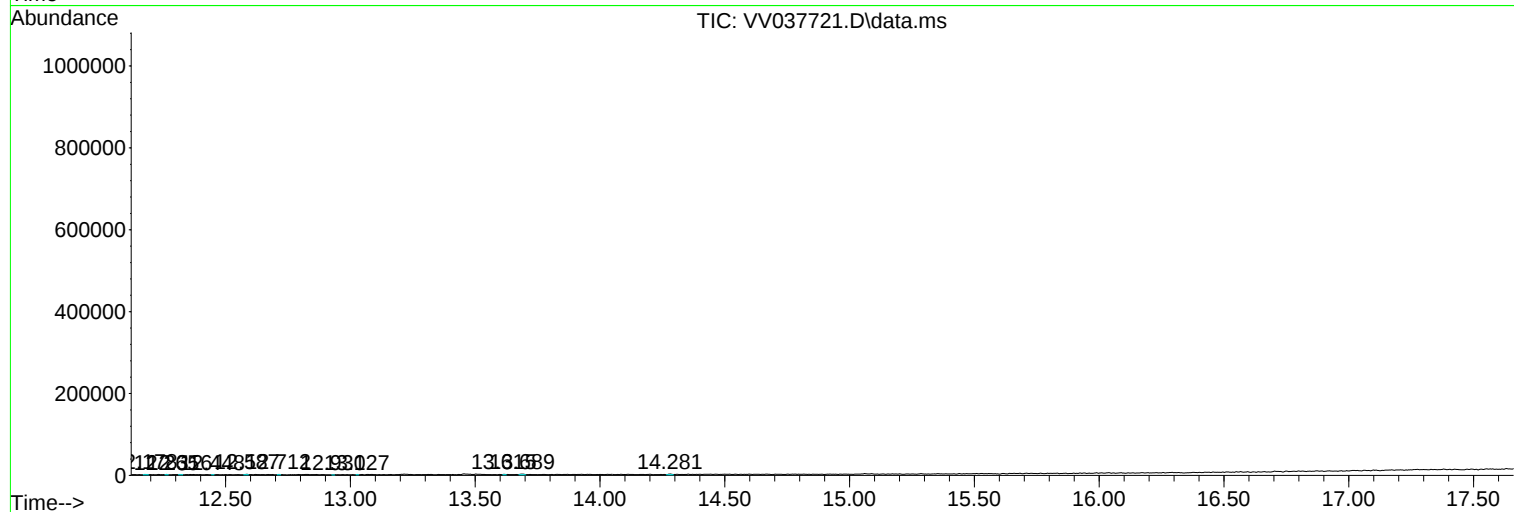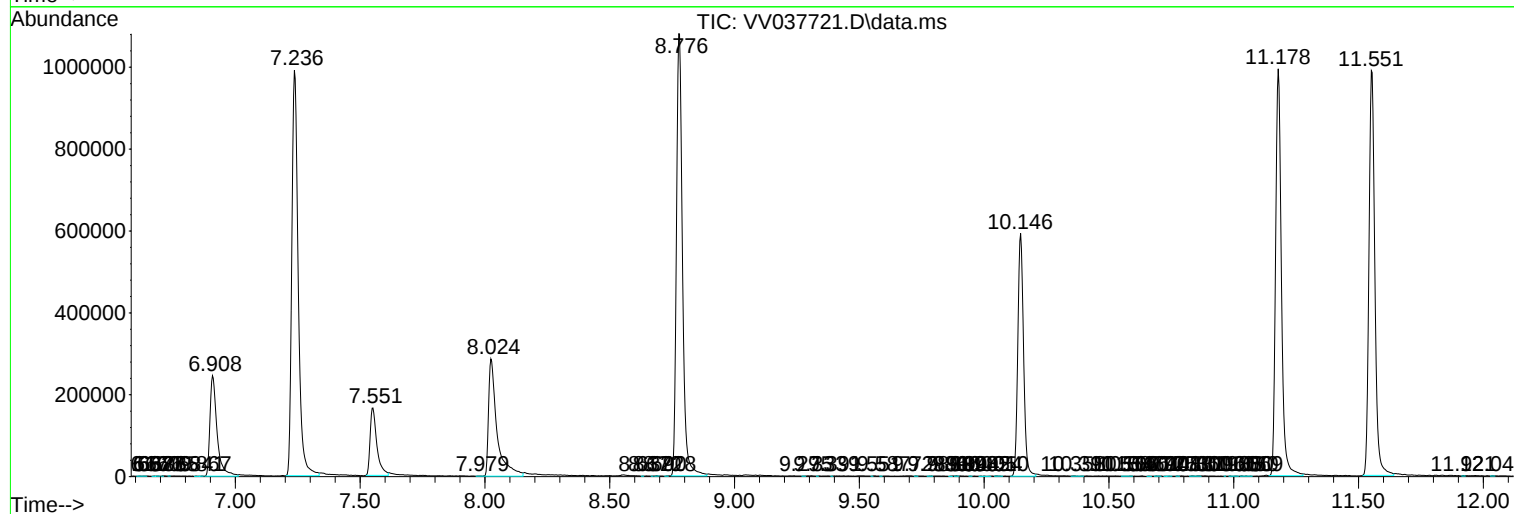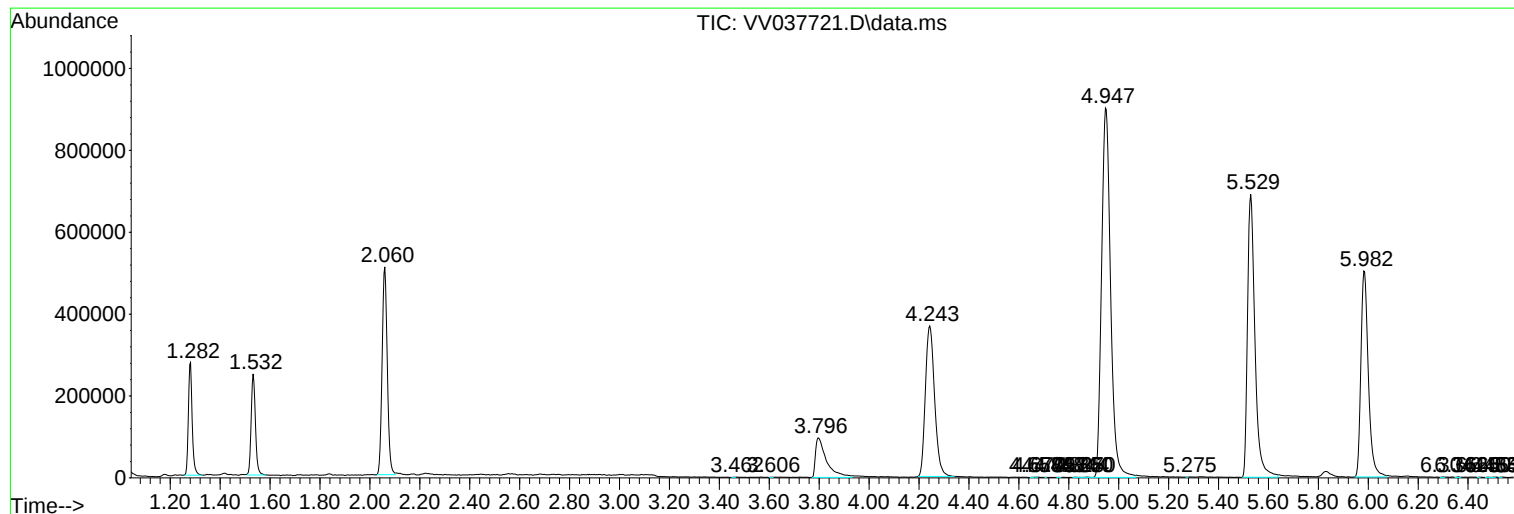

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037821.D
Acq On : 11 Oct 2024 11:35
Operator : SY/MD
Sample : P4379-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037821.D
Acq On : 11 Oct 2024 11:35
Operator : SY/MD
Sample : P4379-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOLH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------