

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037823.D
 Acq On : 11 Oct 2024 12:17
 Operator : SY/MD
 Sample : P4363-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV2	6459	9958	0.43%	0.059%
2	1.281	67	75	89	rBV	275993	298039	12.90%	1.764%
3	1.532	146	153	169	rVB	254124	305412	13.22%	1.807%
4	2.060	307	317	331	rBV	523785	745703	32.28%	4.413%
5	3.217	675	677	681	rBV3	665	553	0.02%	0.003%
6	3.265	688	692	695	rBV3	996	924	0.04%	0.005%
7	3.461	747	753	756	rVB5	815	935	0.04%	0.006%
8	3.558	777	783	786	rBV5	755	781	0.03%	0.005%
9	3.799	849	858	906	rBV	106572	324556	14.05%	1.921%
10	4.079	941	945	951	rVB6	815	954	0.04%	0.006%
11	4.124	956	959	964	rVB5	1166	1149	0.05%	0.007%
12	4.146	964	966	969	rBV2	1313	879	0.04%	0.005%
13	4.243	978	996	1029	rBV	394649	985389	42.65%	5.831%
14	4.490	1071	1073	1077	rVB2	873	462	0.02%	0.003%
15	4.558	1091	1094	1096	rBV4	680	455	0.02%	0.003%
16	4.622	1111	1114	1119	rBV4	570	501	0.02%	0.003%
17	4.789	1163	1166	1168	rBV3	674	433	0.02%	0.003%
18	4.841	1177	1182	1186	rVB4	453	503	0.02%	0.003%
19	4.950	1201	1216	1253	rBV2	921865	2310208	100.00%	13.671%
20	5.143	1274	1276	1280	rVV5	1059	654	0.03%	0.004%
21	5.178	1284	1287	1289	rBV3	934	605	0.03%	0.004%
22	5.207	1293	1296	1297	rBV	1109	553	0.02%	0.003%
23	5.262	1310	1313	1314	rBV4	755	444	0.02%	0.003%
24	5.333	1332	1335	1337	rVV4	923	504	0.02%	0.003%
25	5.352	1340	1341	1346	rVB4	694	521	0.02%	0.003%
26	5.394	1350	1354	1357	rVB2	826	445	0.02%	0.003%
27	5.529	1384	1396	1424	rBV	661924	1365711	59.12%	8.082%
28	5.764	1465	1469	1470	rBV3	865	637	0.03%	0.004%
29	5.831	1478	1490	1509	rBV3	14580	33450	1.45%	0.198%
30	5.982	1524	1537	1574	rBV	521982	1092581	47.29%	6.466%
31	6.194	1601	1603	1607	rVB5	1215	830	0.04%	0.005%
32	6.227	1611	1613	1616	rBV4	1195	742	0.03%	0.004%
33	6.288	1629	1632	1635	rVB3	885	460	0.02%	0.003%
34	6.420	1668	1673	1676	rVB4	764	704	0.03%	0.004%
35	6.442	1676	1680	1685	rBV4	947	881	0.04%	0.005%
36	6.465	1685	1687	1692	rVB5	770	503	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037823.D
 Acq On : 11 Oct 2024 12:17
 Operator : SY/MD
 Sample : P4363-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.555	1708	1715	1718	rBV5	852	869	0.04%	0.005%
38	6.690	1750	1757	1758	rBV2	894	796	0.03%	0.005%
39	6.722	1762	1767	1768	rBV2	852	826	0.04%	0.005%
40	6.812	1791	1795	1798	rVB4	798	645	0.03%	0.004%
41	6.863	1807	1811	1815	rBV2	541	578	0.03%	0.003%
42	6.908	1815	1825	1852	rBV	253692	486244	21.05%	2.877%
43	7.236	1916	1927	1967	rBV	984761	1764836	76.39%	10.444%
44	7.548	2015	2024	2048	rBV	166220	318927	13.81%	1.887%
45	7.828	2109	2111	2117	rBV5	1058	809	0.04%	0.005%
46	8.024	2164	2172	2212	rBV2	312526	697349	30.19%	4.127%
47	8.545	2328	2334	2335	rBV6	1284	1052	0.05%	0.006%
48	8.558	2335	2338	2349	rVB6	2328	2994	0.13%	0.018%
49	8.780	2395	2407	2444	rBV	1046963	1762882	76.31%	10.432%
50	9.037	2484	2487	2489	rBV4	880	612	0.03%	0.004%
51	9.156	2521	2524	2528	rVB4	758	489	0.02%	0.003%
52	9.259	2553	2556	2558	rBV4	812	458	0.02%	0.003%
53	9.297	2566	2568	2570	rBV2	838	436	0.02%	0.003%
54	9.432	2605	2610	2612	rBV3	787	826	0.04%	0.005%
55	9.497	2628	2630	2632	rBV3	881	519	0.02%	0.003%
56	9.554	2646	2648	2651	rVV4	841	572	0.02%	0.003%
57	9.577	2653	2655	2661	rVB4	912	663	0.03%	0.004%
58	9.606	2661	2664	2667	rBV2	876	492	0.02%	0.003%
59	9.735	2699	2704	2708	rVB5	923	771	0.03%	0.005%
60	9.792	2718	2722	2726	rVV3	753	561	0.02%	0.003%
61	9.969	2773	2777	2779	rBV3	746	470	0.02%	0.003%
62	10.001	2783	2787	2791	rBV2	604	657	0.03%	0.004%
63	10.146	2820	2832	2855	rBV	649789	1026914	44.45%	6.077%
64	10.355	2893	2897	2900	rVB2	803	562	0.02%	0.003%
65	10.374	2900	2903	2906	rVB2	649	453	0.02%	0.003%
66	10.442	2921	2924	2927	rBV2	851	441	0.02%	0.003%
67	10.464	2927	2931	2935	rBV6	1016	834	0.04%	0.005%
68	10.506	2941	2944	2949	rBV4	809	748	0.03%	0.004%
69	10.776	3022	3028	3030	rBV3	540	541	0.02%	0.003%
70	10.956	3080	3084	3089	rBV2	630	605	0.03%	0.004%
71	11.178	3142	3153	3189	rBV	1018672	1629449	70.53%	9.643%
72	11.551	3258	3269	3309	rVV	1028808	1683582	72.88%	9.963%
73	11.927	3384	3386	3390	rVB3	1014	767	0.03%	0.005%
74	11.953	3390	3394	3396	rBV3	834	639	0.03%	0.004%
75	12.001	3405	3409	3412	rBV3	981	731	0.03%	0.004%
76	12.033	3417	3419	3423	rVB2	699	499	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037823.D
 Acq On : 11 Oct 2024 12:17
 Operator : SY/MD
 Sample : P4363-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.059	3423	3427	3433	rBV6	844	893	0.04%	0.005%
78	12.185	3463	3466	3468	rBV2	645	534	0.02%	0.003%
79	12.368	3519	3523	3527	rBV3	543	444	0.02%	0.003%
80	12.394	3527	3531	3534	rBV	507	530	0.02%	0.003%
81	12.519	3567	3570	3578	rVB5	564	558	0.02%	0.003%
82	12.554	3578	3581	3583	rVB2	815	460	0.02%	0.003%
83	12.599	3591	3595	3598	rBV3	1102	846	0.04%	0.005%
84	12.776	3646	3650	3653	rBV3	1003	857	0.04%	0.005%
85	12.840	3667	3670	3673	rBV3	776	461	0.02%	0.003%
86	12.902	3684	3689	3692	rBV3	758	695	0.03%	0.004%
87	13.069	3738	3741	3743	rBV3	697	547	0.02%	0.003%
88	13.213	3783	3786	3787	rBV3	897	498	0.02%	0.003%
89	13.461	3858	3863	3865	rBV4	1050	979	0.04%	0.006%
90	13.522	3878	3882	3884	rBV4	670	558	0.02%	0.003%
91	13.564	3893	3895	3902	rVB5	927	926	0.04%	0.005%
92	13.596	3903	3905	3909	rBV3	959	730	0.03%	0.004%
93	13.686	3929	3933	3936	rBV3	1353	1066	0.05%	0.006%
94	13.911	4000	4003	4006	rBV3	614	520	0.02%	0.003%
95	14.310	4124	4127	4130	rBV3	989	589	0.03%	0.003%
96	14.776	4270	4272	4275	rBV4	897	531	0.02%	0.003%
97	14.808	4280	4282	4285	rVB3	1165	569	0.02%	0.003%
98	14.950	4324	4326	4328	rBV3	881	532	0.02%	0.003%
99	15.117	4374	4378	4385	rVB6	1741	1603	0.07%	0.009%
100	15.483	4490	4492	4497	rBV6	1057	1114	0.05%	0.007%




Sum of corrected areas: 16898157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037823.D
Acq On : 11 Oct 2024 12:17
Operator : SY/MD
Sample : P4363-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

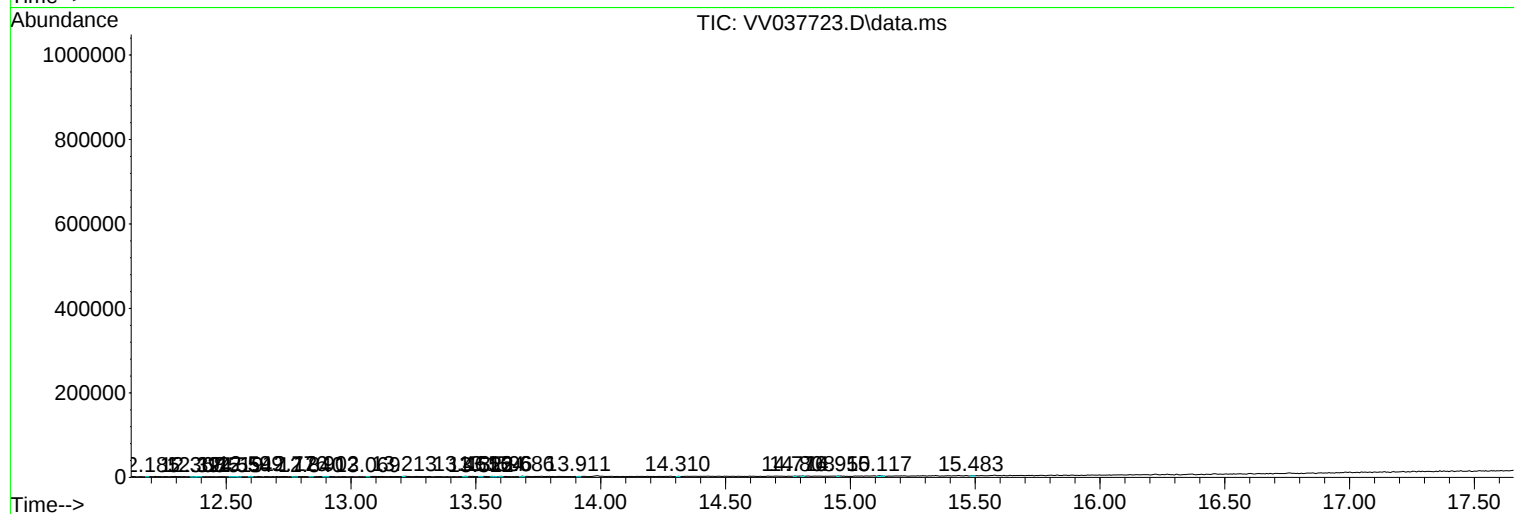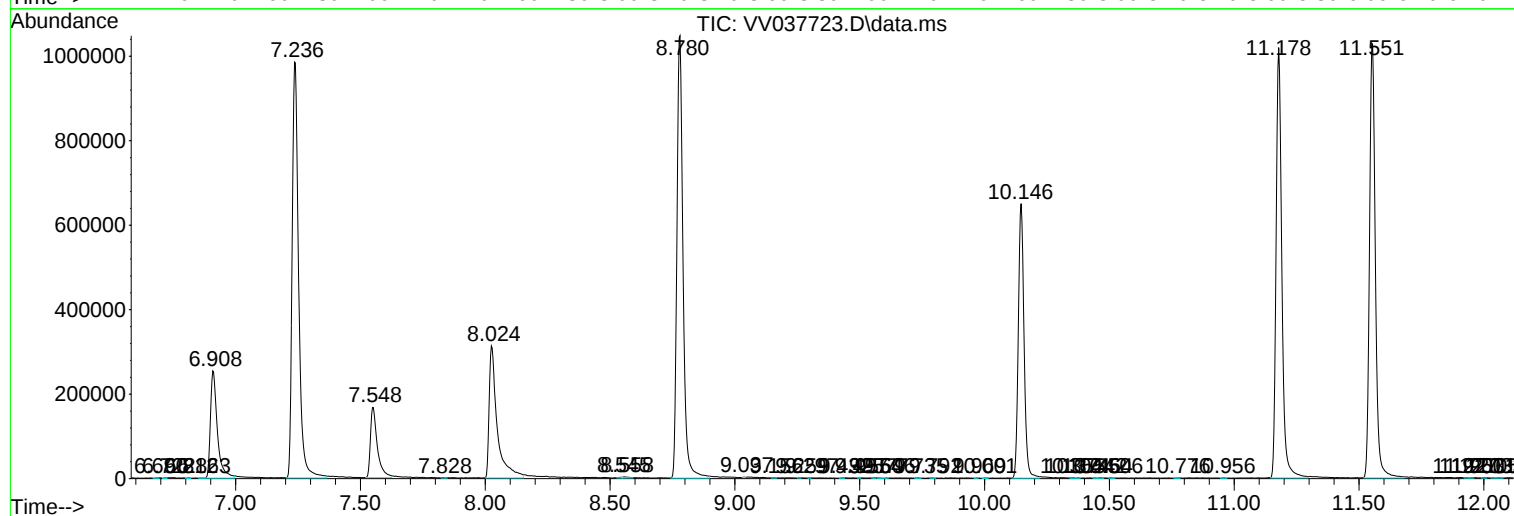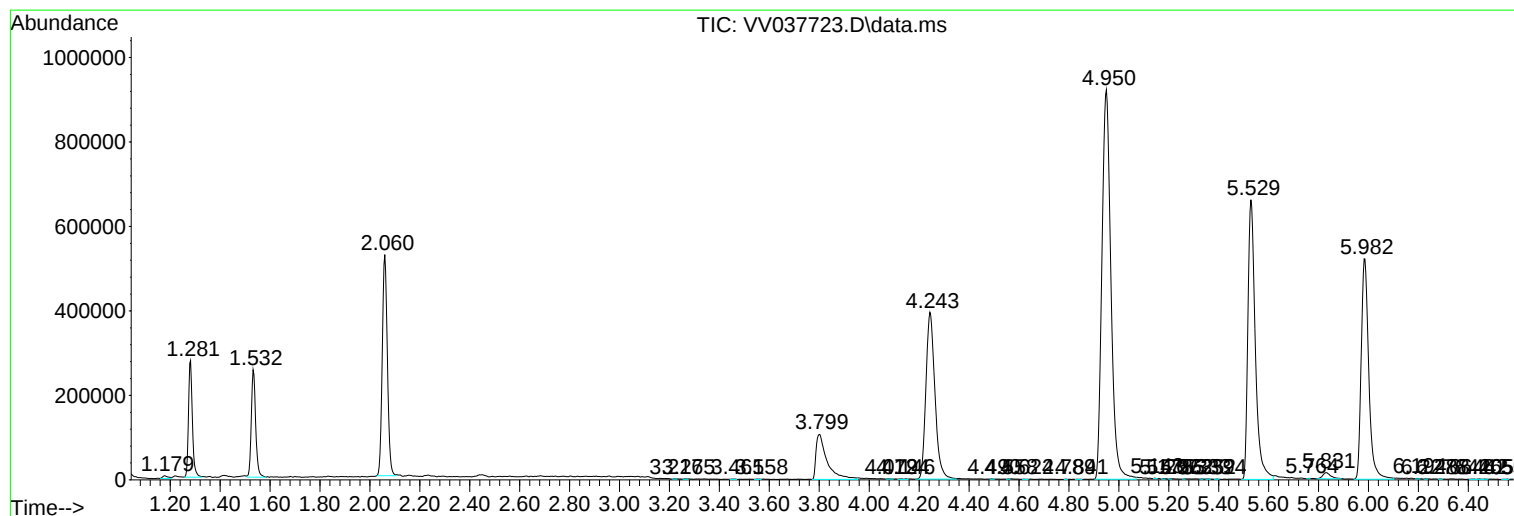

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037823.D
Acq On : 11 Oct 2024 12:17
Operator : SY/MD
Sample : P4363-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037823.D
Acq On : 11 Oct 2024 12:17
Operator : SY/MD
Sample : P4363-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------