

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037831.D
 Acq On : 11 Oct 2024 15:10
 Operator : SY/MD
 Sample : VIBLK203
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	44	rBV2	2577	2119	0.09%	0.012%
2	1.220	51	56	61	rBV2	5656	8109	0.34%	0.044%
3	1.278	67	74	92	rBV	291738	309202	12.81%	1.691%
4	1.532	146	153	170	rVB	255111	305041	12.64%	1.668%
5	2.060	307	317	334	rVB	533884	769665	31.89%	4.209%
6	3.371	722	725	729	rVB4	1028	577	0.02%	0.003%
7	3.539	772	777	778	rBV3	1127	780	0.03%	0.004%
8	3.799	849	858	896	rBV	110501	343320	14.23%	1.877%
9	4.243	978	996	1023	rBV	386127	991519	41.09%	5.422%
10	4.786	1161	1165	1168	rBV4	1037	633	0.03%	0.003%
11	4.947	1200	1215	1246	rBV2	965284	2413220	100.00%	13.196%
12	5.243	1302	1307	1309	rBV5	1230	1058	0.04%	0.006%
13	5.294	1320	1323	1326	rBV4	776	527	0.02%	0.003%
14	5.365	1343	1345	1350	rVB4	1074	696	0.03%	0.004%
15	5.439	1364	1368	1370	rBV3	582	580	0.02%	0.003%
16	5.529	1385	1396	1428	rBV	776878	1591864	65.96%	8.704%
17	5.828	1478	1489	1504	rBV7	17611	42930	1.78%	0.235%
18	5.982	1523	1537	1572	rBV	530150	1111321	46.05%	6.077%
19	6.188	1598	1601	1603	rBV3	1076	808	0.03%	0.004%
20	6.252	1619	1621	1624	rBV3	728	495	0.02%	0.003%
21	6.275	1627	1628	1634	rVB4	1005	671	0.03%	0.004%
22	6.503	1694	1699	1702	rBV4	679	708	0.03%	0.004%
23	6.522	1702	1705	1709	rVB3	634	466	0.02%	0.003%
24	6.690	1752	1757	1761	rBV5	1061	1009	0.04%	0.006%
25	6.776	1782	1784	1788	rVB3	965	637	0.03%	0.003%
26	6.802	1788	1792	1796	rBV4	884	622	0.03%	0.003%
27	6.908	1814	1825	1856	rBV	272523	532736	22.08%	2.913%
28	7.091	1880	1882	1886	rVB3	1152	715	0.03%	0.004%
29	7.169	1902	1906	1909	rBV6	1026	761	0.03%	0.004%
30	7.236	1916	1927	1965	rBV	1075370	1914499	79.33%	10.469%
31	7.551	2015	2025	2060	rVV	180548	350714	14.53%	1.918%
32	7.760	2087	2090	2091	rBV2	891	464	0.02%	0.003%
33	7.828	2108	2111	2116	rVB5	772	673	0.03%	0.004%
34	7.902	2129	2134	2135	rBV3	1925	1550	0.06%	0.008%
35	7.963	2150	2153	2156	rVB4	803	519	0.02%	0.003%
36	7.992	2156	2162	2163	rBV3	670	646	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037831.D
Acq On : 11 Oct 2024 15:10
Operator : SY/MD
Sample : VIBLK203
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

37	8.024	2163	2172	2202	rBV2	320395	683341	28.32%	3.737%
38	8.362	2273	2277	2284	rBV7	1330	1497	0.06%	0.008%
39	8.497	2316	2319	2326	rVB5	1147	1063	0.04%	0.006%
40	8.548	2331	2335	2337	rBV4	1832	1390	0.06%	0.008%
41	8.699	2380	2382	2387	rVB4	755	509	0.02%	0.003%
42	8.776	2395	2406	2435	rBV	1181669	1975773	81.87%	10.804%
43	9.046	2487	2490	2498	rBV8	1335	1936	0.08%	0.011%
44	9.397	2595	2599	2603	rVB3	814	491	0.02%	0.003%
45	9.490	2622	2628	2632	rBV6	3421	3762	0.16%	0.021%
46	9.529	2638	2640	2644	rVB4	903	521	0.02%	0.003%
47	9.635	2669	2673	2675	rBV2	808	621	0.03%	0.003%
48	9.648	2675	2677	2680	rVB3	1010	556	0.02%	0.003%
49	9.731	2701	2703	2708	rBV4	566	521	0.02%	0.003%
50	9.870	2738	2746	2754	rVV6	3832	6261	0.26%	0.034%
51	9.982	2778	2781	2785	rVB3	784	656	0.03%	0.004%
52	10.011	2785	2790	2793	rBV4	1081	893	0.04%	0.005%
53	10.146	2818	2832	2863	rBV	614395	994223	41.20%	5.436%
54	10.374	2901	2903	2908	rVB4	1155	875	0.04%	0.005%
55	10.406	2908	2913	2916	rBV3	744	831	0.03%	0.005%
56	10.480	2929	2936	2946	rVB5	4043	6108	0.25%	0.033%
57	10.551	2954	2958	2961	rBV3	1029	884	0.04%	0.005%
58	10.622	2975	2980	2983	rBV5	576	466	0.02%	0.003%
59	10.638	2983	2985	2993	rVB5	814	794	0.03%	0.004%
60	10.731	3009	3014	3017	rBV4	869	828	0.03%	0.005%
61	10.783	3026	3030	3033	rBV5	1083	730	0.03%	0.004%
62	10.860	3044	3054	3062	rBV8	4201	7467	0.31%	0.041%
63	10.940	3077	3079	3084	rVV2	710	550	0.02%	0.003%
64	11.127	3128	3137	3142	rBV6	8606	12922	0.54%	0.071%
65	11.178	3143	3153	3182	rVV	1157105	1853295	76.80%	10.134%
66	11.551	3257	3269	3304	rBV	1111271	1807586	74.90%	9.884%
67	11.918	3381	3383	3386	rVB3	1000	611	0.03%	0.003%
68	11.943	3386	3391	3394	rBV5	827	838	0.03%	0.005%
69	11.985	3398	3404	3408	rVB6	822	917	0.04%	0.005%
70	12.008	3408	3411	3414	rBV4	756	559	0.02%	0.003%
71	12.239	3482	3483	3488	rVB3	708	468	0.02%	0.003%
72	12.326	3507	3510	3513	rVB4	755	461	0.02%	0.003%
73	12.349	3513	3517	3519	rBV4	1014	751	0.03%	0.004%
74	12.374	3519	3525	3526	rBV5	1495	1261	0.05%	0.007%
75	12.435	3541	3544	3547	rVB3	998	777	0.03%	0.004%
76	12.493	3560	3562	3566	rVB2	1508	786	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037831.D
 Acq On : 11 Oct 2024 15:10
 Operator : SY/MD
 Sample : VIBLK203
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK203

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.529	3566	3573	3575	rBV5	1586	1577	0.07%	0.009%
78	12.583	3581	3590	3602	rBV5	11315	22420	0.93%	0.123%
79	12.747	3637	3641	3643	rVB3	909	754	0.03%	0.004%
80	12.767	3643	3647	3649	rBV3	588	466	0.02%	0.003%
81	12.808	3654	3660	3662	rVV4	924	964	0.04%	0.005%
82	12.837	3666	3669	3673	rVB3	734	523	0.02%	0.003%
83	12.914	3689	3693	3695	rBV4	822	577	0.02%	0.003%
84	12.979	3707	3713	3714	rBV3	535	486	0.02%	0.003%
85	13.149	3764	3766	3771	rVB5	796	497	0.02%	0.003%
86	13.201	3771	3782	3796	rBV5	19030	37638	1.56%	0.206%
87	13.297	3810	3812	3816	rVB3	794	518	0.02%	0.003%
88	13.342	3823	3826	3829	rBV3	1172	597	0.02%	0.003%
89	13.439	3847	3856	3874	rBV	46059	86931	3.60%	0.475%
90	13.680	3921	3931	3944	rBV3	28492	48632	2.02%	0.266%
91	13.757	3953	3955	3959	rVB6	1060	600	0.02%	0.003%
92	13.811	3970	3972	3974	rBV	758	493	0.02%	0.003%
93	14.085	4055	4057	4059	rVB	1036	522	0.02%	0.003%
94	14.104	4060	4063	4068	rBV5	1052	914	0.04%	0.005%
95	14.159	4077	4080	4087	rBV5	789	810	0.03%	0.004%
96	14.278	4114	4117	4119	rBV3	863	512	0.02%	0.003%
97	14.525	4190	4194	4197	rBV3	1560	1690	0.07%	0.009%
98	14.879	4300	4304	4309	rBV7	1634	1888	0.08%	0.010%
99	14.943	4321	4324	4325	rBV3	1042	537	0.02%	0.003%
100	15.246	4416	4418	4420	rBV3	1548	814	0.03%	0.004%




Sum of corrected areas: 18287993

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037831.D
Acq On : 11 Oct 2024 15:10
Operator : SY/MD
Sample : VIBLK203
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

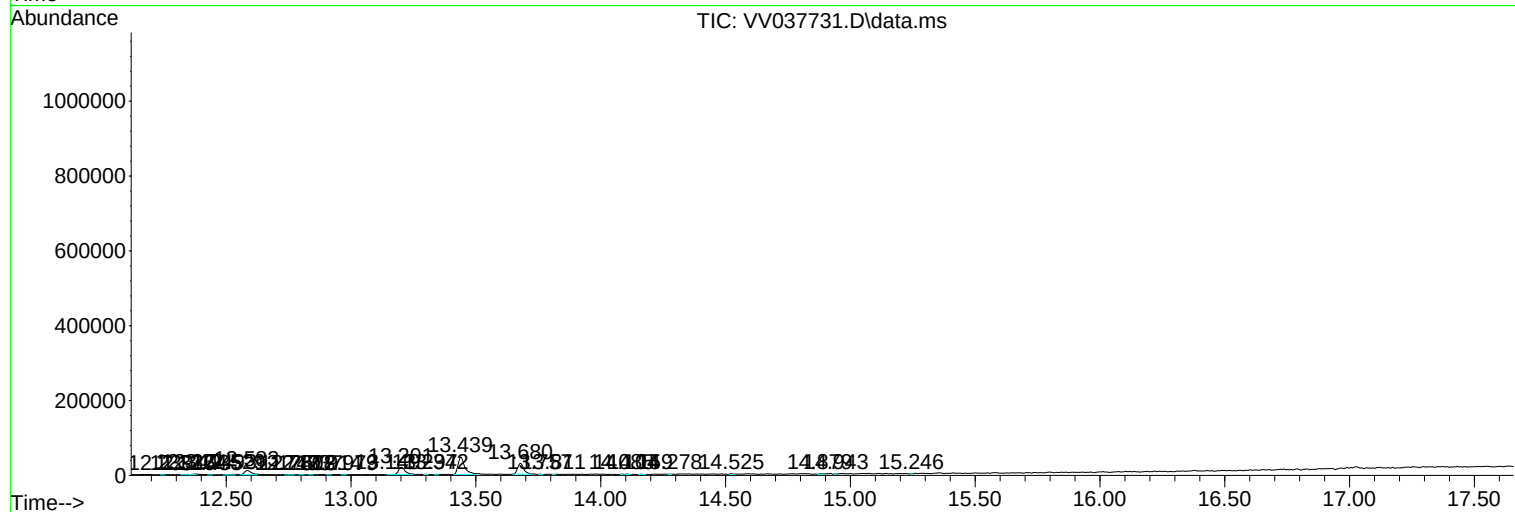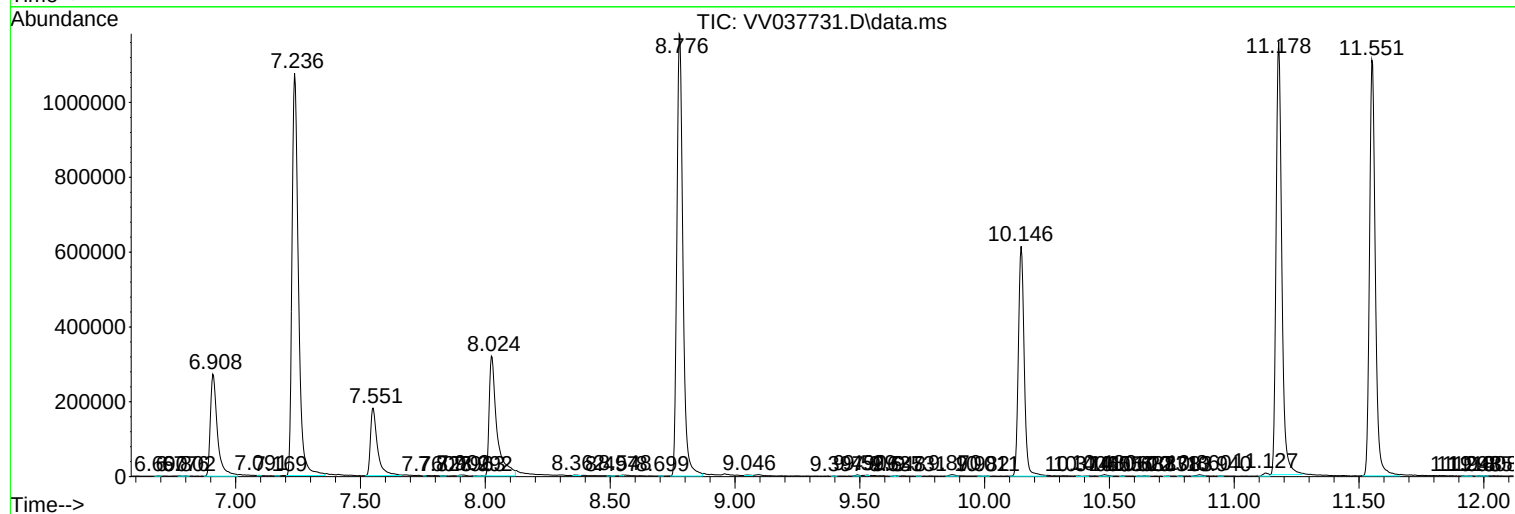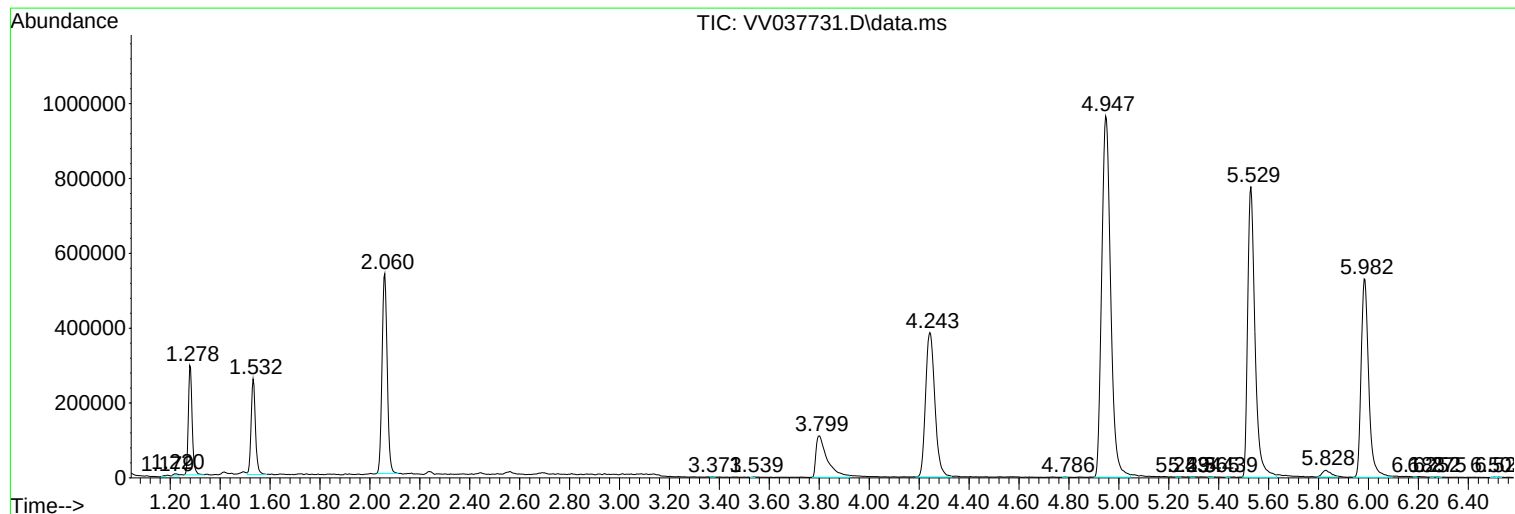

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037831.D
Acq On : 11 Oct 2024 15:10
Operator : SY/MD
Sample : VIBLK203
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037831.D
Acq On : 11 Oct 2024 15:10
Operator : SY/MD
Sample : VIBLK203
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK203

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------