

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037835.D
 Acq On : 11 Oct 2024 16:36
 Operator : SY/MD
 Sample : P4349-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	261857	281347	12.25%	1.680%
2	1.532	146	153	164	rVB	238379	278397	12.12%	1.662%
3	2.060	307	317	329	rBV	500930	718110	31.27%	4.287%
4	3.558	780	783	786	rBV4	684	418	0.02%	0.002%
5	3.616	799	801	805	rVB3	769	407	0.02%	0.002%
6	3.677	818	820	822	rBV3	468	195	0.01%	0.001%
7	3.706	827	829	832	rBV	370	214	0.01%	0.001%
8	3.748	840	842	844	rBV3	588	362	0.02%	0.002%
9	3.799	849	858	891	rBV2	103872	297580	12.96%	1.776%
10	4.243	979	996	1028	rBV2	373220	951481	41.43%	5.680%
11	4.558	1092	1094	1097	rVB2	783	325	0.01%	0.002%
12	4.638	1117	1119	1121	rVB2	742	229	0.01%	0.001%
13	4.664	1123	1127	1129	rBV3	634	584	0.03%	0.003%
14	4.722	1143	1145	1148	rVB2	474	233	0.01%	0.001%
15	4.738	1148	1150	1151	rBV	772	318	0.01%	0.002%
16	4.776	1161	1162	1166	rBV2	286	179	0.01%	0.001%
17	4.947	1200	1215	1252	rBV2	904458	2296492	100.00%	13.709%
18	5.236	1303	1305	1307	rVB2	812	274	0.01%	0.002%
19	5.426	1361	1364	1366	rBV3	717	463	0.02%	0.003%
20	5.529	1383	1396	1432	rBV	687298	1425574	62.08%	8.510%
21	5.831	1480	1490	1503	rBV3	14920	32425	1.41%	0.194%
22	5.985	1525	1538	1569	rBV	505437	1047447	45.61%	6.253%
23	6.281	1626	1630	1632	rBV4	1047	823	0.04%	0.005%
24	6.346	1648	1650	1653	rBV2	443	281	0.01%	0.002%
25	6.387	1660	1663	1668	rVB3	534	509	0.02%	0.003%
26	6.436	1674	1678	1679	rBV	749	476	0.02%	0.003%
27	6.493	1694	1696	1699	rBV2	359	214	0.01%	0.001%
28	6.516	1702	1703	1706	rVB	632	225	0.01%	0.001%
29	6.538	1707	1710	1712	rBV	527	318	0.01%	0.002%
30	6.564	1716	1718	1721	rVB4	683	312	0.01%	0.002%
31	6.587	1721	1725	1728	rBV5	484	364	0.02%	0.002%
32	6.651	1743	1745	1746	rBV	635	200	0.01%	0.001%
33	6.699	1757	1760	1762	rVB3	459	305	0.01%	0.002%
34	6.722	1762	1767	1769	rBV2	1251	945	0.04%	0.006%
35	6.747	1771	1775	1779	rVV5	865	664	0.03%	0.004%
36	6.802	1788	1792	1793	rBV2	526	368	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037835.D
 Acq On : 11 Oct 2024 16:36
 Operator : SY/MD
 Sample : P4349-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.825	1796	1799	1802	rVB3	533	370	0.02%	0.002%
38	6.847	1802	1806	1808	rVB	358	244	0.01%	0.001%
39	6.863	1808	1811	1813	rBV2	359	190	0.01%	0.001%
40	6.908	1813	1825	1856	rBV	248592	491663	21.41%	2.935%
41	7.159	1901	1903	1906	rBV2	830	592	0.03%	0.004%
42	7.236	1917	1927	1960	rBV	1008295	1798451	78.31%	10.736%
43	7.551	2016	2025	2060	rBV	167291	322625	14.05%	1.926%
44	7.844	2114	2116	2119	rBV2	595	284	0.01%	0.002%
45	7.956	2148	2151	2154	rBV4	813	616	0.03%	0.004%
46	8.027	2164	2173	2210	rBV2	298714	672835	29.30%	4.017%
47	8.622	2356	2358	2360	rBV2	791	494	0.02%	0.003%
48	8.661	2366	2370	2372	rBV2	710	659	0.03%	0.004%
49	8.677	2373	2375	2377	rBV4	812	275	0.01%	0.002%
50	8.699	2380	2382	2387	rVB3	886	638	0.03%	0.004%
51	8.725	2387	2390	2392	rBV2	803	498	0.02%	0.003%
52	8.780	2396	2407	2433	rBV	1067224	1780734	77.54%	10.630%
53	9.236	2545	2549	2551	rBV3	549	382	0.02%	0.002%
54	9.313	2571	2573	2575	rBV2	601	414	0.02%	0.002%
55	9.355	2584	2586	2587	rBV	466	213	0.01%	0.001%
56	9.442	2611	2613	2614	rBV	443	197	0.01%	0.001%
57	9.596	2657	2661	2665	rVB4	518	500	0.02%	0.003%
58	9.635	2671	2673	2675	rBV2	334	171	0.01%	0.001%
59	9.689	2685	2690	2693	rBV5	600	628	0.03%	0.004%
60	9.734	2701	2704	2709	rBV2	429	330	0.01%	0.002%
61	9.770	2711	2715	2717	rBV2	375	320	0.01%	0.002%
62	9.792	2719	2722	2726	rBV2	683	533	0.02%	0.003%
63	9.860	2740	2743	2745	rBV2	476	369	0.02%	0.002%
64	9.902	2754	2756	2758	rBV2	394	208	0.01%	0.001%
65	9.988	2781	2783	2786	rBV2	467	247	0.01%	0.001%
66	10.034	2793	2797	2802	rBV5	900	847	0.04%	0.005%
67	10.075	2808	2810	2812	rBV2	345	172	0.01%	0.001%
68	10.146	2820	2832	2852	rBV	601094	955881	41.62%	5.706%
69	10.468	2931	2932	2934	rBV	293	143	0.01%	0.001%
70	10.509	2943	2945	2949	rVB3	523	297	0.01%	0.002%
71	10.545	2953	2956	2961	rVB3	669	613	0.03%	0.004%
72	10.567	2961	2963	2965	rBV3	279	134	0.01%	0.001%
73	10.734	3013	3015	3016	rBV	415	177	0.01%	0.001%
74	10.786	3029	3031	3033	rVB2	750	334	0.01%	0.002%
75	10.802	3034	3036	3039	rBV2	459	309	0.01%	0.002%
76	10.869	3050	3057	3060	rBV5	947	1287	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037835.D
 Acq On : 11 Oct 2024 16:36
 Operator : SY/MD
 Sample : P4349-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.947	3076	3081	3082	rBV3	568	519	0.02%	0.003%
78	11.030	3105	3107	3109	rBV	321	213	0.01%	0.001%
79	11.069	3117	3119	3122	rVB2	376	188	0.01%	0.001%
80	11.088	3123	3125	3127	rBV3	340	181	0.01%	0.001%
81	11.133	3131	3139	3142	rBV7	1637	1836	0.08%	0.011%
82	11.178	3142	3153	3189	rBV	1017451	1640769	71.45%	9.795%
83	11.496	3242	3252	3259	rBV7	10828	23949	1.04%	0.143%
84	11.551	3259	3269	3301	rVB	1039823	1697286	73.91%	10.132%
85	12.223	3474	3478	3481	rBV2	996	689	0.03%	0.004%
86	12.242	3481	3484	3486	rBV2	803	524	0.02%	0.003%
87	12.410	3533	3536	3538	rBV2	772	407	0.02%	0.002%
88	12.422	3538	3540	3545	rVB	1421	988	0.04%	0.006%
89	12.445	3545	3547	3551	rBV3	588	477	0.02%	0.003%
90	12.477	3553	3557	3560	rBV4	849	842	0.04%	0.005%
91	12.535	3573	3575	3578	rBV3	849	566	0.02%	0.003%
92	12.580	3587	3589	3591	rBV2	1068	617	0.03%	0.004%
93	12.783	3650	3652	3653	rBV	623	187	0.01%	0.001%
94	12.824	3661	3665	3666	rBV2	689	416	0.02%	0.002%
95	12.847	3666	3672	3676	rVB3	1268	1260	0.05%	0.008%
96	12.879	3677	3682	3685	rBV5	829	789	0.03%	0.005%
97	12.988	3714	3716	3719	rBV2	674	373	0.02%	0.002%
98	13.027	3723	3728	3731	rBV6	724	701	0.03%	0.004%
99	13.332	3819	3823	3830	rBV4	573	764	0.03%	0.005%
100	13.686	3927	3933	3937	rBV4	1969	2218	0.10%	0.013%




Sum of corrected areas: 16751691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037835.D
Acq On : 11 Oct 2024 16:36
Operator : SY/MD
Sample : P4349-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

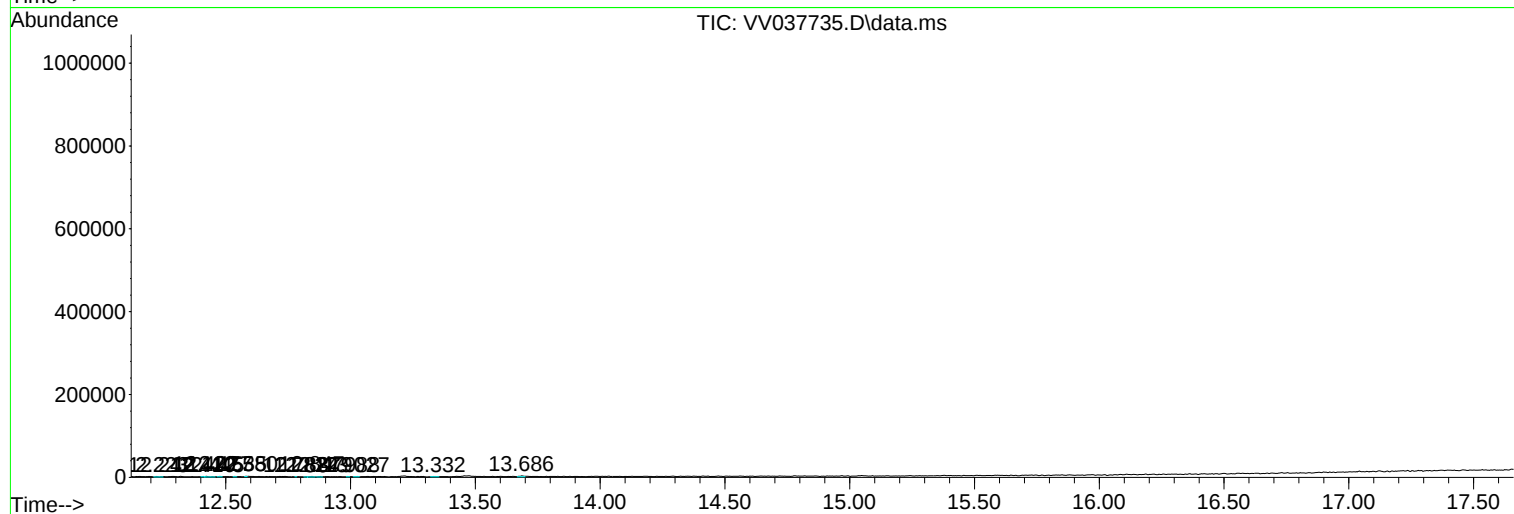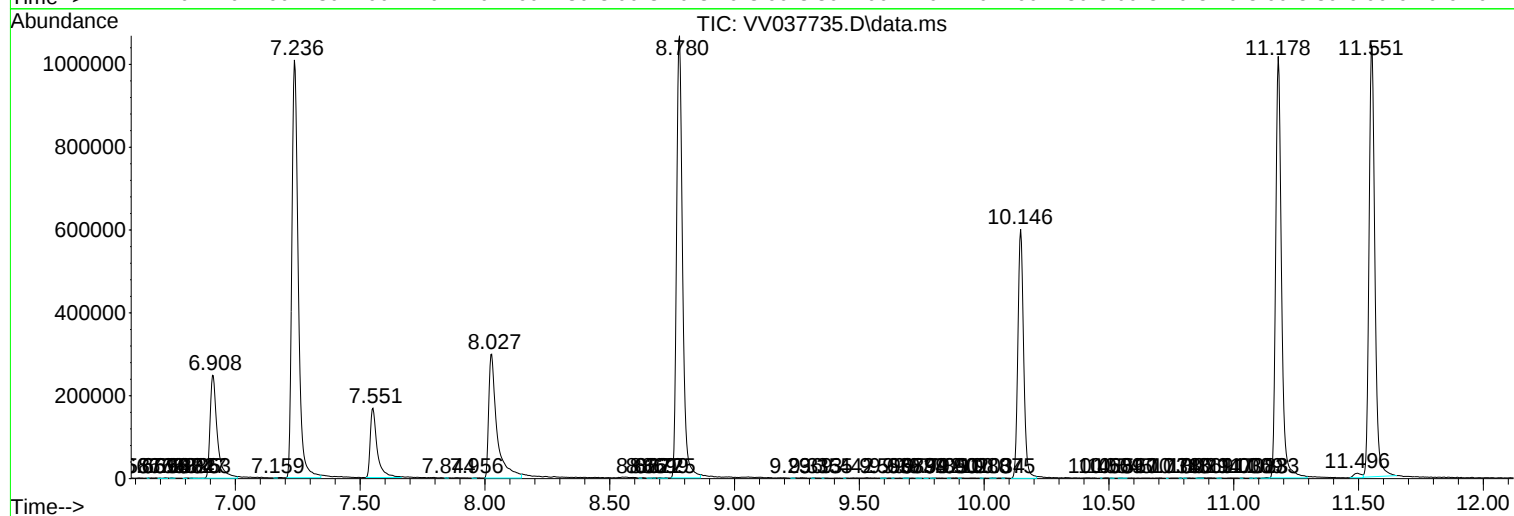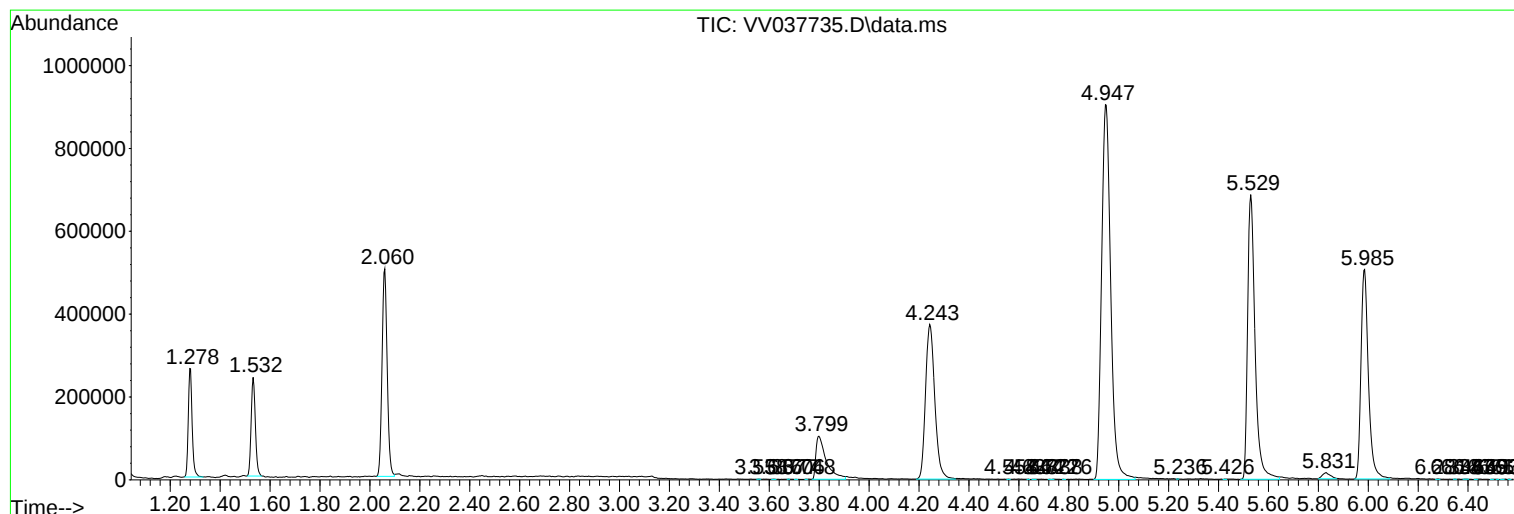

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037835.D
Acq On : 11 Oct 2024 16:36
Operator : SY/MD
Sample : P4349-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037835.D
Acq On : 11 Oct 2024 16:36
Operator : SY/MD
Sample : P4349-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc