

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037836.D
 Acq On : 11 Oct 2024 16:58
 Operator : SY/MD
 Sample : P4349-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	263744	283540	12.38%	1.705%
2	1.532	146	153	167	rVB	242924	286744	12.52%	1.724%
3	2.060	308	317	330	rBV	495356	710511	31.02%	4.272%
4	3.465	751	754	758	rBV2	708	612	0.03%	0.004%
5	3.545	777	779	784	rVB5	957	659	0.03%	0.004%
6	3.706	826	829	830	rBV	408	199	0.01%	0.001%
7	3.732	836	837	842	rVB2	556	242	0.01%	0.001%
8	3.754	842	844	846	rBV	342	234	0.01%	0.001%
9	3.799	850	858	894	rBV	100795	295765	12.91%	1.778%
10	4.166	968	972	975	rBV3	666	681	0.03%	0.004%
11	4.243	980	996	1033	rVV	370566	946364	41.31%	5.690%
12	4.523	1081	1083	1084	rVB3	567	170	0.01%	0.001%
13	4.654	1120	1124	1127	rBV3	774	683	0.03%	0.004%
14	4.805	1169	1171	1177	rVB5	585	463	0.02%	0.003%
15	4.947	1200	1215	1251	rBV2	916050	2290788	100.00%	13.774%
16	5.420	1360	1362	1366	rVV3	735	455	0.02%	0.003%
17	5.439	1366	1368	1372	rVB3	656	461	0.02%	0.003%
18	5.529	1385	1396	1429	rBV	679199	1407828	61.46%	8.465%
19	5.828	1482	1489	1502	rVB4	16728	31180	1.36%	0.187%
20	5.982	1524	1537	1569	rBV	508078	1063926	46.44%	6.397%
21	6.410	1668	1670	1673	rBV4	364	227	0.01%	0.001%
22	6.432	1673	1677	1680	rBV3	802	552	0.02%	0.003%
23	6.474	1688	1690	1695	rVB3	940	577	0.03%	0.003%
24	6.500	1695	1698	1700	rVB3	976	538	0.02%	0.003%
25	6.516	1700	1703	1711	rBV7	827	1030	0.04%	0.006%
26	6.551	1711	1714	1719	rVB5	862	593	0.03%	0.004%
27	6.580	1719	1723	1724	rBV	308	215	0.01%	0.001%
28	6.596	1724	1728	1731	rBV5	809	483	0.02%	0.003%
29	6.641	1740	1742	1745	rVB4	745	425	0.02%	0.003%
30	6.677	1750	1753	1756	rBV3	342	226	0.01%	0.001%
31	6.693	1756	1758	1761	rVV3	566	372	0.02%	0.002%
32	6.789	1783	1788	1789	rBV3	440	378	0.02%	0.002%
33	6.828	1797	1800	1802	rVV	613	307	0.01%	0.002%
34	6.908	1815	1825	1853	rBV	246819	485684	21.20%	2.920%
35	7.236	1916	1927	1949	rBV	1020788	1801733	78.65%	10.833%
36	7.551	2016	2025	2055	rBV	163687	320275	13.98%	1.926%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037836.D
 Acq On : 11 Oct 2024 16:58
 Operator : SY/MD
 Sample : P4349-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.940	2144	2146	2148	rBV3	701	340	0.01%	0.002%
38	7.982	2155	2159	2160	rBV	760	380	0.02%	0.002%
39	8.024	2163	2172	2219	rBV2	299031	684845	29.90%	4.118%
40	8.622	2356	2358	2362	rBV4	728	486	0.02%	0.003%
41	8.780	2396	2407	2440	rBV	1064884	1773741	77.43%	10.665%
42	9.323	2574	2576	2582	rBV6	717	785	0.03%	0.005%
43	9.374	2589	2592	2593	rVB	456	214	0.01%	0.001%
44	9.387	2593	2596	2598	rBV4	788	626	0.03%	0.004%
45	9.439	2609	2612	2615	rVB4	758	433	0.02%	0.003%
46	9.484	2619	2626	2635	rBV8	3776	6543	0.29%	0.039%
47	9.699	2690	2693	2696	rBV	316	268	0.01%	0.002%
48	9.725	2696	2701	2705	rVV4	543	594	0.03%	0.004%
49	9.770	2713	2715	2720	rVB3	1032	675	0.03%	0.004%
50	9.799	2720	2724	2727	rBV3	1004	772	0.03%	0.005%
51	9.821	2727	2731	2734	rVV2	580	394	0.02%	0.002%
52	9.837	2734	2736	2742	rVB3	529	374	0.02%	0.002%
53	9.876	2742	2748	2750	rBV5	1032	938	0.04%	0.006%
54	9.931	2762	2765	2767	rVV2	618	329	0.01%	0.002%
55	9.947	2767	2770	2771	rVV3	292	182	0.01%	0.001%
56	10.037	2796	2798	2799	rBV	420	196	0.01%	0.001%
57	10.088	2810	2814	2816	rBV3	441	364	0.02%	0.002%
58	10.146	2820	2832	2856	rBV	594639	946140	41.30%	5.689%
59	10.304	2878	2881	2882	rBV3	925	523	0.02%	0.003%
60	10.519	2945	2948	2951	rBV3	725	609	0.03%	0.004%
61	10.561	2959	2961	2965	rBV3	654	445	0.02%	0.003%
62	10.590	2968	2970	2973	rVB	524	256	0.01%	0.002%
63	10.616	2976	2978	2980	rBV3	507	263	0.01%	0.002%
64	10.625	2980	2981	2984	rVB3	551	194	0.01%	0.001%
65	10.654	2987	2990	2992	rBV	570	380	0.02%	0.002%
66	10.702	3002	3005	3008	rVB4	522	306	0.01%	0.002%
67	10.728	3011	3013	3015	rBV4	825	432	0.02%	0.003%
68	10.779	3025	3029	3030	rBV3	920	628	0.03%	0.004%
69	10.818	3039	3041	3044	rVB3	702	377	0.02%	0.002%
70	10.857	3050	3053	3056	rBV4	1044	893	0.04%	0.005%
71	10.934	3075	3077	3081	rBV	412	321	0.01%	0.002%
72	10.960	3081	3085	3087	rVV3	859	569	0.02%	0.003%
73	10.979	3089	3091	3096	rVB2	527	392	0.02%	0.002%
74	11.005	3096	3099	3101	rBV2	409	228	0.01%	0.001%
75	11.017	3101	3103	3104	rBV	444	163	0.01%	0.001%
76	11.082	3116	3123	3125	rBV3	730	713	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037836.D
 Acq On : 11 Oct 2024 16:58
 Operator : SY/MD
 Sample : P4349-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.140	3137	3141	3142	rBV3	1119	724	0.03%	0.004%
78	11.178	3142	3153	3178	rBV	990244	1594980	69.63%	9.590%
79	11.455	3236	3239	3244	rBV6	1715	1825	0.08%	0.011%
80	11.554	3259	3270	3294	rBV	1032158	1661284	72.52%	9.989%
81	12.001	3407	3409	3411	rBV2	625	411	0.02%	0.002%
82	12.085	3432	3435	3438	rBV5	1086	776	0.03%	0.005%
83	12.268	3490	3492	3496	rVB3	1449	794	0.03%	0.005%
84	12.291	3496	3499	3501	rBV2	1150	589	0.03%	0.004%
85	12.394	3529	3531	3532	rBV2	508	188	0.01%	0.001%
86	12.519	3566	3570	3572	rBV4	765	531	0.02%	0.003%
87	12.596	3589	3594	3596	rBV4	1058	949	0.04%	0.006%
88	12.741	3636	3639	3642	rBV2	653	482	0.02%	0.003%
89	12.792	3653	3655	3657	rBV	400	172	0.01%	0.001%
90	12.837	3668	3669	3671	rBV	698	329	0.01%	0.002%
91	12.905	3687	3690	3692	rVB2	637	370	0.02%	0.002%
92	12.921	3692	3695	3698	rBV3	996	709	0.03%	0.004%
93	12.937	3698	3700	3704	rVB2	939	629	0.03%	0.004%
94	13.017	3722	3725	3726	rBV2	1163	544	0.02%	0.003%
95	13.313	3814	3817	3820	rBV2	667	492	0.02%	0.003%
96	13.345	3825	3827	3829	rBV	583	253	0.01%	0.002%
97	13.365	3829	3833	3835	rBV3	937	646	0.03%	0.004%
98	13.426	3849	3852	3854	rBV3	805	520	0.02%	0.003%
99	13.439	3854	3856	3858	rBV2	832	423	0.02%	0.003%
100	13.538	3885	3887	3890	rBV3	790	415	0.02%	0.002%




Sum of corrected areas: 16631466

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037836.D
Acq On : 11 Oct 2024 16:58
Operator : SY/MD
Sample : P4349-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

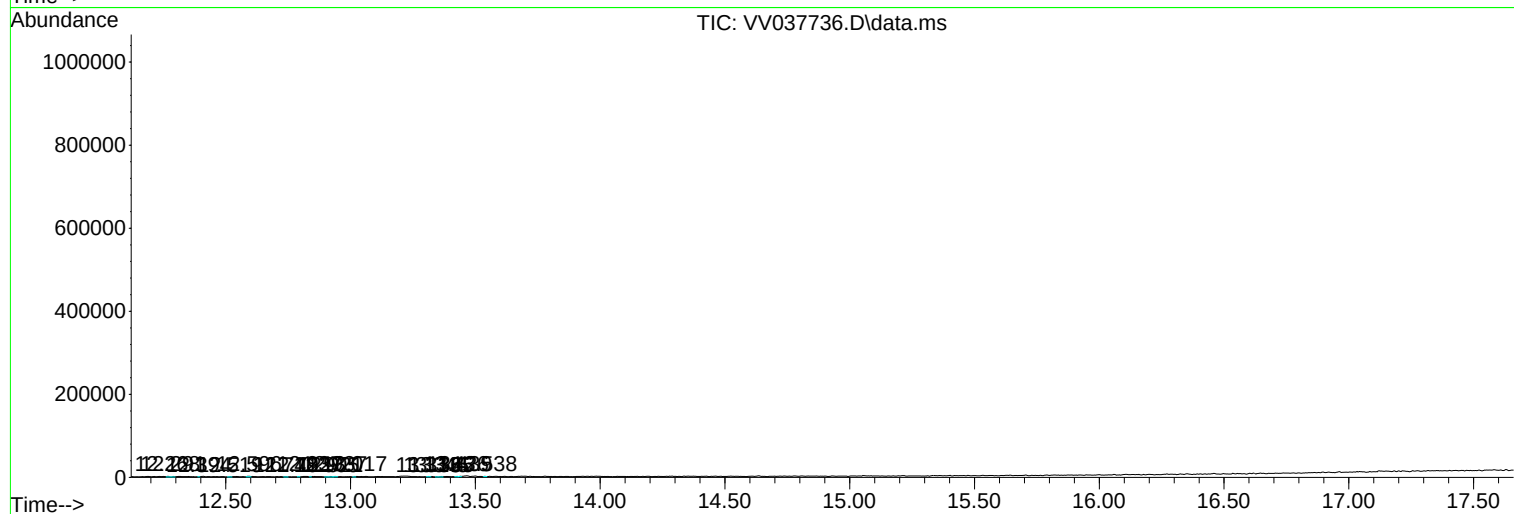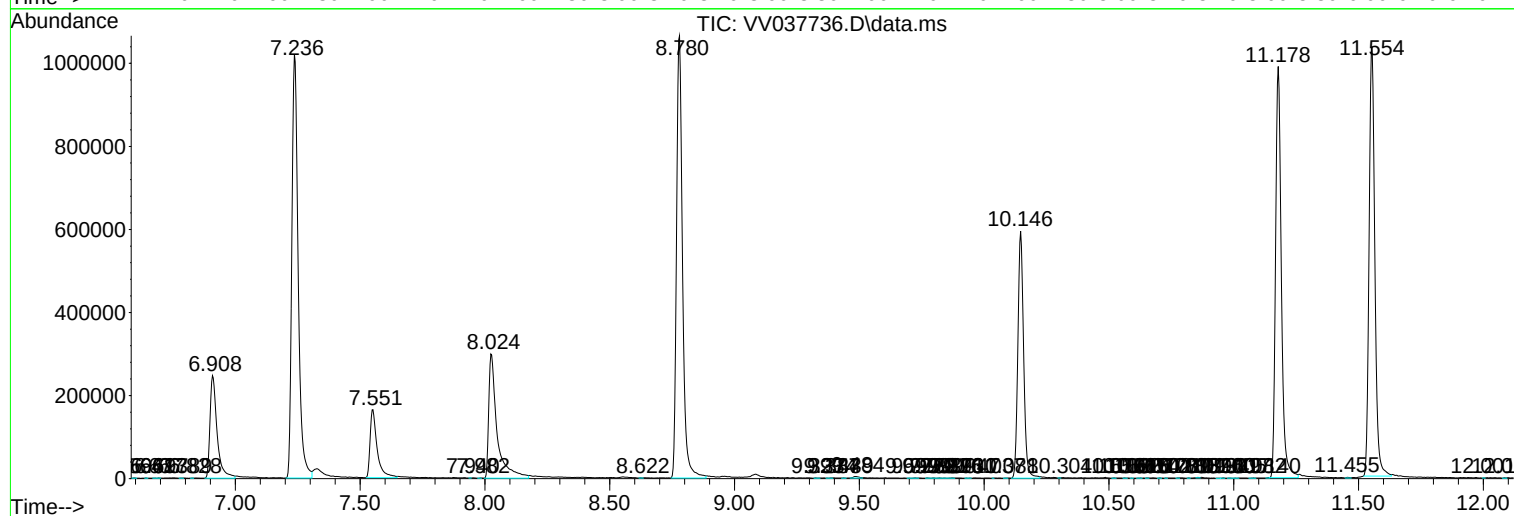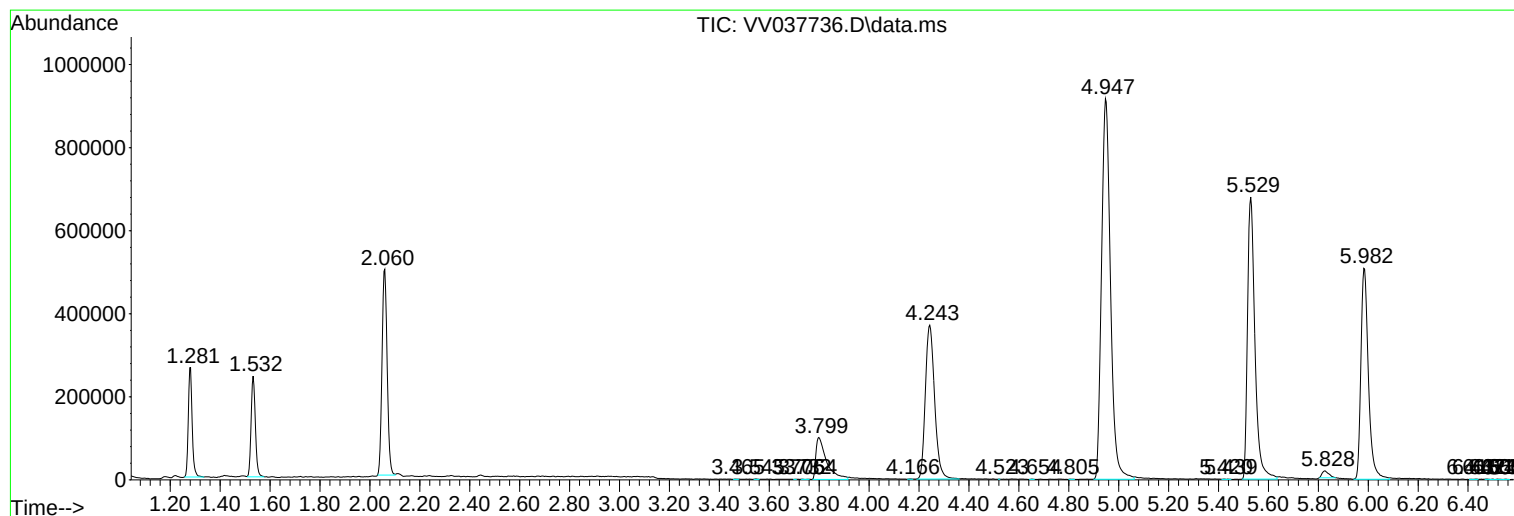

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037836.D
Acq On : 11 Oct 2024 16:58
Operator : SY/MD
Sample : P4349-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037836.D
Acq On : 11 Oct 2024 16:58
Operator : SY/MD
Sample : P4349-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------