

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037837.D
 Acq On : 11 Oct 2024 17:19
 Operator : SY/MD
 Sample : P4349-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037737.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	45	rBV	5521	6177	0.28%	0.038%
2	1.217	52	55	61	rBV3	3659	4195	0.19%	0.026%
3	1.278	68	74	89	rVB	254885	268562	12.31%	1.657%
4	1.413	112	116	124	rBV9	4071	5795	0.27%	0.036%
5	1.532	145	153	168	rVB	236607	274162	12.56%	1.692%
6	2.060	307	317	330	rBV	476496	687132	31.49%	4.240%
7	3.339	712	715	721	rVB4	658	702	0.03%	0.004%
8	3.513	764	769	772	rBV3	787	885	0.04%	0.005%
9	3.574	783	788	792	rBV3	870	953	0.04%	0.006%
10	3.799	847	858	895	rBV	97619	287312	13.17%	1.773%
11	4.095	947	950	952	rBV3	894	504	0.02%	0.003%
12	4.156	966	969	974	rBV4	702	526	0.02%	0.003%
13	4.243	978	996	1022	rBV	355047	913470	41.86%	5.636%
14	4.477	1067	1069	1074	rVB6	877	563	0.03%	0.003%
15	4.564	1092	1096	1099	rBV3	590	633	0.03%	0.004%
16	4.780	1159	1163	1168	rVB4	853	631	0.03%	0.004%
17	4.805	1168	1171	1175	rVB4	591	504	0.02%	0.003%
18	4.947	1199	1215	1263	rBV2	864221	2182279	100.00%	13.465%
19	5.198	1288	1293	1296	rBV4	919	944	0.04%	0.006%
20	5.278	1314	1318	1320	rBV3	740	513	0.02%	0.003%
21	5.329	1329	1334	1335	rBV4	1232	1052	0.05%	0.006%
22	5.529	1385	1396	1438	rBV	688087	1436798	65.84%	8.865%
23	5.828	1480	1489	1506	rVB3	14366	31704	1.45%	0.196%
24	5.982	1525	1537	1565	rBV	483609	1007756	46.18%	6.218%
25	6.146	1585	1588	1590	rBV3	1399	842	0.04%	0.005%
26	6.230	1612	1614	1618	rVB3	936	578	0.03%	0.004%
27	6.252	1618	1621	1624	rBV5	527	500	0.02%	0.003%
28	6.365	1653	1656	1659	rBV3	912	682	0.03%	0.004%
29	6.426	1672	1675	1681	rVB5	434	509	0.02%	0.003%
30	6.455	1681	1684	1685	rBV2	1115	595	0.03%	0.004%
31	6.481	1688	1692	1694	rVV4	935	756	0.03%	0.005%
32	6.725	1763	1768	1770	rVB3	640	537	0.02%	0.003%
33	6.754	1770	1777	1780	rBV6	1220	1430	0.07%	0.009%
34	6.799	1789	1791	1795	rVB3	866	630	0.03%	0.004%
35	6.908	1814	1825	1850	rBV	235028	461616	21.15%	2.848%
36	7.124	1890	1892	1897	rVB3	837	530	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037837.D
 Acq On : 11 Oct 2024 17:19
 Operator : SY/MD
 Sample : P4349-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.236	1916	1927	1958	rBV	946926	1698512	77.83%	10.480%
38	7.551	2016	2025	2053	rBV	158839	305258	13.99%	1.884%
39	7.773	2092	2094	2098	rVB5	861	603	0.03%	0.004%
40	7.799	2098	2102	2105	rBV3	770	549	0.03%	0.003%
41	8.027	2164	2173	2215	rBV2	277570	629776	28.86%	3.886%
42	8.484	2311	2315	2316	rBV2	688	492	0.02%	0.003%
43	8.551	2331	2336	2338	rBV3	2387	2187	0.10%	0.013%
44	8.776	2396	2406	2436	rBV	1087906	1803514	82.64%	11.128%
45	9.149	2516	2522	2524	rBV6	895	705	0.03%	0.004%
46	9.210	2538	2541	2543	rBV3	1079	654	0.03%	0.004%
47	9.220	2543	2544	2551	rVB3	1658	1044	0.05%	0.006%
48	9.259	2551	2556	2557	rBV2	759	489	0.02%	0.003%
49	9.291	2564	2566	2571	rVB4	704	497	0.02%	0.003%
50	9.542	2639	2644	2648	rBV3	605	533	0.02%	0.003%
51	9.628	2666	2671	2673	rBV3	549	481	0.02%	0.003%
52	9.741	2700	2706	2712	rBV5	872	782	0.04%	0.005%
53	9.773	2713	2716	2721	rBV3	771	742	0.03%	0.005%
54	9.879	2744	2749	2753	rVB4	865	946	0.04%	0.006%
55	9.985	2777	2782	2785	rBV6	602	567	0.03%	0.003%
56	10.008	2785	2789	2794	rVB4	584	531	0.02%	0.003%
57	10.072	2804	2809	2815	rVV4	827	690	0.03%	0.004%
58	10.146	2820	2832	2860	rBV	566516	908351	41.62%	5.605%
59	10.480	2932	2936	2937	rBV2	910	496	0.02%	0.003%
60	10.538	2951	2954	2956	rVV3	958	492	0.02%	0.003%
61	10.709	3000	3007	3009	rBV4	895	886	0.04%	0.005%
62	10.786	3028	3031	3038	rVV3	855	818	0.04%	0.005%
63	10.889	3058	3063	3067	rVB3	786	925	0.04%	0.006%
64	10.914	3067	3071	3073	rBV3	692	532	0.02%	0.003%
65	11.104	3124	3130	3132	rBV2	707	518	0.02%	0.003%
66	11.127	3132	3137	3141	rBV2	1213	1144	0.05%	0.007%
67	11.178	3141	3153	3183	rBV	1019356	1638978	75.10%	10.113%
68	11.403	3220	3223	3230	rVB6	1897	1735	0.08%	0.011%
69	11.551	3257	3269	3301	rBV	989116	1598895	73.27%	9.866%
70	11.937	3387	3389	3391	rBV2	878	486	0.02%	0.003%
71	11.966	3394	3398	3401	rVB3	989	834	0.04%	0.005%
72	12.030	3416	3418	3423	rBV	851	717	0.03%	0.004%
73	12.361	3514	3521	3522	rBV4	603	639	0.03%	0.004%
74	12.403	3531	3534	3537	rVB3	1103	664	0.03%	0.004%
75	12.422	3537	3540	3542	rBV2	749	483	0.02%	0.003%
76	12.548	3575	3579	3582	rBV4	799	502	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
 Data File : VV037837.D
 Acq On : 11 Oct 2024 17:19
 Operator : SY/MD
 Sample : P4349-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.725	3628	3634	3635	rBV4	773	729	0.03%	0.004%
78	12.795	3650	3656	3658	rBV3	587	592	0.03%	0.004%
79	12.905	3687	3690	3692	rBV2	1139	746	0.03%	0.005%
80	12.969	3705	3710	3714	rBV5	714	686	0.03%	0.004%
81	12.995	3714	3718	3721	rVV4	629	608	0.03%	0.004%
82	13.114	3752	3755	3758	rBV4	857	670	0.03%	0.004%
83	13.210	3782	3785	3789	rBV4	1078	716	0.03%	0.004%
84	13.284	3804	3808	3809	rBV2	723	498	0.02%	0.003%
85	13.326	3815	3821	3825	rBV6	881	940	0.04%	0.006%
86	13.551	3887	3891	3894	rBV2	980	869	0.04%	0.005%
87	13.664	3920	3926	3929	rBV4	884	1160	0.05%	0.007%
88	13.683	3929	3932	3933	rBV2	1246	576	0.03%	0.004%
89	13.779	3958	3962	3967	rBV4	881	695	0.03%	0.004%
90	13.847	3981	3983	3987	rBV2	723	532	0.02%	0.003%
91	13.963	4015	4019	4020	rBV4	920	530	0.02%	0.003%
92	14.046	4040	4045	4049	rBV4	693	743	0.03%	0.005%
93	14.358	4139	4142	4145	rBV2	774	546	0.03%	0.003%
94	14.519	4189	4192	4194	rBV2	910	667	0.03%	0.004%
95	14.696	4245	4247	4249	rBV3	790	486	0.02%	0.003%
96	14.731	4255	4258	4260	rBV	853	539	0.02%	0.003%
97	14.824	4284	4287	4290	rBV3	1139	881	0.04%	0.005%
98	14.898	4308	4310	4313	rBV3	813	558	0.03%	0.003%
99	14.966	4328	4331	4332	rBV2	922	538	0.02%	0.003%
100	15.487	4491	4493	4495	rBV4	1256	720	0.03%	0.004%




Sum of corrected areas: 16206829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037837.D
Acq On : 11 Oct 2024 17:19
Operator : SY/MD
Sample : P4349-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

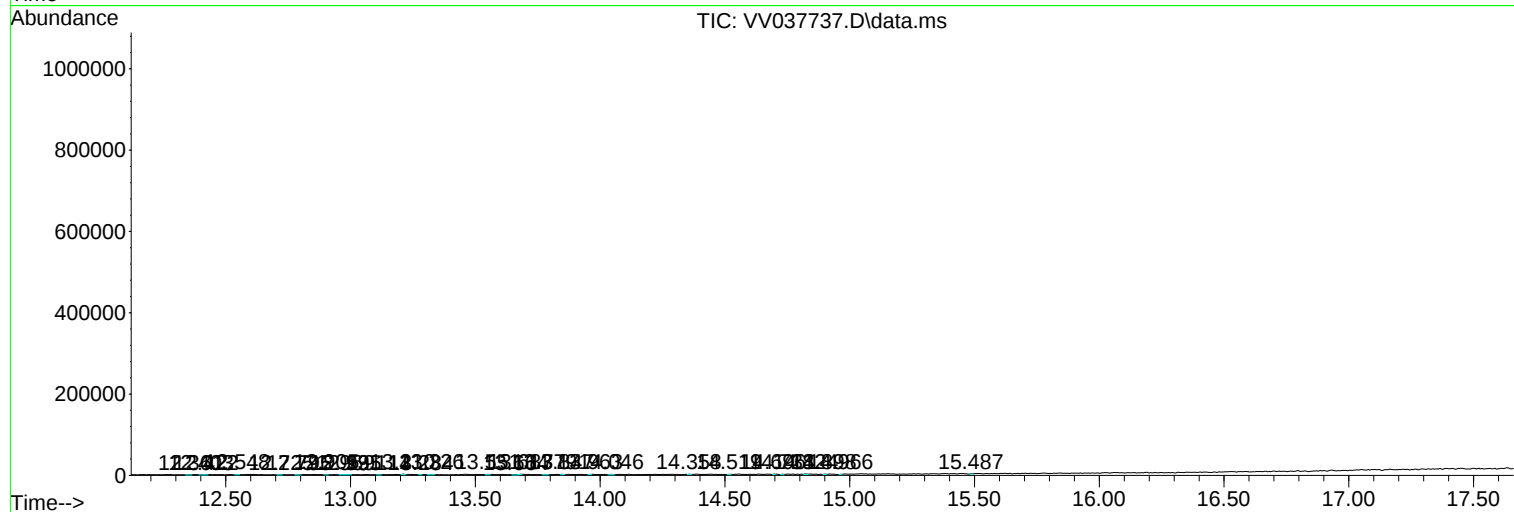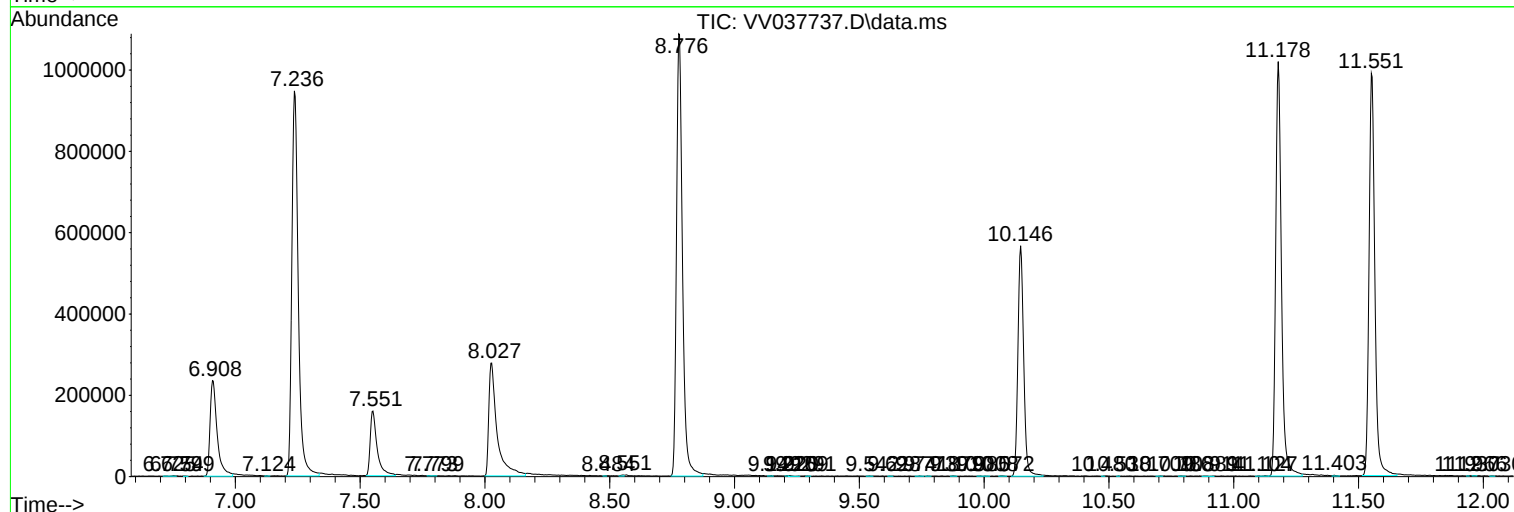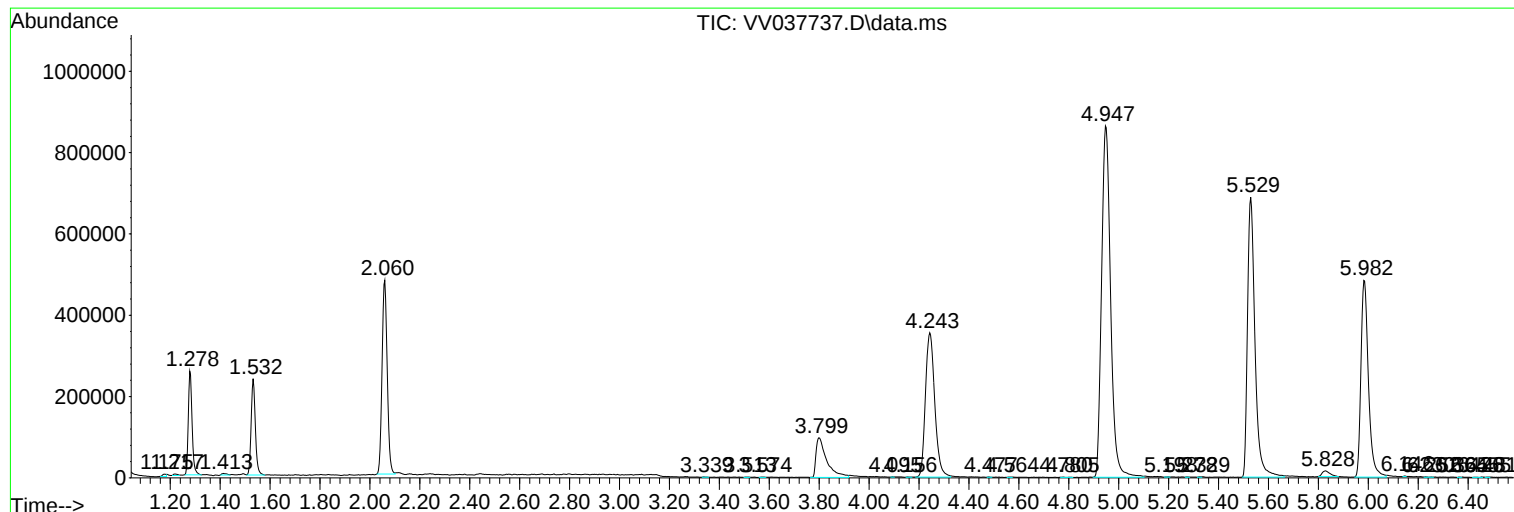

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037837.D
Acq On : 11 Oct 2024 17:19
Operator : SY/MD
Sample : P4349-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037837.D
Acq On : 11 Oct 2024 17:19
Operator : SY/MD
Sample : P4349-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc