
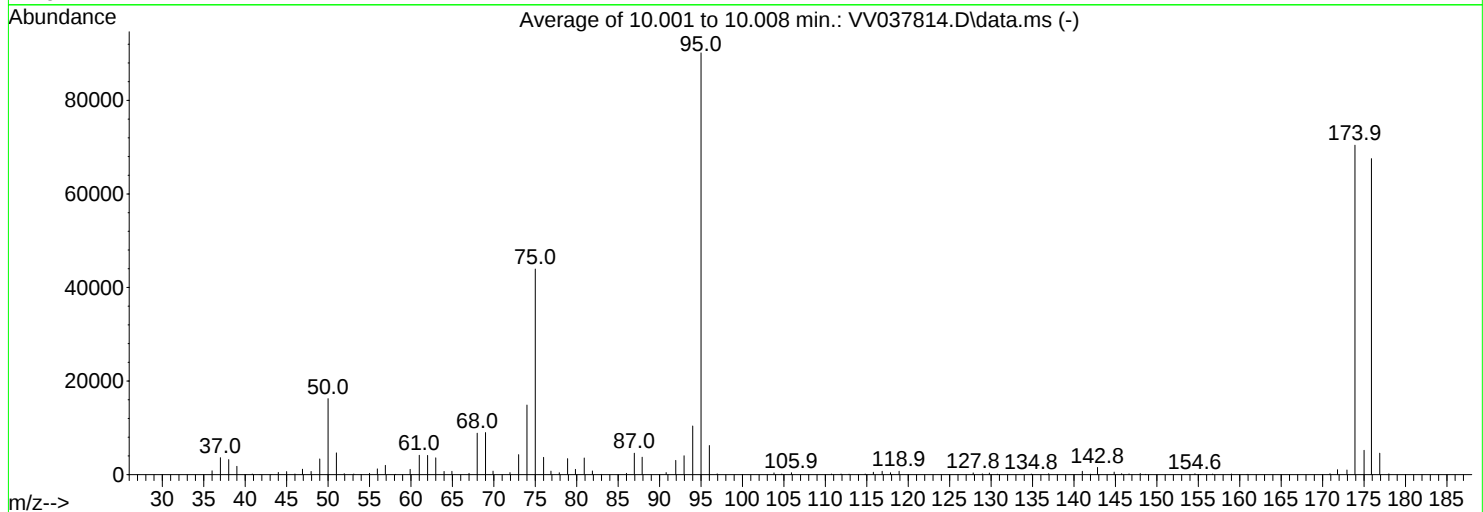


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101124\
Data File : VV037814.D
Acq On : 11 Oct 2024 08:38
Operator : SY/MD
Sample : BFB392
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB392

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Mon Oct 14 06:04:26 2024

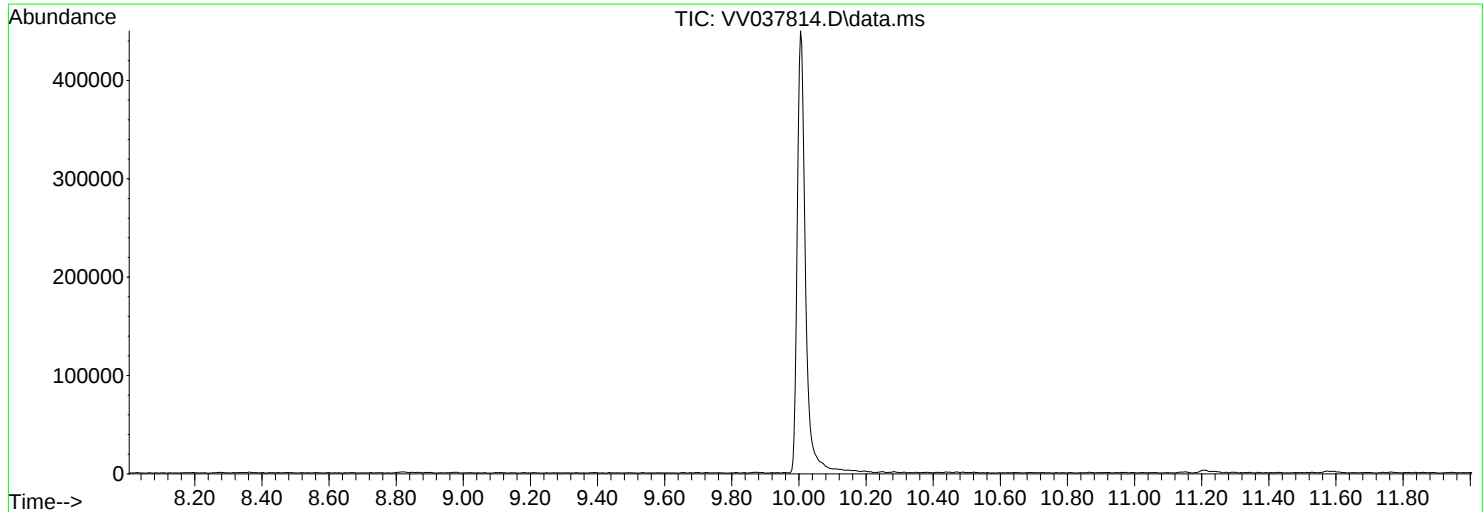

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	16260	PASS
75	95	30	80	48.7	43936	PASS
95	95	100	100	100.0	90155	PASS
96	95	5	9	6.9	6220	PASS
173	174	0.00	2	1.4	976	PASS
174	95	50	120	78.1	70424	PASS
175	174	5	9	7.4	5205	PASS
176	174	95	105	95.9	67557	PASS
177	176	5	10	6.8	4587	PASS

m/z	Abundance
39.90	317.0
44.00	583.0
45.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
36.00	786.0
37.00	3468.0
38.00	3219.0
39.00	1638.0
40.00	344.0
40.80	132.0
43.10	117.0
44.00	1105.0
45.00	718.0
46.00	112.0
46.90	1153.0
47.90	636.0
49.00	3390.0
50.00	15499.0
51.00	4642.0
51.90	196.0
53.10	157.0
54.00	102.0
55.00	323.0
55.90	1170.0
56.90	1843.0
59.90	1095.0
61.00	4102.0
62.00	4005.0
63.00	3743.0
64.00	687.0
64.90	707.0
67.00	275.0
68.00	8457.0
69.00	8716.0
69.90	758.0
72.00	480.0
73.00	4058.0
74.00	14091.0
75.00	42448.0
76.00	3479.0
76.90	701.0
77.90	505.0
78.90	3346.0
79.80	1027.0
80.90	3521.0
81.90	758.0
82.90	118.0
86.00	207.0
87.00	4233.0
87.90	3748.0
90.80	393.0
91.90	2975.0
93.00	3869.0
94.00	10184.0
95.00	87296.0
96.00	6282.0
96.90	171.0
103.80	397.0
104.80	178.0
105.90	386.0
110.70	108.0
111.90	156.0
112.90	138.0
114.80	110.0
115.80	533.0
116.90	599.0
117.80	417.0
118.90	729.0
127.80	371.0
129.00	128.0
129.80	299.0
130.80	130.0
134.90	153.0
137.00	219.0
141.00	695.0
142.80	1290.0
144.90	602.0
145.80	189.0
146.70	171.0
148.00	222.0
148.70	138.0
154.60	176.0
156.80	135.0
159.00	123.0
170.90	192.0
171.80	919.0
172.90	847.0
173.90	66672.0
175.00	5052.0
175.90	63544.0
176.90	4406.0
178.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
36.00	868.0
37.00	3815.0
38.00	3236.0
39.00	1862.0
40.00	334.0
40.90	148.0
41.80	104.0
44.00	1074.0
45.00	781.0
46.00	119.0
46.90	1226.0
47.90	670.0
49.00	3428.0
50.00	16872.0
51.00	4732.0
52.00	204.0
53.10	143.0
55.00	291.0
56.00	1266.0
56.90	2067.0
58.10	126.0
59.90	1195.0
61.00	4340.0
62.00	4181.0
63.00	3704.0
64.00	695.0
65.00	743.0
67.00	274.0
68.00	9147.0
69.00	9333.0
69.90	791.0
72.00	461.0
73.00	4415.0
74.00	15437.0
75.00	45384.0
76.00	3839.0
76.90	780.0
77.90	420.0
78.90	3465.0
79.80	1162.0
80.90	3645.0
81.90	805.0
83.00	111.0
86.00	296.0
87.00	4832.0
87.90	3869.0
90.80	444.0
91.90	3210.0
93.00	4198.0
94.00	10683.0
95.00	93360.0
96.00	6468.0
96.90	152.0
103.80	391.0
104.80	147.0
105.90	419.0
110.80	155.0
111.90	142.0
112.90	115.0
114.80	170.0
115.80	564.0
116.80	739.0
117.80	435.0
118.90	741.0
127.90	386.0
129.00	164.0
129.80	356.0
130.80	109.0
134.90	159.0
137.00	197.0
141.00	709.0
142.00	115.0
142.90	1596.0
144.90	581.0
145.80	225.0
146.70	185.0
148.00	254.0
148.60	122.0
154.60	214.0
155.30	114.0
156.80	146.0
159.00	163.0
160.90	121.0
170.90	201.0
171.80	1104.0
173.00	984.0
173.90	72616.0
175.00	5417.0
175.90	69824.0
176.90	4732.0
178.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392

m/z	Abundance
36.00	809.0
37.00	3625.0
38.00	3156.0
39.00	1813.0
40.00	321.0
40.90	135.0
44.00	962.0
45.00	760.0
46.00	169.0
46.90	1123.0
48.00	701.0
49.00	3196.0
50.00	16408.0
51.00	4565.0
52.00	221.0
53.10	120.0
55.00	236.0
56.00	1234.0
56.90	2067.0
58.10	123.0
59.90	1070.0
61.00	3947.0
62.00	4089.0
63.00	3347.0
64.00	693.0
65.00	759.0
67.00	235.0
68.00	8949.0
69.00	8969.0
69.90	697.0
71.90	430.0
73.00	4382.0
74.00	15106.0
75.00	43976.0
76.00	3730.0
76.90	814.0
77.90	367.0
78.90	3458.0
79.90	1193.0
80.90	3475.0
81.90	771.0
86.00	303.0
86.90	4720.0
87.90	3595.0
90.80	490.0
92.00	2986.0
92.90	3993.0
94.00	10355.0
95.00	89808.0
96.00	5911.0
97.00	163.0
103.80	368.0
104.70	125.0
105.90	382.0
108.00	119.0
110.70	148.0
111.90	111.0
112.80	108.0
114.80	184.0
115.80	467.0
116.90	787.0
117.90	409.0
118.90	692.0
127.80	384.0
128.90	191.0
129.80	383.0
130.70	127.0
134.80	142.0
136.80	165.0
141.00	738.0
142.00	172.0
142.90	1690.0
144.80	505.0
145.70	207.0
146.60	132.0
148.00	278.0
153.90	100.0
154.60	206.0
156.70	180.0
159.00	153.0
160.90	127.0
170.90	187.0
171.80	1122.0
173.00	1098.0
173.90	71984.0
175.00	5147.0
175.90	69304.0
176.90	4622.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB392