

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
 Data File : VV037863.D
 Acq On : 15 Oct 2024 10:20
 Operator : SY/MD
 Sample : VV1015WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 16 03:30:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 16 03:26:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	534026	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	527465	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	244499	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	226076	48.225	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	96.460%	
7) Chloroethane-d5	1.532	69	193560	53.193	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	106.380%	
11) 1,1-Dichloroethene-d2	2.060	65	101741	51.947	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	103.900%	
21) 2-Butanone-d5	3.796	46	142185	85.154	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.150%	
24) Chloroform-d	4.243	84	437985	52.514	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.020%	
26) 1,2-Dichloroethane-d4	4.937	65	260823	53.428	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.860%	
32) Benzene-d6	4.953	84	885596	53.655	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	107.300%	
36) 1,2-Dichloropropane-d6	5.982	67	279770	53.231	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.460%	
41) Toluene-d8	7.236	98	772081	51.587	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.180%	
43) trans-1,3-Dichloroprop...	7.548	79	111815	45.797	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	91.600%	
47) 2-Hexanone-d5	8.024	63	92745	83.568	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	83.570%	
56) 1,1,2,2-Tetrachloroeth...	10.143	84	289109	47.342	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.680%	
66) 1,2-Dichlorobenzene-d4	11.551	152	284666	55.253	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	110.500%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3202	0.841	ug/L	Qvalue # 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037863.D
Acq On : 15 Oct 2024 10:20
Operator : SY/MD
Sample : VV1015WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 16 03:30:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 16 03:26:57 2024
Response via : Initial Calibration

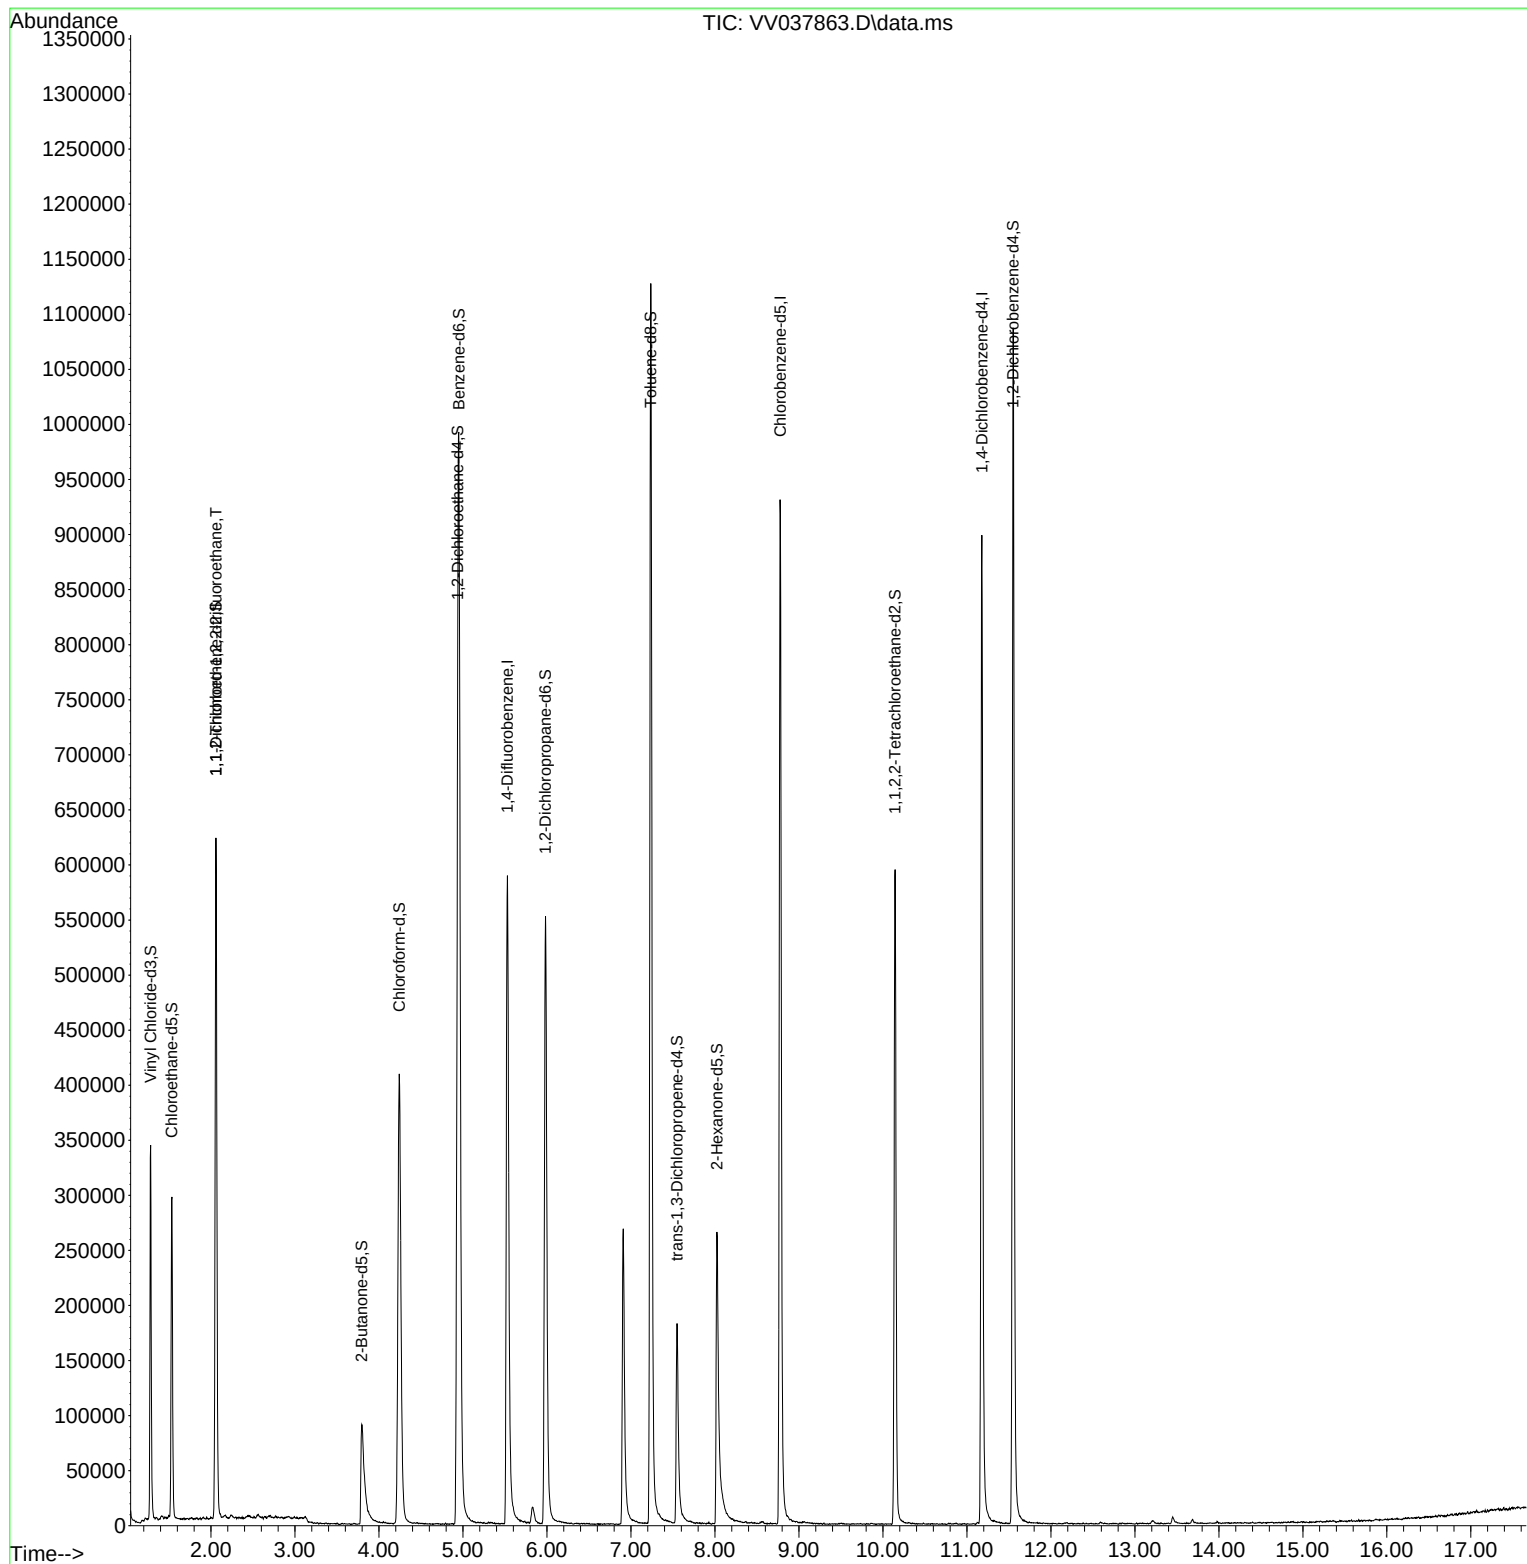

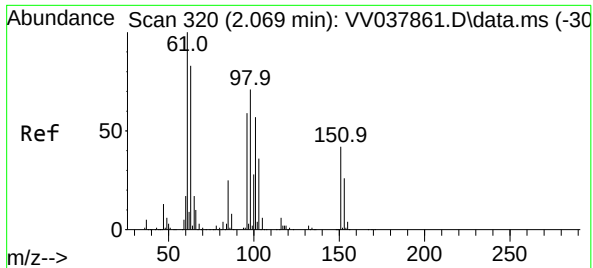

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.841 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV037863.D
 Acq: 15 Oct 2024 10:20

Instrument :
 MSVOA_V
 ClientSampleId :

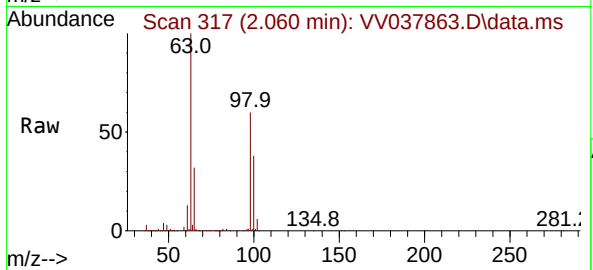

Tgt Ion:	101	Resp:	3202
Ion	Ratio	Lower	Upper
101	100		
85	2.8	34.6	52.0#
151	4.0	57.5	86.3#

