

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
 Data File : VV037864.D
 Acq On : 15 Oct 2024 10:59
 Operator : SY/MD
 Sample : VV1015WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	410810	435796	14.68%	2.409%
2	1.532	146	153	167	rVB	360643	416444	14.02%	2.302%
3	2.059	307	317	333	rBV	713397	1031279	34.73%	5.701%
4	3.465	752	754	757	rVB3	679	399	0.01%	0.002%
5	3.548	778	780	783	rBV2	448	259	0.01%	0.001%
6	3.632	802	806	807	rBV	496	340	0.01%	0.002%
7	3.690	823	824	828	rVB	563	287	0.01%	0.002%
8	3.712	828	831	834	rBV	354	319	0.01%	0.002%
9	3.792	847	856	884	rBV	99384	282701	9.52%	1.563%
10	4.239	977	995	1028	rBV	474584	1219226	41.06%	6.740%
11	4.526	1080	1084	1085	rBV4	583	354	0.01%	0.002%
12	4.603	1106	1108	1110	rBV2	485	182	0.01%	0.001%
13	4.638	1114	1119	1121	rBV4	715	718	0.02%	0.004%
14	4.719	1139	1144	1147	rVB3	1031	938	0.03%	0.005%
15	4.735	1147	1149	1150	rBV	317	96	0.00%	0.001%
16	4.747	1150	1153	1156	rBV3	562	319	0.01%	0.002%
17	4.770	1156	1160	1162	rBV2	678	713	0.02%	0.004%
18	4.834	1176	1180	1182	rBV3	347	204	0.01%	0.001%
19	4.857	1184	1187	1188	rBV	567	265	0.01%	0.001%
20	4.944	1199	1214	1262	rBV2	1167627	2969330	100.00%	16.414%
21	5.294	1320	1323	1325	rBV3	1059	785	0.03%	0.004%
22	5.362	1342	1344	1345	rBV2	728	300	0.01%	0.002%
23	5.400	1353	1356	1359	rVB3	717	398	0.01%	0.002%
24	5.526	1385	1395	1432	rBV	436753	915223	30.82%	5.059%
25	5.828	1478	1489	1500	rBV5	14660	34881	1.17%	0.193%
26	5.979	1523	1536	1582	rBV	649244	1353849	45.59%	7.484%
27	6.362	1652	1655	1657	rBV3	574	297	0.01%	0.002%
28	6.381	1659	1661	1665	rVB3	906	453	0.02%	0.003%
29	6.410	1668	1670	1675	rVB3	673	518	0.02%	0.003%
30	6.461	1683	1686	1688	rBV2	1010	600	0.02%	0.003%
31	6.554	1713	1715	1716	rBV2	309	95	0.00%	0.001%
32	6.571	1716	1720	1724	rVB4	665	641	0.02%	0.004%
33	6.599	1724	1729	1730	rBV4	384	283	0.01%	0.002%
34	6.728	1767	1769	1770	rBV	472	262	0.01%	0.001%
35	6.786	1785	1787	1792	rVB2	1176	829	0.03%	0.005%
36	6.821	1792	1798	1800	rBV2	666	582	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037864.D
Acq On : 15 Oct 2024 10:59
Operator : SY/MD
Sample : VV1015WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

37	6.857	1807	1809	1811	rBV2	398	256	0.01%	0.001%
38	6.905	1814	1824	1864	rBV	323162	626186	21.09%	3.462%
39	7.233	1915	1926	1959	rBV	1343880	2367724	79.74%	13.089%
40	7.545	2015	2023	2045	rBV	214131	393595	13.26%	2.176%
41	7.950	2145	2149	2151	rBV3	769	613	0.02%	0.003%
42	8.024	2163	2172	2217	rBV2	291925	665394	22.41%	3.678%
43	8.776	2396	2406	2434	rBV	697597	1186051	39.94%	6.557%
44	9.233	2545	2548	2549	rBV2	258	161	0.01%	0.001%
45	9.249	2550	2553	2556	rVV3	693	482	0.02%	0.003%
46	9.310	2567	2572	2574	rBV3	448	408	0.01%	0.002%
47	9.349	2581	2584	2586	rVB2	493	240	0.01%	0.001%
48	9.365	2586	2589	2594	rVB3	606	569	0.02%	0.003%
49	9.390	2594	2597	2600	rBV4	546	392	0.01%	0.002%
50	9.419	2603	2606	2608	rBV2	577	341	0.01%	0.002%
51	9.451	2612	2616	2618	rBV	761	512	0.02%	0.003%
52	9.496	2627	2630	2632	rBV2	765	582	0.02%	0.003%
53	9.548	2644	2646	2647	rBV	597	228	0.01%	0.001%
54	9.628	2668	2671	2674	rBV2	423	318	0.01%	0.002%
55	9.667	2682	2683	2684	rBV	366	82	0.00%	0.000%
56	9.709	2692	2696	2698	rBV3	587	385	0.01%	0.002%
57	9.783	2717	2719	2720	rBV	315	107	0.00%	0.001%
58	9.840	2734	2737	2740	rBV2	664	528	0.02%	0.003%
59	9.860	2740	2743	2746	rVV4	896	511	0.02%	0.003%
60	9.876	2746	2748	2754	rVB2	1070	787	0.03%	0.004%
61	9.902	2754	2756	2757	rBV	330	131	0.00%	0.001%
62	9.911	2757	2759	2762	rVV2	286	147	0.00%	0.001%
63	9.931	2762	2765	2768	rVB3	456	324	0.01%	0.002%
64	9.979	2777	2780	2785	rBV2	595	625	0.02%	0.003%
65	10.027	2792	2795	2798	rVB4	616	404	0.01%	0.002%
66	10.143	2819	2831	2859	rBV	647678	1050741	35.39%	5.809%
67	10.377	2902	2904	2908	rVB3	1013	635	0.02%	0.004%
68	10.400	2908	2911	2914	rBV2	842	751	0.03%	0.004%
69	10.429	2918	2920	2921	rBV	379	160	0.01%	0.001%
70	10.490	2937	2939	2940	rBV	454	159	0.01%	0.001%
71	10.522	2947	2949	2954	rVB3	541	341	0.01%	0.002%
72	10.551	2954	2958	2961	rBV4	510	512	0.02%	0.003%
73	10.570	2961	2964	2968	rVB3	613	383	0.01%	0.002%
74	10.593	2969	2971	2978	rVB4	659	639	0.02%	0.004%
75	10.625	2978	2981	2983	rBV3	537	379	0.01%	0.002%
76	10.686	2997	3000	3002	rBV2	347	212	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037864.D
Acq On : 15 Oct 2024 10:59
Operator : SY/MD
Sample : VV1015WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	10.699	3002	3004	3006	rBV2	366	157	0.01%	0.001%
78	10.744	3015	3018	3022	rBV3	637	570	0.02%	0.003%
79	10.763	3022	3024	3026	rVV	562	262	0.01%	0.001%
80	10.831	3043	3045	3047	rVB	269	105	0.00%	0.001%
81	10.840	3047	3048	3051	rVB2	434	146	0.00%	0.001%
82	10.866	3051	3056	3062	rBV4	1119	1626	0.05%	0.009%
83	10.895	3062	3065	3067	rBV2	549	278	0.01%	0.002%
84	10.927	3073	3075	3076	rBV2	197	101	0.00%	0.001%
85	10.940	3077	3079	3084	rVV2	560	371	0.01%	0.002%
86	11.011	3098	3101	3102	rBV2	584	323	0.01%	0.002%
87	11.020	3102	3104	3105	rVV2	413	155	0.01%	0.001%
88	11.049	3111	3113	3117	rBV3	298	240	0.01%	0.001%
89	11.072	3117	3120	3124	rBV2	616	478	0.02%	0.003%
90	11.120	3132	3135	3137	rBV3	827	573	0.02%	0.003%
91	11.178	3143	3153	3190	rBV	668483	1081241	36.41%	5.977%
92	11.551	3257	3269	3300	rBV	1264608	2023165	68.14%	11.184%
93	11.901	3375	3378	3380	rBV3	925	688	0.02%	0.004%
94	12.075	3430	3432	3434	rBV2	638	407	0.01%	0.002%
95	12.377	3524	3526	3527	rBV	524	182	0.01%	0.001%
96	12.664	3612	3615	3618	rBV3	857	378	0.01%	0.002%
97	13.291	3808	3810	3815	rVB3	584	480	0.02%	0.003%
98	13.458	3856	3862	3865	rBV6	2937	3312	0.11%	0.018%
99	13.612	3902	3910	3913	rBV4	1047	1292	0.04%	0.007%




Sum of corrected areas: 18089690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037864.D
Acq On : 15 Oct 2024 10:59
Operator : SY/MD
Sample : VV1015WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

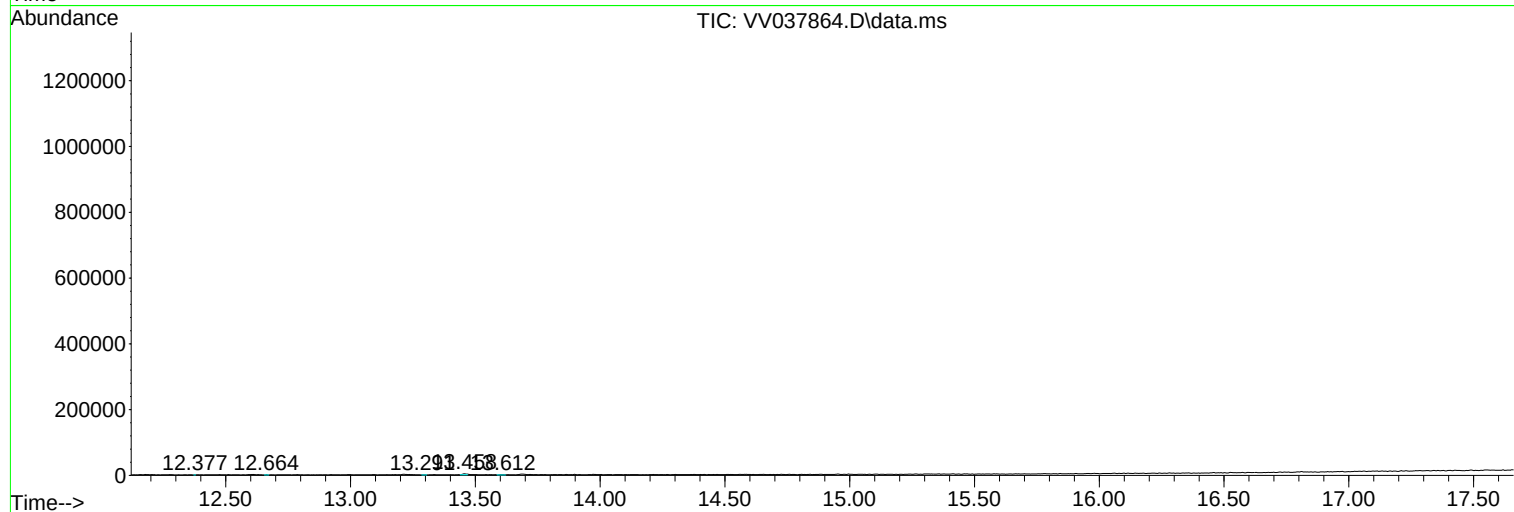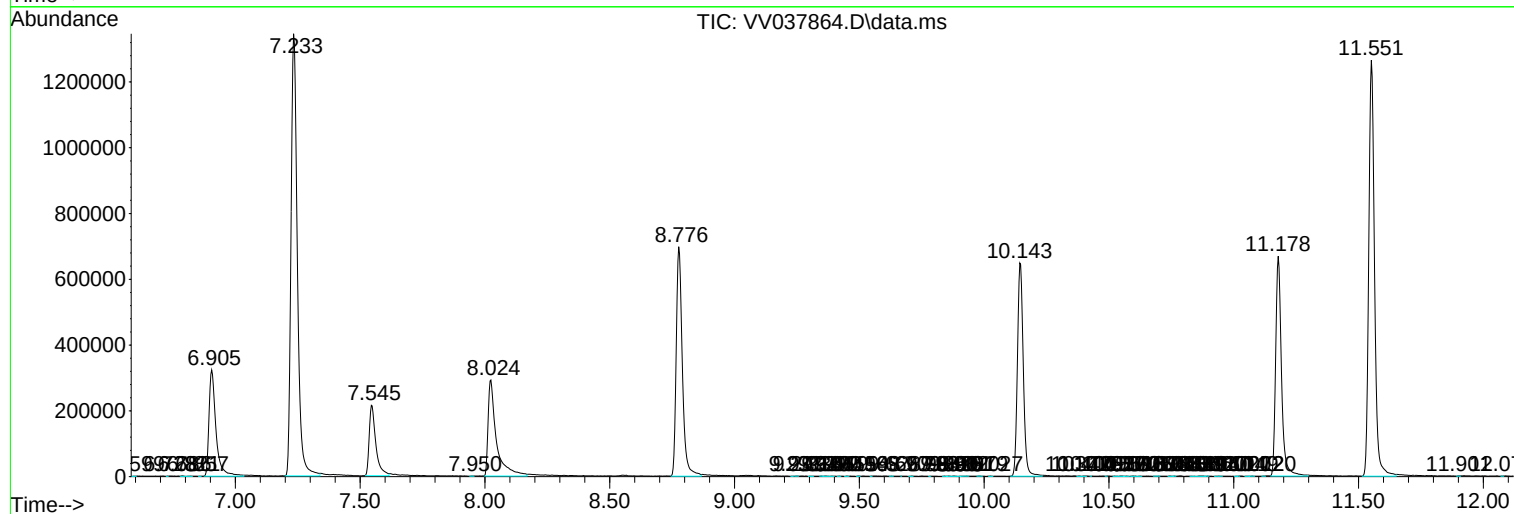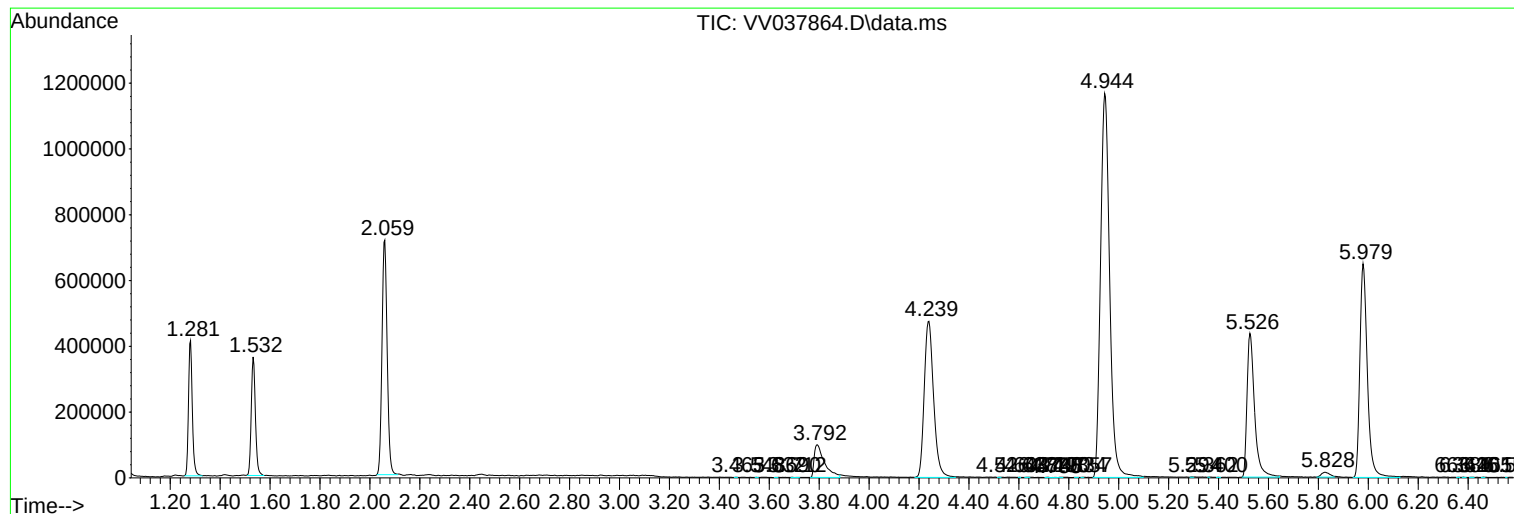

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037864.D
Acq On : 15 Oct 2024 10:59
Operator : SY/MD
Sample : VV1015WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037864.D
Acq On : 15 Oct 2024 10:59
Operator : SY/MD
Sample : VV1015WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK246

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------