

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
 Data File : VV037867.D
 Acq On : 15 Oct 2024 13:30
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037867.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	317901	337114	14.04%	2.030%
2	1.535	146	154	169	rVB	274753	324824	13.53%	1.956%
3	2.063	308	318	342	rVB	575820	845968	35.25%	5.095%
4	3.317	706	708	712	rBV	823	474	0.02%	0.003%
5	3.510	765	768	771	rBV4	720	475	0.02%	0.003%
6	3.625	801	804	806	rBV2	471	333	0.01%	0.002%
7	3.657	810	814	821	rVV3	687	833	0.03%	0.005%
8	3.735	836	838	841	rBV2	288	168	0.01%	0.001%
9	3.799	850	858	892	rBV	93704	275515	11.48%	1.659%
10	4.246	980	997	1025	rBV	384167	994446	41.43%	5.989%
11	4.612	1108	1111	1112	rBV	690	340	0.01%	0.002%
12	4.648	1119	1122	1125	rBV3	1012	576	0.02%	0.003%
13	4.741	1149	1151	1152	rVB2	301	87	0.00%	0.001%
14	4.767	1155	1159	1162	rVB	957	662	0.03%	0.004%
15	4.786	1162	1165	1166	rBV2	605	261	0.01%	0.002%
16	4.799	1167	1169	1172	rVB3	648	309	0.01%	0.002%
17	4.950	1198	1216	1248	rBV2	954400	2400249	100.00%	14.455%
18	5.445	1367	1370	1373	rBV4	598	482	0.02%	0.003%
19	5.529	1385	1396	1435	rBV	586833	1236638	51.52%	7.448%
20	5.831	1481	1490	1505	rVB4	13796	28649	1.19%	0.173%
21	5.985	1524	1538	1567	rBV	528158	1098080	45.75%	6.613%
22	6.255	1620	1622	1626	rVB4	540	357	0.01%	0.002%
23	6.336	1644	1647	1649	rVB3	789	351	0.01%	0.002%
24	6.352	1650	1652	1655	rVV2	559	255	0.01%	0.002%
25	6.436	1676	1678	1682	rBV3	850	840	0.03%	0.005%
26	6.551	1711	1714	1717	rBV3	586	287	0.01%	0.002%
27	6.564	1717	1718	1720	rVV	265	92	0.00%	0.001%
28	6.603	1727	1730	1734	rVB3	1184	795	0.03%	0.005%
29	6.622	1734	1736	1738	rBV	713	365	0.02%	0.002%
30	6.741	1771	1773	1774	rBV	453	140	0.01%	0.001%
31	6.796	1789	1790	1798	rVB4	729	515	0.02%	0.003%
32	6.825	1798	1799	1801	rVB	353	72	0.00%	0.000%
33	6.844	1803	1805	1811	rVB3	389	338	0.01%	0.002%
34	6.908	1815	1825	1857	rBV	259009	502889	20.95%	3.029%
35	7.236	1916	1927	1968	rBV	1062385	1908121	79.50%	11.491%
36	7.551	2016	2025	2050	rBV	176981	326371	13.60%	1.966%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
 Data File : VV037867.D
 Acq On : 15 Oct 2024 13:30
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.898	2130	2133	2135	rBV2	931	668	0.03%	0.004%
38	7.953	2147	2150	2151	rBV2	387	230	0.01%	0.001%
39	7.969	2153	2155	2162	rVB6	1182	1257	0.05%	0.008%
40	8.024	2162	2172	2212	rBV2	278624	643904	26.83%	3.878%
41	8.779	2396	2407	2443	rBV	941917	1583680	65.98%	9.538%
42	9.249	2550	2553	2559	rBV5	864	945	0.04%	0.006%
43	9.278	2559	2562	2564	rBV2	597	402	0.02%	0.002%
44	9.316	2571	2574	2577	rBV3	696	420	0.02%	0.003%
45	9.336	2578	2580	2584	rVB3	681	353	0.01%	0.002%
46	9.358	2584	2587	2589	rBV3	787	466	0.02%	0.003%
47	9.451	2613	2616	2620	rVB2	624	370	0.02%	0.002%
48	9.474	2620	2623	2626	rBV3	558	366	0.02%	0.002%
49	9.535	2638	2642	2643	rBV2	470	320	0.01%	0.002%
50	9.558	2647	2649	2653	rBV2	594	491	0.02%	0.003%
51	9.577	2653	2655	2658	rBV2	494	283	0.01%	0.002%
52	9.673	2683	2685	2687	rVB2	281	116	0.00%	0.001%
53	9.699	2687	2693	2695	rBV3	798	970	0.04%	0.006%
54	9.747	2701	2708	2711	rBV4	748	848	0.04%	0.005%
55	9.799	2722	2724	2728	rVB4	472	278	0.01%	0.002%
56	9.828	2731	2733	2735	rVB2	435	161	0.01%	0.001%
57	9.863	2742	2744	2748	rBV2	766	417	0.02%	0.003%
58	9.882	2748	2750	2752	rBV2	353	206	0.01%	0.001%
59	9.914	2759	2760	2762	rVB2	661	161	0.01%	0.001%
60	9.979	2778	2780	2782	rBV2	269	118	0.00%	0.001%
61	9.992	2782	2784	2788	rVB2	572	371	0.02%	0.002%
62	10.021	2788	2793	2794	rBV	590	505	0.02%	0.003%
63	10.069	2805	2808	2810	rBV	374	252	0.01%	0.002%
64	10.098	2815	2817	2820	rBV2	281	130	0.01%	0.001%
65	10.146	2820	2832	2859	rBV	591003	937609	39.06%	5.647%
66	10.323	2885	2887	2890	rBV3	703	363	0.02%	0.002%
67	10.368	2900	2901	2904	rVB3	675	313	0.01%	0.002%
68	10.397	2908	2910	2912	rBV2	548	293	0.01%	0.002%
69	10.439	2922	2923	2924	rBV	367	117	0.00%	0.001%
70	10.467	2929	2932	2934	rBV	412	285	0.01%	0.002%
71	10.496	2938	2941	2942	rBV	749	437	0.02%	0.003%
72	10.583	2966	2968	2970	rBV	575	223	0.01%	0.001%
73	10.612	2975	2977	2978	rBV	412	188	0.01%	0.001%
74	10.738	3014	3016	3019	rBV2	677	408	0.02%	0.002%
75	10.789	3031	3032	3036	rVB2	741	378	0.02%	0.002%
76	10.892	3059	3064	3065	rBV3	647	452	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
 Data File : VV037867.D
 Acq On : 15 Oct 2024 13:30
 Operator : SY/MD
 Sample : P4379-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	11.072	3116	3120	3121	rBV	524	310	0.01%	0.002%
78	11.082	3121	3123	3127	rVV3	700	520	0.02%	0.003%
79	11.178	3142	3153	3183	rBV	904493	1449323	60.38%	8.728%
80	11.551	3258	3269	3299	rBV	1044018	1682198	70.08%	10.131%
81	12.033	3417	3419	3422	rVB	850	354	0.01%	0.002%
82	12.104	3436	3441	3442	rBV3	854	680	0.03%	0.004%
83	12.172	3460	3462	3465	rBV2	683	456	0.02%	0.003%
84	12.429	3540	3542	3544	rBV2	530	225	0.01%	0.001%
85	12.461	3550	3552	3554	rBV2	642	315	0.01%	0.002%
86	13.040	3730	3732	3734	rBV2	459	200	0.01%	0.001%
87	13.130	3755	3760	3765	rBV5	837	1147	0.05%	0.007%
88	13.268	3801	3803	3806	rBV3	704	486	0.02%	0.003%
89	13.339	3823	3825	3829	rBV4	662	419	0.02%	0.003%




Sum of corrected areas: 16604658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037867.D
Acq On : 15 Oct 2024 13:30
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

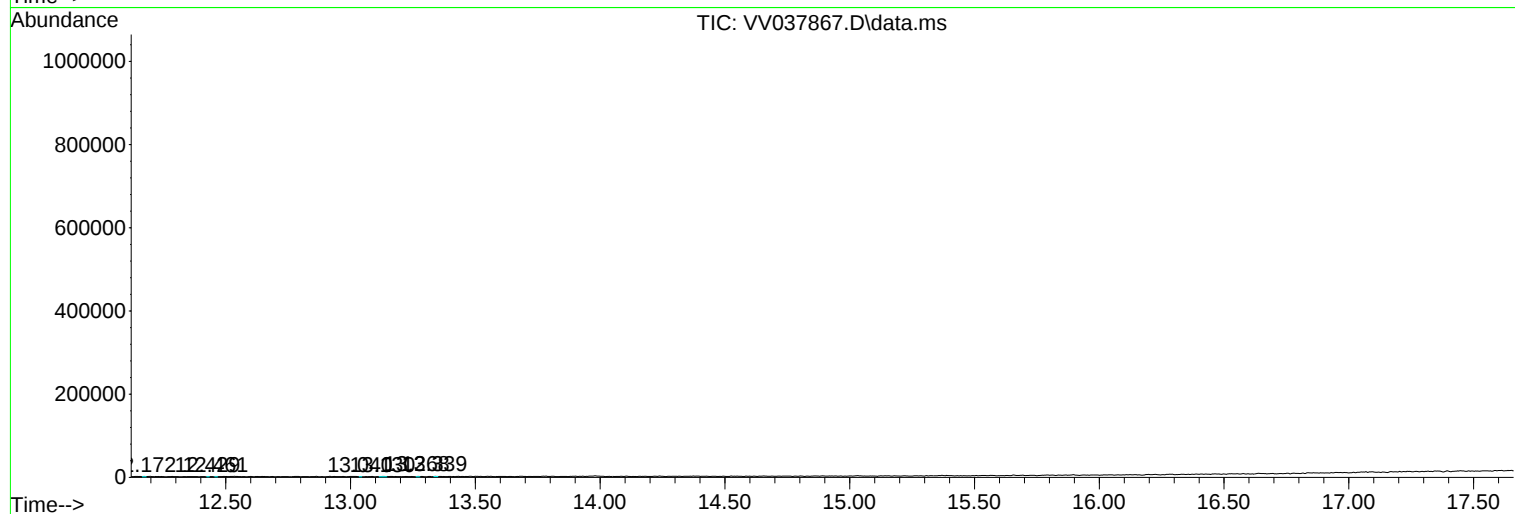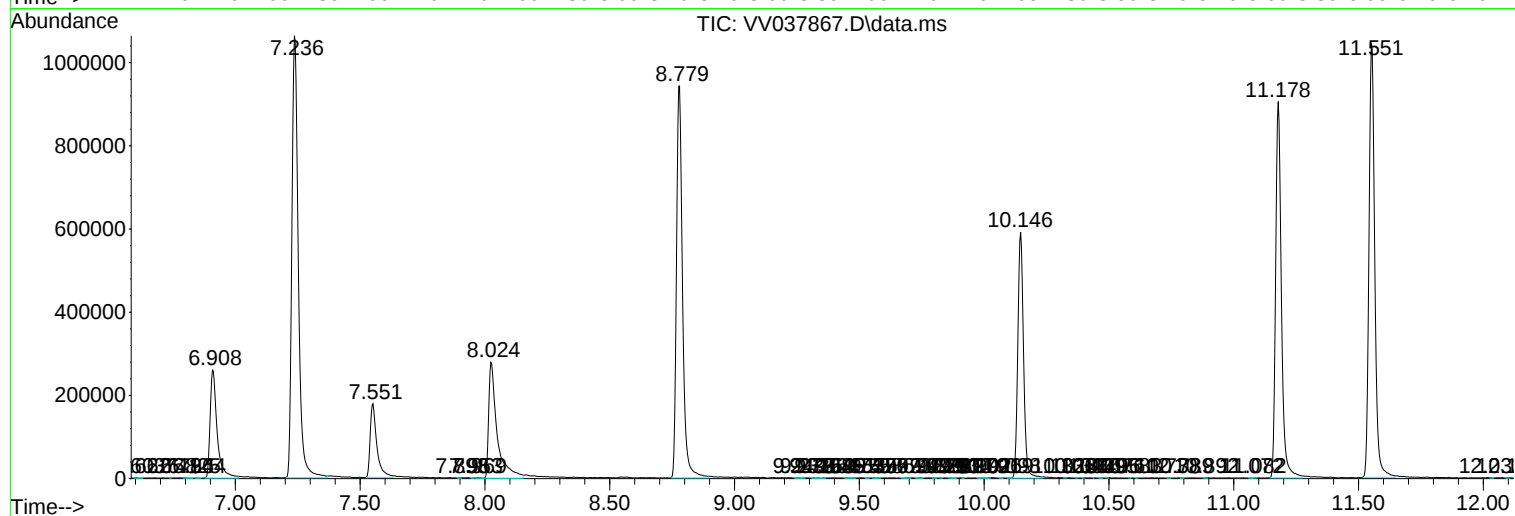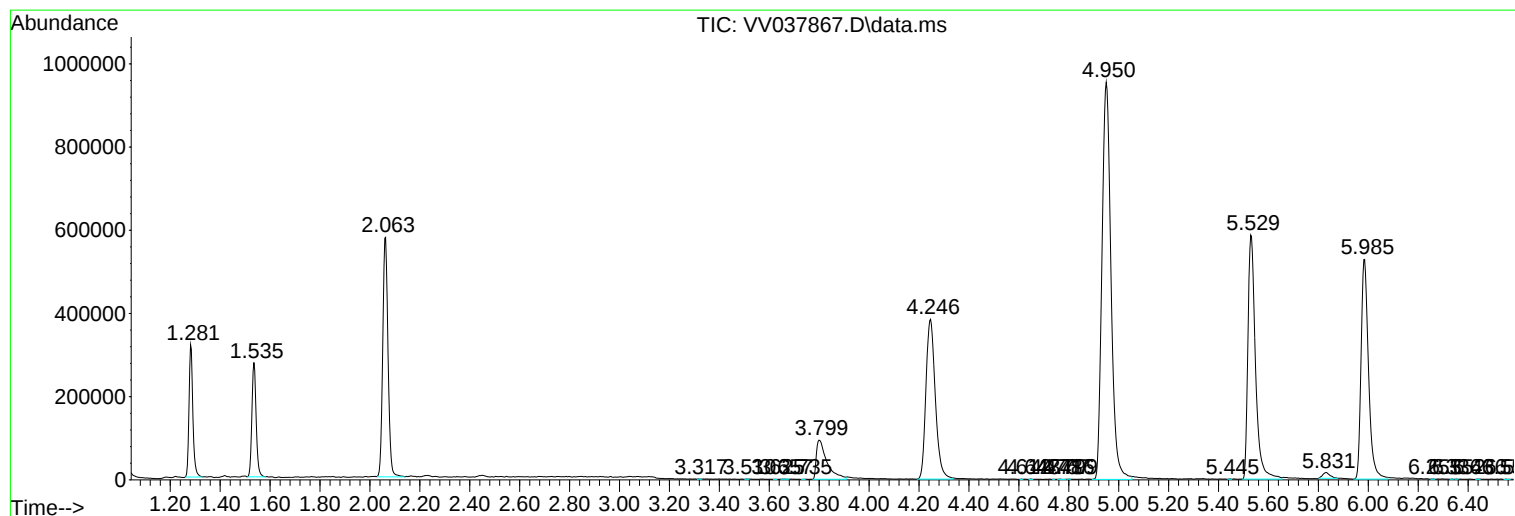

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037867.D
Acq On : 15 Oct 2024 13:30
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037867.D
Acq On : 15 Oct 2024 13:30
Operator : SY/MD
Sample : P4379-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------