
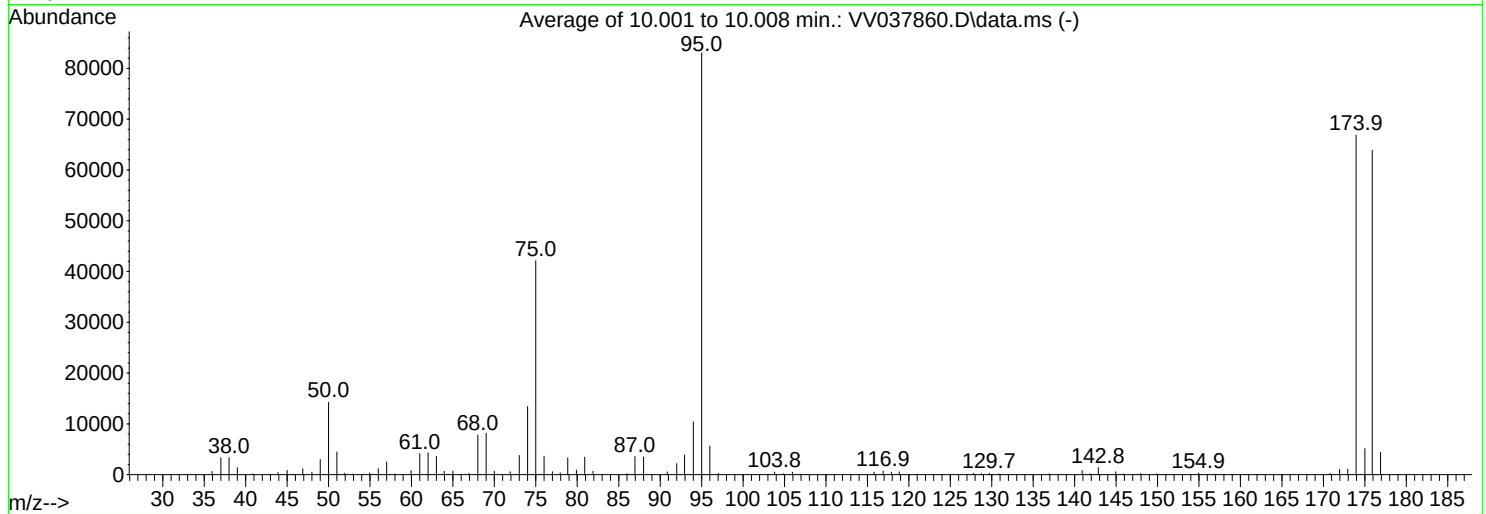


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101524\
Data File : VV037860.D
Acq On : 15 Oct 2024 08:33
Operator : SY/MD
Sample : BFB394
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB394

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Wed Oct 16 03:26:57 2024

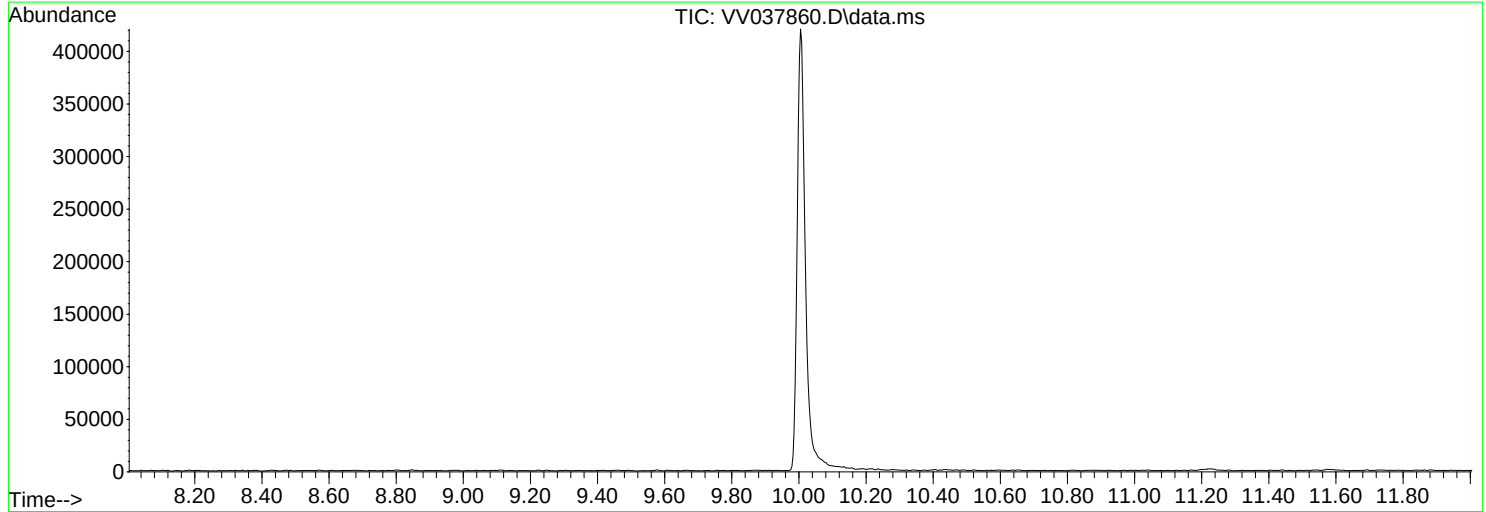

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14259	PASS
75	95	30	80	50.7	42139	PASS
95	95	100	100	100.0	83059	PASS
96	95	5	9	6.8	5615	PASS
173	174	0.00	2	1.6	1068	PASS
174	95	50	120	80.5	66867	PASS
175	174	5	9	7.7	5137	PASS
176	174	95	105	95.5	63880	PASS
177	176	5	10	6.9	4427	PASS

m/z	Abundance
38.10	102.0
39.90	543.0
43.90	504.0
72.70	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
35.90	645.0
37.00	3401.0
38.00	3542.0
39.00	1458.0
39.90	464.0
40.90	143.0
42.90	117.0
43.90	915.0
45.00	828.0
45.80	173.0
46.90	1140.0
48.10	448.0
49.00	2931.0
50.00	14401.0
51.00	4426.0
51.90	231.0
52.90	154.0
54.20	104.0
55.00	259.0
56.00	1167.0
57.00	2456.0
58.00	158.0
60.00	918.0
61.00	3855.0
62.00	4300.0
63.00	3529.0
63.90	604.0
65.00	615.0
67.00	326.0
68.00	7587.0
69.00	7887.0
70.00	745.0
71.90	609.0
73.00	3654.0
74.00	12906.0
75.00	41296.0
76.00	3595.0
77.10	534.0
77.90	360.0
78.90	3283.0
79.90	818.0
80.90	3185.0
81.90	633.0
83.10	105.0
86.00	242.0
87.00	3595.0
88.00	3595.0
90.90	573.0
92.00	2223.0
92.90	3559.0
94.00	9814.0
95.00	80320.0
96.00	5538.0
97.10	207.0
103.80	565.0
104.80	179.0
105.90	491.0
106.90	133.0
115.80	483.0
116.90	657.0
117.90	504.0
118.80	485.0
127.80	249.0
128.80	166.0
129.70	315.0
130.80	149.0
136.80	173.0
140.90	753.0
141.90	164.0
142.80	1223.0
145.00	493.0
145.80	183.0
147.70	153.0
148.10	172.0
149.90	111.0
155.00	256.0
161.00	147.0
170.80	271.0
171.90	958.0
173.00	964.0
173.90	63112.0
175.00	4932.0
175.90	60184.0
176.90	4193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
35.90	625.0
37.00	3456.0
38.00	3552.0
39.00	1396.0
39.90	478.0
40.90	167.0
42.90	103.0
43.90	940.0
45.00	892.0
45.70	152.0
46.90	1170.0
48.00	515.0
49.00	3097.0
50.00	14701.0
51.00	4614.0
51.90	303.0
53.00	183.0
55.00	366.0
56.00	1186.0
57.00	2661.0
58.00	176.0
59.90	862.0
61.00	4333.0
62.00	4436.0
63.00	3657.0
64.00	663.0
65.00	714.0
67.00	301.0
68.00	8064.0
69.00	8347.0
70.00	692.0
71.90	593.0
73.00	3909.0
74.00	13903.0
75.00	43352.0
76.00	3717.0
77.00	588.0
78.00	391.0
78.80	3417.0
79.90	926.0
80.90	3551.0
81.90	701.0
86.00	227.0
86.90	3607.0
88.00	3607.0
90.80	585.0
92.00	2237.0
93.00	3952.0
94.00	10718.0
95.00	85672.0
96.00	5819.0
97.10	268.0
103.80	545.0
104.80	178.0
105.90	482.0
106.90	121.0
115.80	559.0
116.90	740.0
117.90	502.0
118.90	566.0
127.80	302.0
128.80	194.0
129.70	312.0
130.80	141.0
136.90	173.0
140.90	798.0
141.90	184.0
142.80	1440.0
145.00	603.0
145.90	157.0
147.90	211.0
149.90	155.0
154.90	344.0
156.80	137.0
160.60	115.0
170.80	270.0
172.00	1059.0
173.00	1120.0
173.90	69064.0
175.00	5443.0
175.90	66128.0
176.90	4596.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394

m/z	Abundance
36.00	634.0
37.00	3179.0
38.00	3350.0
39.00	1351.0
39.90	538.0
40.80	149.0
44.00	924.0
45.00	836.0
46.90	1169.0
47.90	576.0
49.00	2987.0
50.00	13674.0
51.00	4339.0
51.90	340.0
53.00	174.0
54.90	393.0
56.00	1108.0
57.00	2339.0
58.00	126.0
59.90	712.0
61.00	4248.0
62.00	4081.0
63.00	3589.0
64.00	710.0
65.00	747.0
66.90	268.0
68.00	7660.0
69.00	8131.0
70.00	599.0
71.90	492.0
73.00	3762.0
74.00	13506.0
75.00	41768.0
76.00	3541.0
76.90	572.0
77.90	376.0
78.80	3281.0
79.90	991.0
80.90	3532.0
81.90	696.0
85.90	144.0
86.90	3536.0
88.00	3164.0
90.90	449.0
92.00	2072.0
93.00	3984.0
94.00	10636.0
95.00	83184.0
96.00	5487.0
97.00	301.0
103.80	429.0
104.90	161.0
106.00	422.0
115.80	502.0
116.90	788.0
117.90	457.0
118.90	608.0
127.80	340.0
128.70	175.0
129.70	277.0
130.80	117.0
137.00	148.0
140.90	822.0
141.80	181.0
142.90	1472.0
144.90	571.0
145.90	115.0
147.90	250.0
149.90	190.0
154.90	396.0
156.90	161.0
170.80	242.0
172.00	1088.0
172.90	1121.0
174.00	68424.0
175.00	5036.0
175.90	65328.0
176.90	4493.0
177.90	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB394