
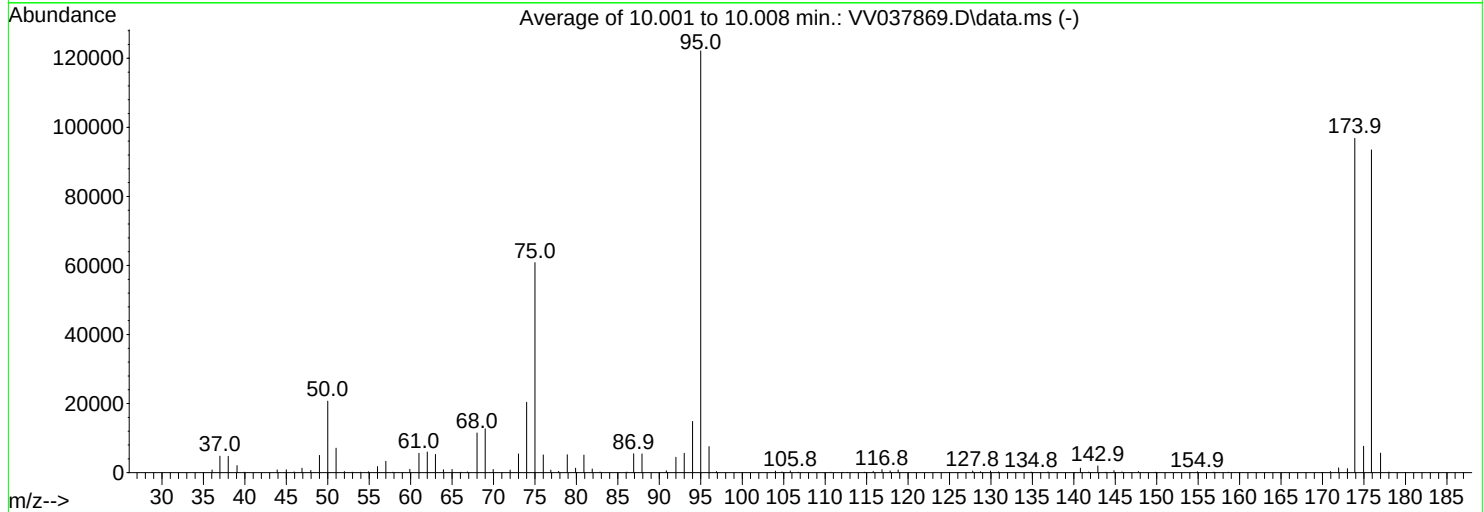


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101624\
Data File : VV037869.D
Acq On : 16 Oct 2024 09:41
Operator : SY/MD
Sample : BFB279
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB279

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 17 02:37:45 2024

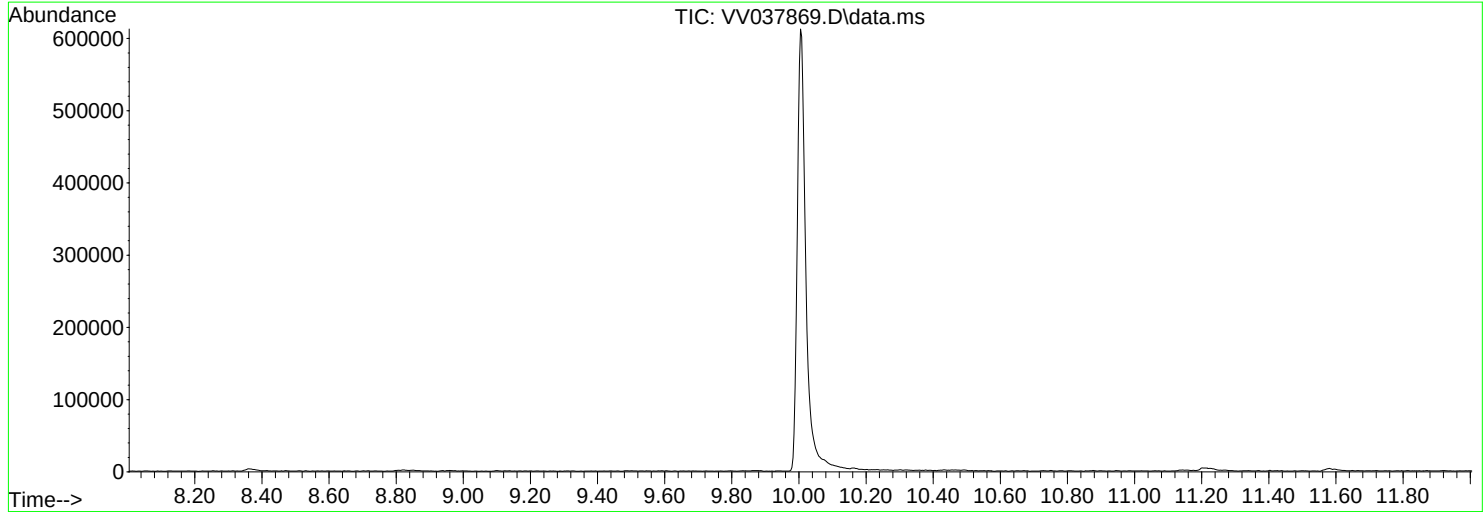

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	20699	PASS
75	95	30	80	49.8	60827	PASS
95	95	100	100	100.0	122157	PASS
96	95	5	9	6.2	7551	PASS
173	174	0.00	2	1.2	1182	PASS
174	95	50	120	79.3	96819	PASS
175	174	5	9	7.9	7639	PASS
176	174	95	105	96.6	93488	PASS
177	176	5	10	6.1	5662	PASS

Scan 2775 (9.963 min): VV037869.D\data.ms
BFB279

m/z	Abundance
39.90	516.0
43.90	546.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.10	841.0
37.00	4591.0
38.00	4576.0
39.10	2002.0
40.00	655.0
43.90	1348.0
45.00	897.0
46.00	215.0
46.90	1302.0
47.90	678.0
49.00	4765.0
50.00	20072.0
51.00	6809.0
52.00	280.0
53.00	131.0
53.90	107.0
54.90	276.0
56.00	1907.0
57.00	3124.0
57.90	120.0
59.90	940.0
61.00	5442.0
62.00	5618.0
63.00	4839.0
63.90	759.0
65.00	919.0
66.00	169.0
67.00	257.0
68.00	11037.0
69.00	12149.0
70.00	890.0
72.00	774.0
73.00	5103.0
74.00	19248.0
75.00	58088.0
76.00	5000.0
76.90	676.0
77.80	362.0
78.90	5172.0
79.90	1258.0
80.90	4833.0
81.90	952.0
82.80	150.0
86.10	277.0
86.90	5257.0
87.90	5447.0
90.80	455.0
92.00	4383.0
93.00	5690.0
94.00	14138.0
95.00	117640.0
96.00	7382.0
96.90	358.0
104.00	453.0
104.80	196.0
105.70	515.0
106.80	117.0
110.70	111.0
112.70	129.0
114.80	124.0
115.70	329.0
116.80	880.0
117.80	375.0
118.80	675.0
127.80	477.0
128.80	246.0
130.00	409.0
130.90	152.0
135.00	219.0
136.90	215.0
140.80	1136.0
141.80	177.0
142.90	1833.0
143.90	154.0
144.90	551.0
145.80	283.0
146.80	130.0
147.90	410.0
149.90	165.0
154.90	287.0
156.80	224.0
158.70	103.0
169.90	113.0
171.00	262.0
171.90	1231.0
173.00	1146.0
173.90	90216.0
175.00	7060.0
175.90	87616.0
177.00	5586.0
178.00	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.00	764.0
37.00	4997.0
38.00	4922.0
39.00	2031.0
40.00	661.0
43.90	1353.0
45.00	889.0
45.90	262.0
46.90	1331.0
47.90	653.0
49.00	5171.0
50.00	21520.0
51.00	7339.0
52.00	342.0
53.00	141.0
54.00	151.0
54.90	304.0
56.00	1838.0
57.00	3432.0
57.80	134.0
59.90	1014.0
61.00	5748.0
62.00	6127.0
63.00	5460.0
64.00	796.0
65.00	942.0
66.00	154.0
66.80	258.0
68.00	11803.0
69.00	13287.0
70.00	938.0
72.00	759.0
73.00	5659.0
74.00	21088.0
75.00	63112.0
76.00	5356.0
76.90	743.0
77.80	380.0
78.90	5387.0
79.90	1318.0
80.90	5310.0
81.90	1094.0
82.80	208.0
86.10	208.0
86.90	5679.0
87.90	5670.0
90.90	546.0
92.00	4667.0
93.00	5819.0
94.00	15456.0
95.00	125536.0
96.00	7661.0
96.90	345.0
104.00	467.0
104.80	270.0
105.80	512.0
106.80	133.0
110.70	141.0
112.10	130.0
112.70	120.0
114.80	157.0
115.80	370.0
116.80	881.0
117.90	510.0
118.80	805.0
127.80	560.0
128.70	277.0
130.00	470.0
130.90	218.0
134.80	184.0
136.90	262.0
140.80	1342.0
141.80	196.0
142.90	2033.0
143.80	164.0
144.80	649.0
145.80	235.0
146.80	130.0
147.80	357.0
149.90	159.0
155.00	288.0
156.80	193.0
157.00	188.0
158.60	165.0
170.90	303.0
172.00	1430.0
173.00	1181.0
173.90	100040.0
174.90	7934.0
175.90	96856.0
177.00	5825.0
178.00	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279

m/z	Abundance
36.00	729.0
37.00	4710.0
38.00	4742.0
39.00	2056.0
40.00	636.0
43.90	1302.0
45.00	785.0
45.90	233.0
46.90	1309.0
48.00	613.0
49.00	5109.0
50.00	20504.0
51.00	7185.0
52.00	352.0
52.90	187.0
54.00	153.0
54.90	297.0
56.00	1555.0
57.00	3312.0
57.80	126.0
59.90	994.0
61.00	5644.0
62.00	6219.0
63.00	5600.0
64.00	899.0
65.00	938.0
66.10	124.0
66.80	254.0
68.00	11715.0
69.00	12661.0
69.90	960.0
71.00	125.0
72.00	647.0
73.00	5565.0
74.00	20904.0
75.00	61280.0
76.00	5136.0
76.90	816.0
77.90	415.0
78.90	5025.0
79.90	1267.0
80.90	5102.0
81.90	1128.0
82.90	194.0
86.00	144.0
86.90	5527.0
87.90	5155.0
90.90	614.0
92.00	4255.0
93.00	5385.0
94.00	14914.0
95.00	123296.0
96.00	7611.0
96.90	315.0
104.00	455.0
104.80	312.0
105.90	543.0
106.70	137.0
110.70	131.0
112.10	128.0
114.80	147.0
115.90	385.0
116.90	916.0
117.90	584.0
118.80	890.0
127.80	552.0
128.70	332.0
129.90	466.0
130.90	265.0
134.70	200.0
136.00	125.0
136.90	253.0
140.10	118.0
140.80	1367.0
141.80	179.0
142.90	1981.0
143.80	141.0
144.90	630.0
145.80	146.0
147.70	284.0
149.80	161.0
154.80	260.0
157.00	177.0
158.60	186.0
170.90	367.0
172.00	1502.0
173.00	1219.0
173.90	100200.0
175.00	7922.0
175.90	95992.0
177.00	5576.0
178.00	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB279