
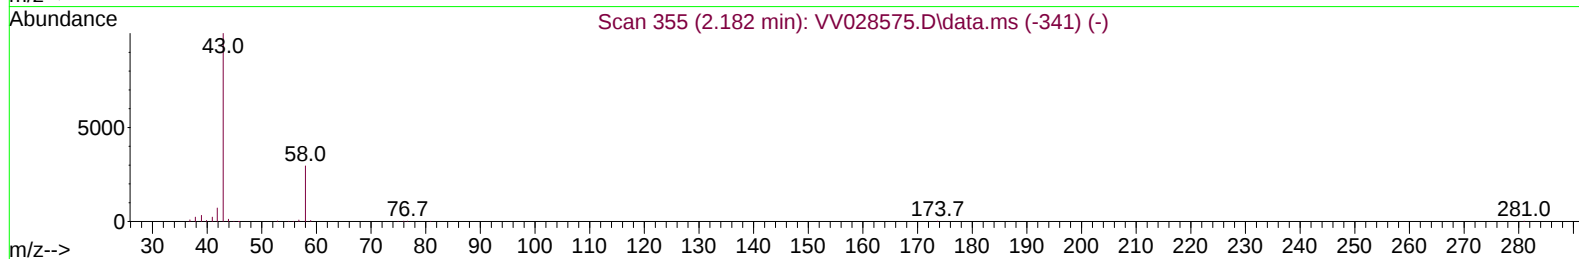
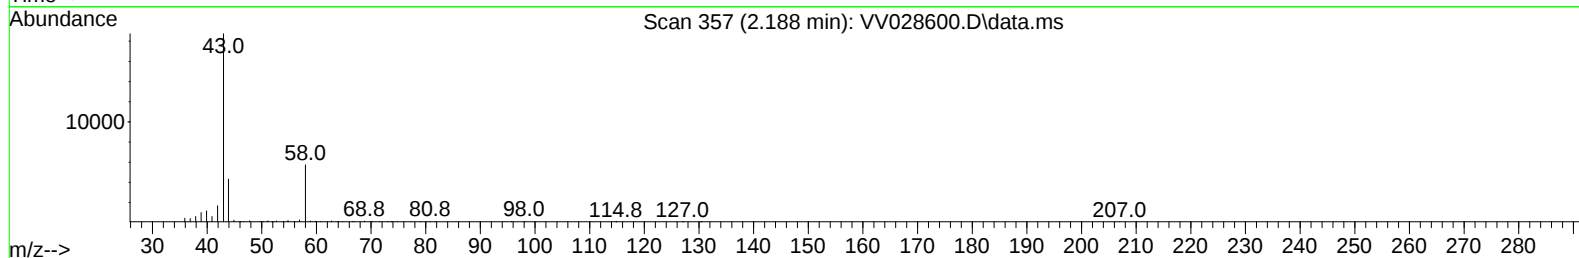


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028600.D
Acq On : 17 Oct 2022 20:08
Operator : SY/MD
Sample : VSTDCCC005EC
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 18 02:52:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 18 01:19:01 2022
Response via : Initial Calibration

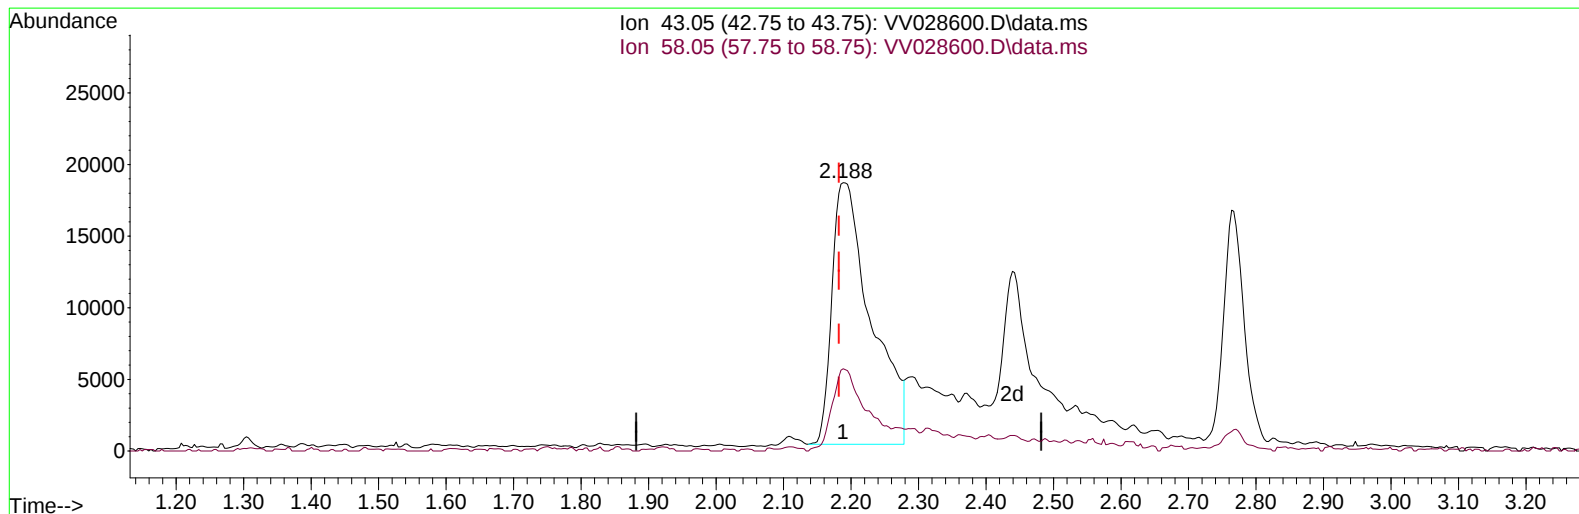

TIC: VV028600.D\data.ms

(13) Acetone (T)

2.188min (+ 0.007) 27.54 ug/L

response 73785

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	24.30	27.56
0.00	0.00	0.00
0.00	0.00	0.00