

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028590.D
 Acq On : 17 Oct 2022 15:44
 Operator : SY/MD
 Sample : N5109-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 18 01:24:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Oct 18 01:19:01 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	185965	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	179389	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	82591	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	82844	5.176	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.600%
7) Chloroethane-d5	1.565	69	75546	5.742	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.800%
11) 1,1-Dichloroethene-d2	2.101	63	120346	4.152	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	83.000%
20) 2-Butanone-d5	3.912	46	120883	35.134	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	70.260%
24) Chloroform-d	4.346	84	131708	5.374	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.400%
26) 1,2-Dichloroethane-d4	5.031	65	68961	5.399	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.000%
32) Benzene-d6	5.047	84	277613	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
36) 1,2-Dichloropropane-d6	6.066	67	94573	5.059	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.314	98	231972	5.055	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
43) trans-1,3-Dichloroprop...	7.622	79	27440	4.345	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.000%
46) 2-Hexanone-d5	8.088	63	140148	51.421	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.840%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	58378	5.244	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.800%
66) 1,2-Dichlorobenzene-d4	11.616	152	74552	5.470	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	5607	0.344	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028590.D
Acq On : 17 Oct 2022 15:44
Operator : SY/MD
Sample : N5109-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Oct 18 01:24:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Oct 18 01:19:01 2022
Response via : Initial Calibration

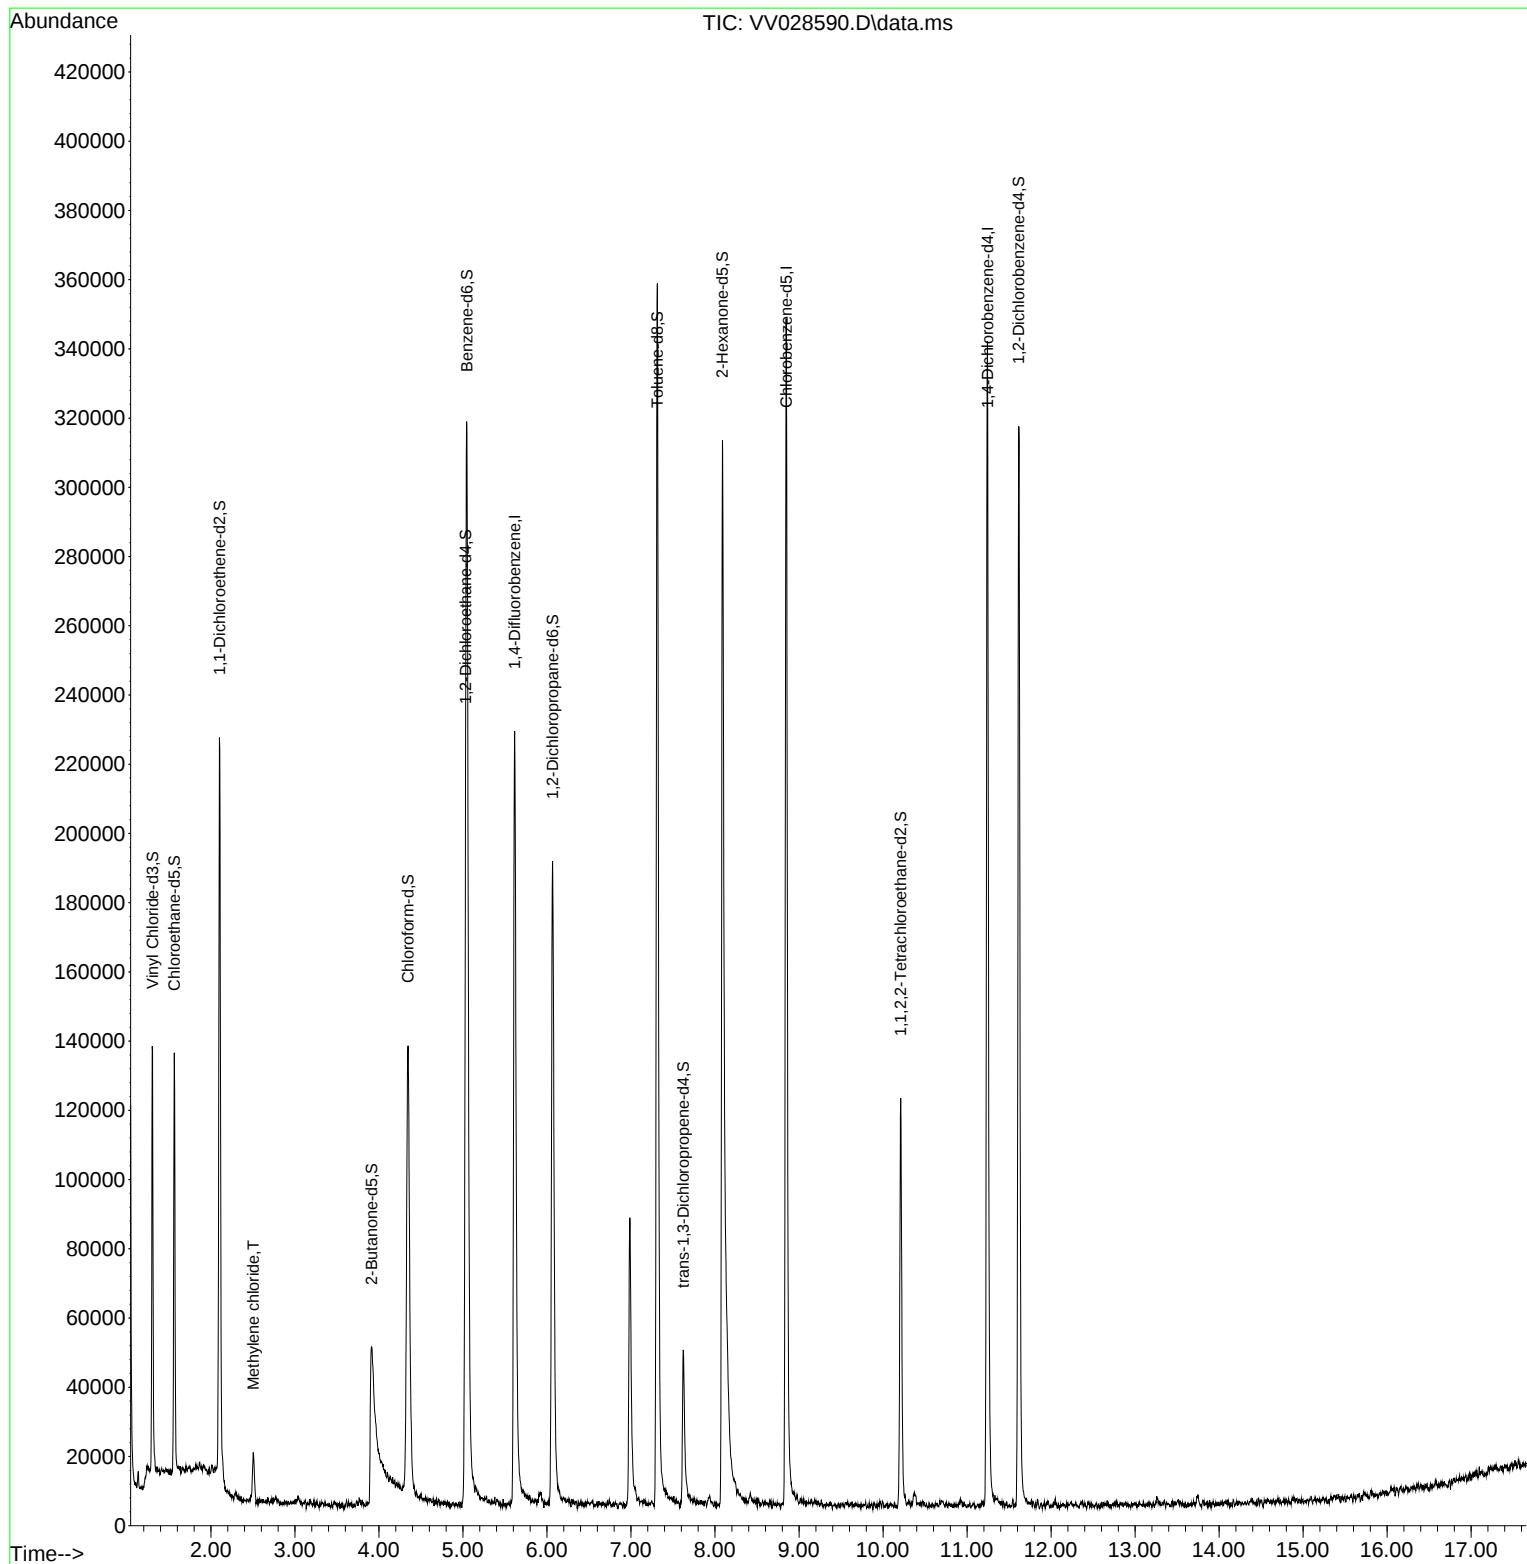

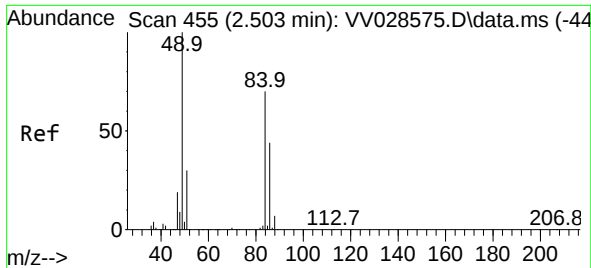

#16
Methylene chloride
Concen: 0.344 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV028590.D
Acq: 17 Oct 2022 15:44

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

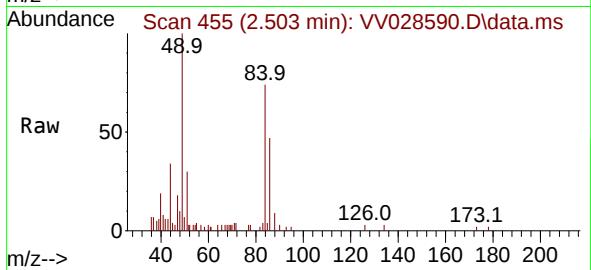

Tgt Ion: 84 Resp: 5607
Ion Ratio Lower Upper
84 100
86 63.9 42.8 79.6
49 144.0 106.4 197.6

