

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028577.D
 Acq On : 17 Oct 2022 10:39
 Operator : SY/MD
 Sample : N5163-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD715

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	103	rVB2	150124	205857	23.97%	2.766%
2	1.568	157	164	174	rVB	128282	141523	16.48%	1.901%
3	2.105	322	331	347	rVB	216141	312535	36.39%	4.199%
4	2.506	450	456	465	rVB2	12804	19733	2.30%	0.265%
5	3.895	878	888	922	rBV	76510	291783	33.98%	3.920%
6	4.342	1011	1027	1058	rBV2	134653	364698	42.47%	4.900%
7	5.043	1229	1245	1279	rBV2	318959	858807	100.00%	11.538%
8	5.612	1408	1422	1445	rBV	277342	579458	67.47%	7.785%
9	6.066	1550	1563	1584	rBV2	190452	398306	46.38%	5.351%
10	6.985	1835	1849	1866	rBV	91446	174665	20.34%	2.347%
11	7.310	1939	1950	1965	rBV	364569	644275	75.02%	8.656%
12	7.384	1965	1973	1994	rVB	102184	196499	22.88%	2.640%
13	7.622	2035	2047	2066	rBV	50176	99941	11.64%	1.343%
14	7.934	2134	2144	2155	rBV3	17670	32347	3.77%	0.435%
15	8.085	2182	2191	2231	rBV	346869	734668	85.55%	9.870%
16	8.847	2417	2428	2452	rBV	412690	693274	80.73%	9.314%
17	9.136	2507	2518	2538	rBV2	28573	61567	7.17%	0.827%
18	9.538	2628	2643	2657	rBV	61725	109343	12.73%	1.469%
19	10.210	2838	2852	2864	rBV	114652	186009	21.66%	2.499%
20	10.377	2892	2904	2916	rVB2	54535	97714	11.38%	1.313%
21	10.538	2943	2954	2961	rBV9	6526	11055	1.29%	0.149%
22	10.908	3062	3069	3078	rBV6	7109	12874	1.50%	0.173%
23	11.242	3162	3173	3192	rBV	405020	649073	75.58%	8.720%
24	11.332	3193	3201	3212	rVB3	11208	21221	2.47%	0.285%
25	11.525	3251	3261	3273	rVB5	8803	16769	1.95%	0.225%
26	11.615	3276	3289	3306	rBV	301198	499859	58.20%	6.716%
27	12.242	3474	3484	3485	rBV9	9423	9645	1.12%	0.130%
28	13.503	3868	3876	3888	rVB2	11778	19594	2.28%	0.263%




Sum of corrected areas: 7443092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028577.D
Acq On : 17 Oct 2022 10:39
Operator : SY/MD
Sample : N5163-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD715

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

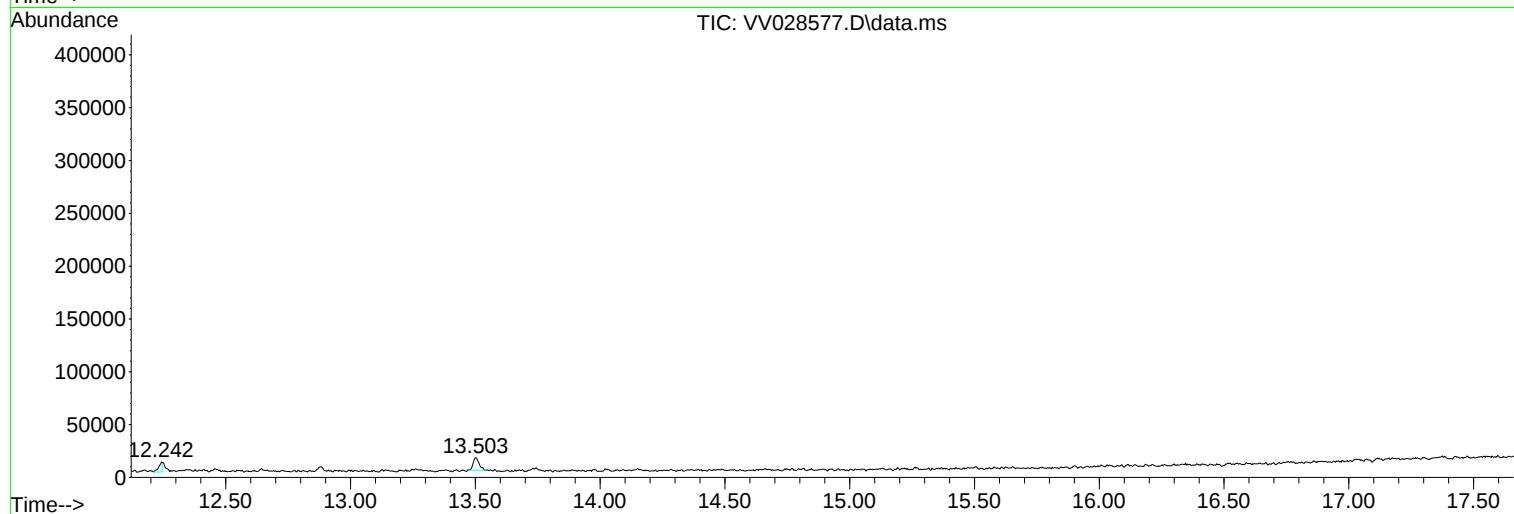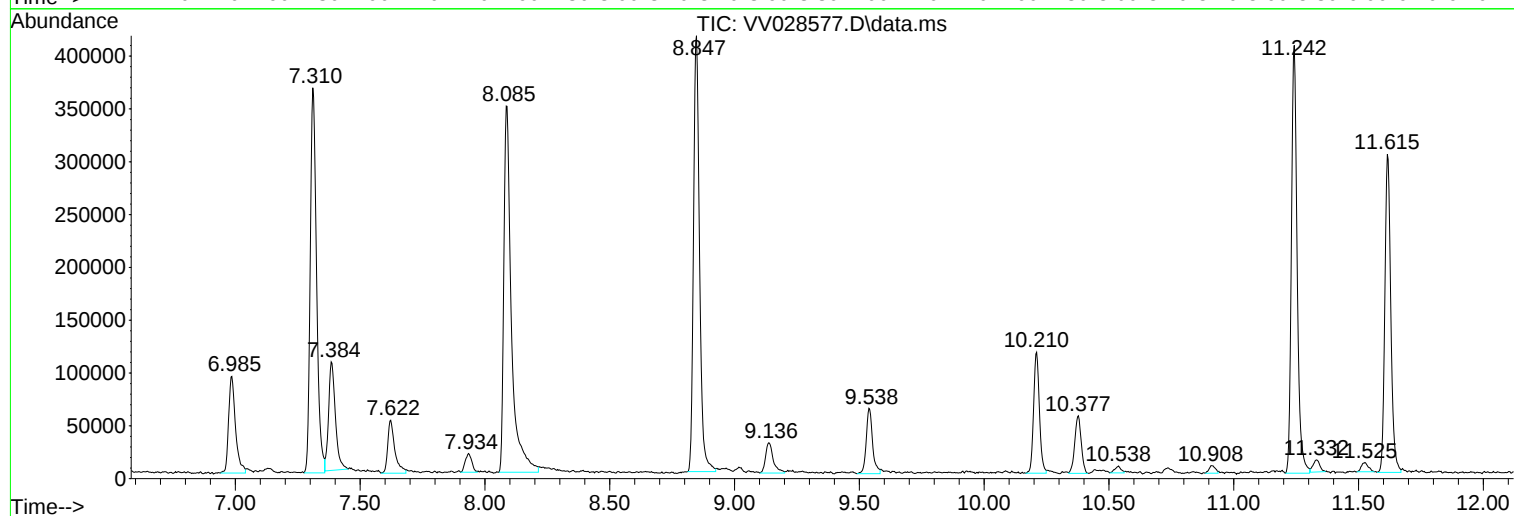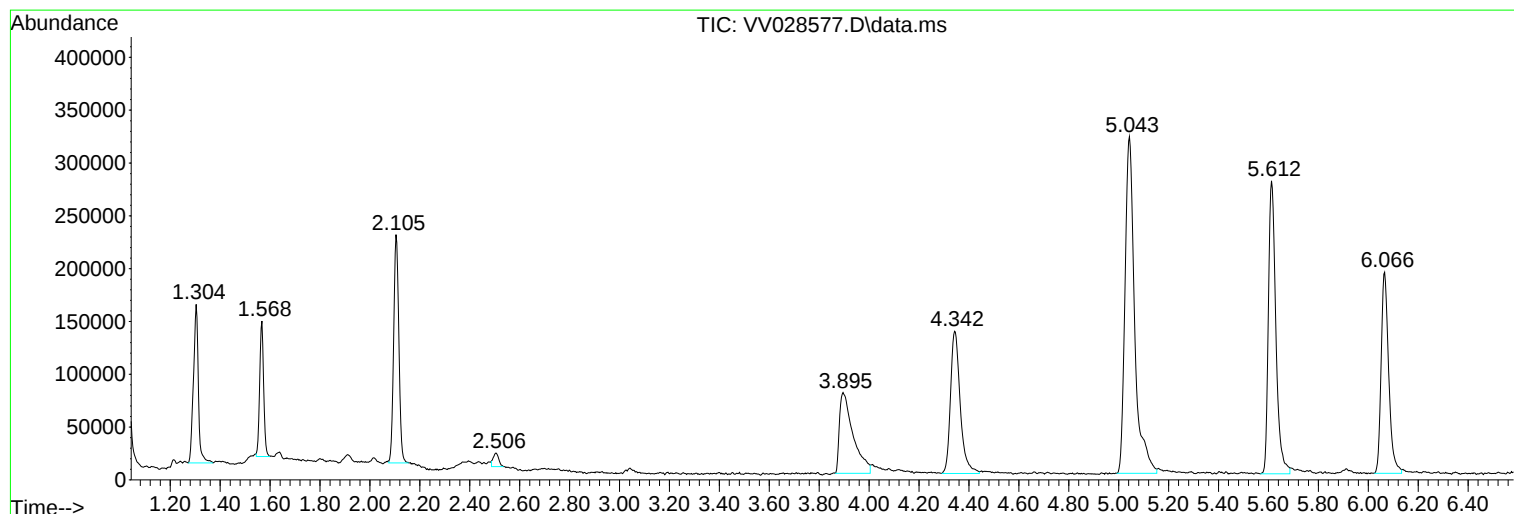

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028577.D
Acq On : 17 Oct 2022 10:39
Operator : SY/MD
Sample : N5163-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD715

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028577.D
Acq On : 17 Oct 2022 10:39
Operator : SY/MD
Sample : N5163-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD715

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc