

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028578.D
 Acq On : 17 Oct 2022 11:03
 Operator : SY/MD
 Sample : N5163-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BD716

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	57	62	71	rVV2	9828	15978	1.80%	0.213%
2	1.304	72	82	94	rVV2	151593	217224	24.45%	2.896%
3	1.468	127	133	134	rBV3	10089	9391	1.06%	0.125%
4	1.564	157	163	173	rVB	123515	142265	16.01%	1.897%
5	1.912	263	271	283	rVB5	8656	14409	1.62%	0.192%
6	2.105	322	331	345	rVB	217880	315984	35.56%	4.213%
7	3.896	878	888	924	rBV	75381	296812	33.41%	3.957%
8	4.346	1012	1028	1046	rBV	137333	355502	40.01%	4.740%
9	5.043	1229	1245	1285	rBV2	324185	888473	100.00%	11.846%
10	5.612	1410	1422	1446	rBV	269070	558209	62.83%	7.442%
11	6.066	1551	1563	1586	rBV	191612	397458	44.73%	5.299%
12	6.985	1838	1849	1866	rBV2	90004	174635	19.66%	2.328%
13	7.313	1939	1951	1965	rBV	362695	645414	72.64%	8.605%
14	7.387	1965	1974	1994	rVB	124226	233099	26.24%	3.108%
15	7.622	2035	2047	2070	rBV	47940	90710	10.21%	1.209%
16	7.937	2134	2145	2153	rBV2	10820	18485	2.08%	0.246%
17	8.088	2179	2192	2228	rBV	356817	748443	84.24%	9.979%
18	8.847	2416	2428	2452	rBV	401257	679407	76.47%	9.058%
19	9.136	2504	2518	2536	rBV2	34715	66516	7.49%	0.887%
20	9.538	2630	2643	2655	rBV	72885	122127	13.75%	1.628%
21	10.210	2842	2852	2871	rVB	116334	189852	21.37%	2.531%
22	10.378	2889	2904	2913	rBV2	28818	50262	5.66%	0.670%
23	10.535	2942	2953	2961	rBV8	7570	12671	1.43%	0.169%
24	10.734	3008	3015	3024	rBV7	6373	10198	1.15%	0.136%
25	10.918	3061	3072	3091	rBV3	9789	20754	2.34%	0.277%
26	11.242	3161	3173	3192	rBV	390457	638013	71.81%	8.506%
27	11.333	3192	3201	3216	rVB4	12624	24197	2.72%	0.323%
28	11.522	3249	3260	3271	rBV5	10598	21778	2.45%	0.290%
29	11.615	3277	3289	3311	rBV	310557	516040	58.08%	6.880%
30	13.503	3864	3876	3887	rBV2	13774	26062	2.93%	0.347%




Sum of corrected areas: 7500368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028578.D
Acq On : 17 Oct 2022 11:03
Operator : SY/MD
Sample : N5163-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

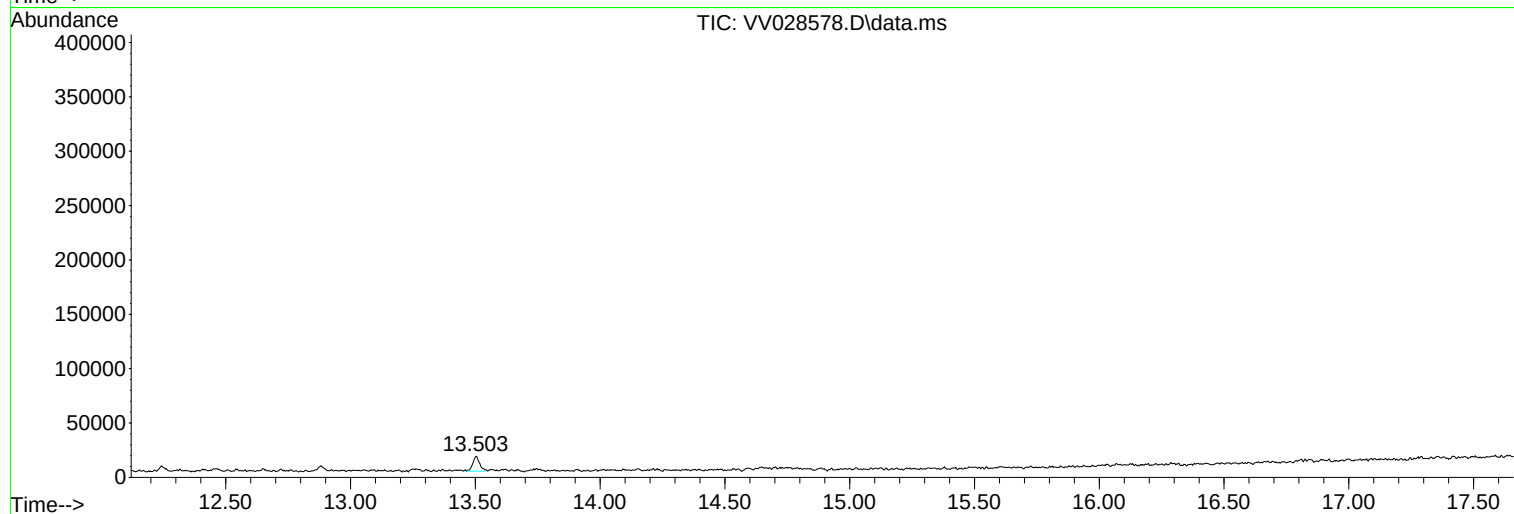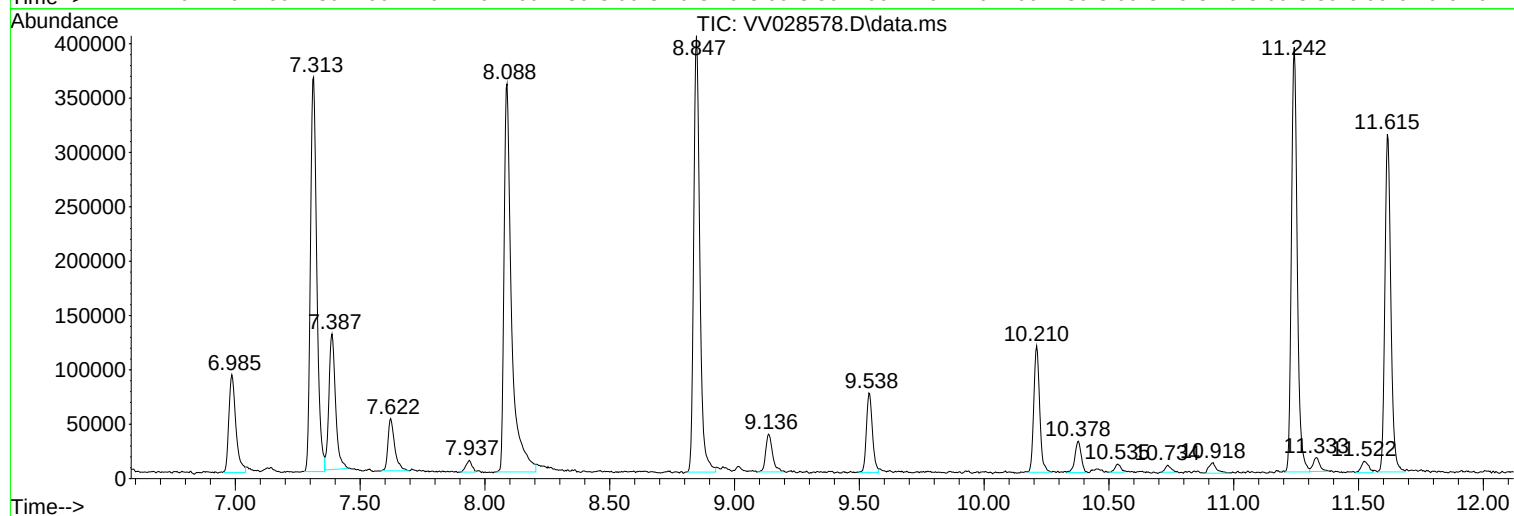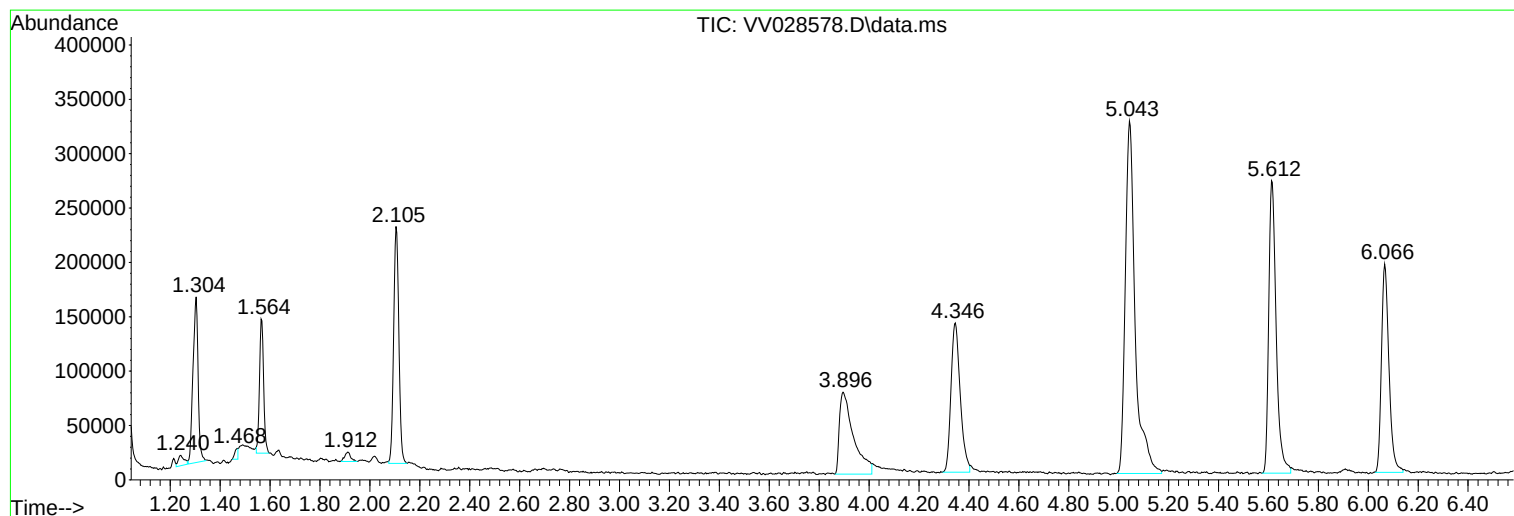

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028578.D
Acq On : 17 Oct 2022 11:03
Operator : SY/MD
Sample : N5163-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028578.D
Acq On : 17 Oct 2022 11:03
Operator : SY/MD
Sample : N5163-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BD716

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc