

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028579.D
 Acq On : 17 Oct 2022 11:27
 Operator : SY/MD
 Sample : N5041-02DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS19DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	102	rVB	130802	137544	16.20%	1.854%
2	1.565	156	163	174	rVB	121931	137254	16.17%	1.850%
3	2.105	321	331	346	rVB	215690	309673	36.48%	4.174%
4	2.503	446	455	467	rBB	21174	32988	3.89%	0.445%
5	3.905	875	891	930	rBV3	248021	791015	93.18%	10.662%
6	4.343	1011	1027	1050	rBV2	133336	341471	40.23%	4.603%
7	5.043	1231	1245	1265	rBV3	320127	792337	93.34%	10.680%
8	5.613	1410	1422	1454	rBV	274794	578771	68.18%	7.801%
9	6.066	1550	1563	1589	rBV2	192350	408247	48.09%	5.503%
10	6.986	1838	1849	1863	rBV	91796	172544	20.33%	2.326%
11	7.310	1939	1950	1972	rBV	350320	632368	74.49%	8.524%
12	7.622	2033	2047	2069	rBV	52229	109230	12.87%	1.472%
13	7.937	2139	2145	2152	rVB3	6853	10362	1.22%	0.140%
14	8.088	2179	2192	2227	rBV	397026	848884	100.00%	11.442%
15	8.847	2417	2428	2447	rBV	419849	695551	81.94%	9.375%
16	10.210	2836	2852	2866	rBV	127681	206927	24.38%	2.789%
17	10.378	2895	2904	2916	rVB3	17821	31418	3.70%	0.423%
18	11.243	3159	3173	3191	rBV	408935	657311	77.43%	8.860%
19	11.616	3277	3289	3311	rBV	316621	525117	61.86%	7.078%




Sum of corrected areas: 7419012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028579.D
Acq On : 17 Oct 2022 11:27
Operator : SY/MD
Sample : N5041-02DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

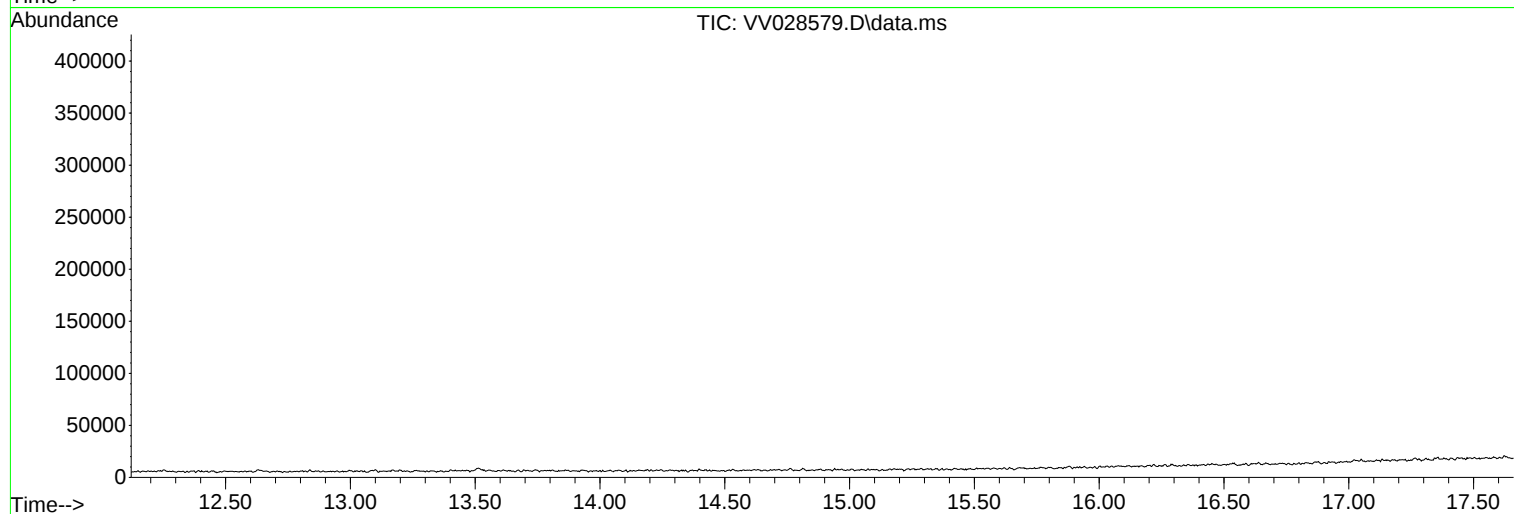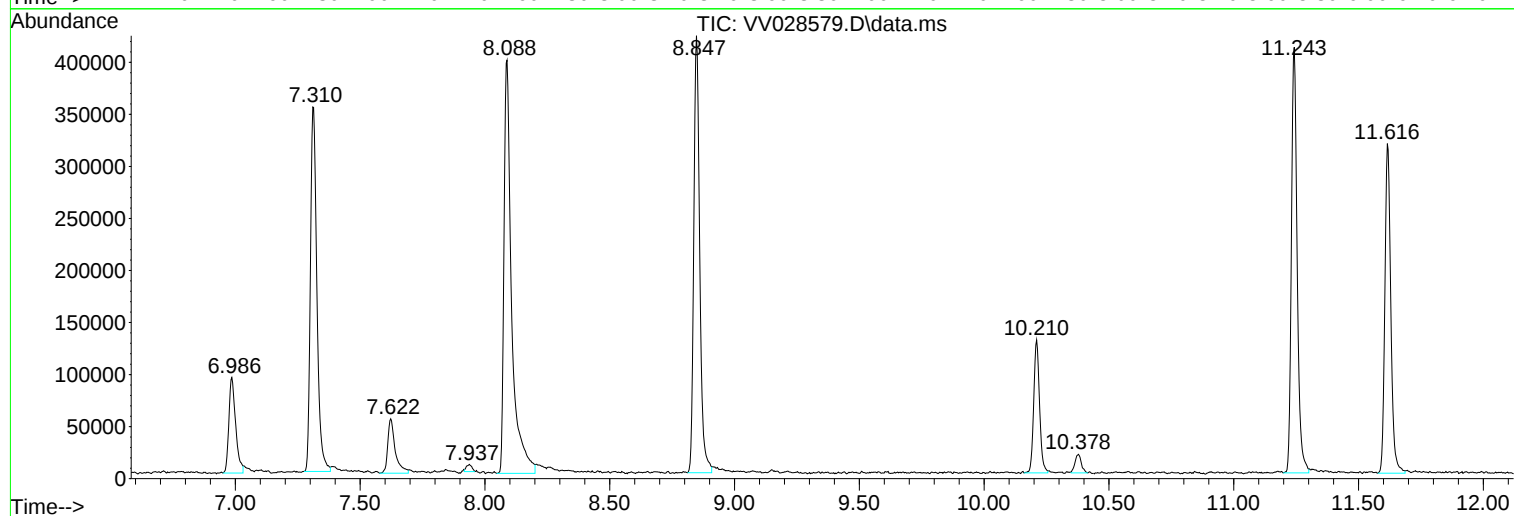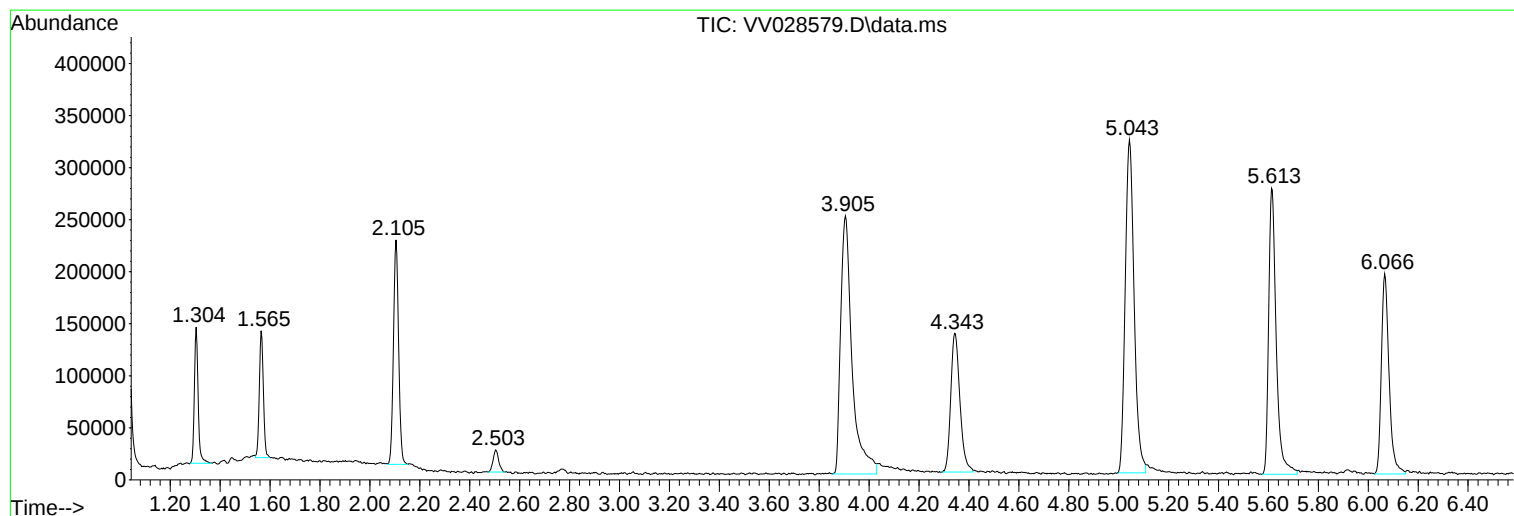

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028579.D
Acq On : 17 Oct 2022 11:27
Operator : SY/MD
Sample : N5041-02DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028579.D
Acq On : 17 Oct 2022 11:27
Operator : SY/MD
Sample : N5041-02DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS19DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc