

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028586.D
 Acq On : 17 Oct 2022 14:09
 Operator : SY/MD
 Sample : N5144-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	48	63	67	rBV	6371	13673	1.73%	0.227%
2	1.304	76	82	95	rVB	108189	109796	13.89%	1.819%
3	1.564	156	163	173	rBV	104659	120421	15.23%	1.995%
4	2.105	321	331	346	rVB	187787	270827	34.26%	4.487%
5	3.899	877	889	917	rBV2	49467	191192	24.19%	3.168%
6	4.343	1013	1027	1057	rVB	123245	311750	39.44%	5.165%
7	5.043	1229	1245	1267	rBV2	283876	709659	89.77%	11.758%
8	5.616	1409	1423	1448	rBV	217763	453949	57.43%	7.521%
9	6.066	1549	1563	1584	rBV2	172746	367095	46.44%	6.082%
10	6.985	1837	1849	1868	rBV	79558	159299	20.15%	2.639%
11	7.313	1936	1951	1969	rBV2	314655	570385	72.16%	9.450%
12	7.622	2037	2047	2066	rBV2	43847	91441	11.57%	1.515%
13	7.934	2135	2144	2145	rBV8	13969	16911	2.14%	0.280%
14	8.088	2182	2192	2236	rBV	308187	790495	100.00%	13.097%
15	8.847	2416	2428	2446	rBV	329526	553450	70.01%	9.170%
16	10.210	2838	2852	2864	rBV	118515	195757	24.76%	3.243%
17	10.378	2888	2904	2916	rBV2	42107	74405	9.41%	1.233%
18	11.243	3160	3173	3192	rBV	328400	534714	67.64%	8.859%
19	11.616	3278	3289	3309	rBV	296675	484313	61.27%	8.024%
20	12.249	3476	3486	3495	rBV2	10062	16212	2.05%	0.269%




Sum of corrected areas: 6035744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028586.D
Acq On : 17 Oct 2022 14:09
Operator : SY/MD
Sample : N5144-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

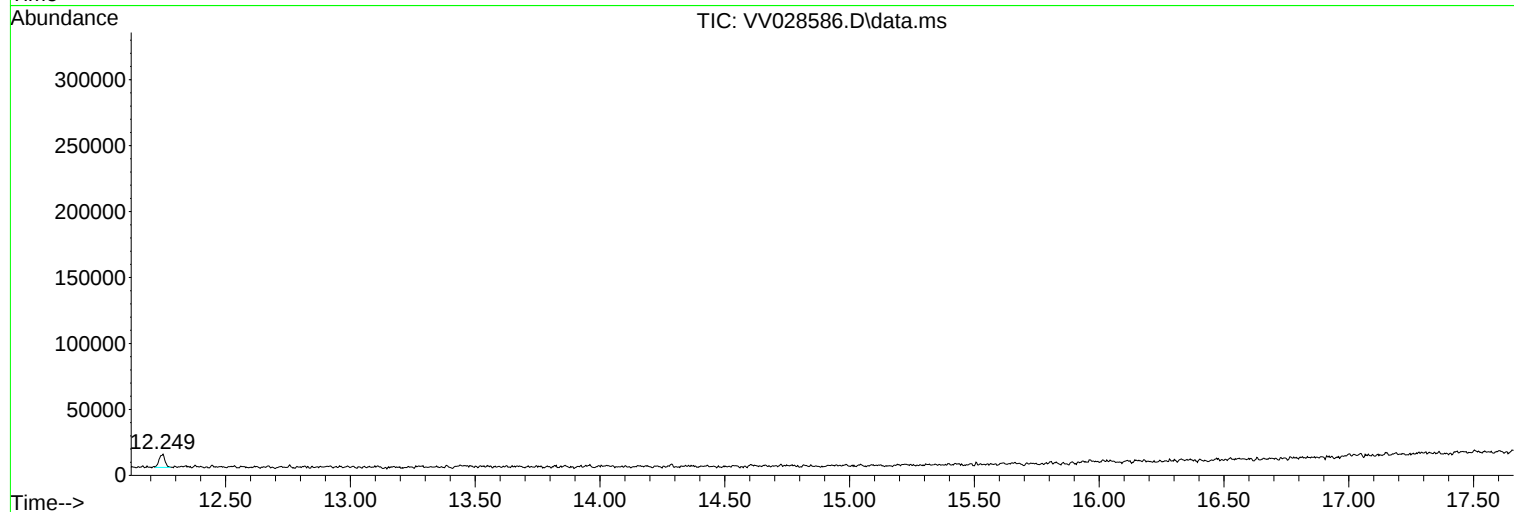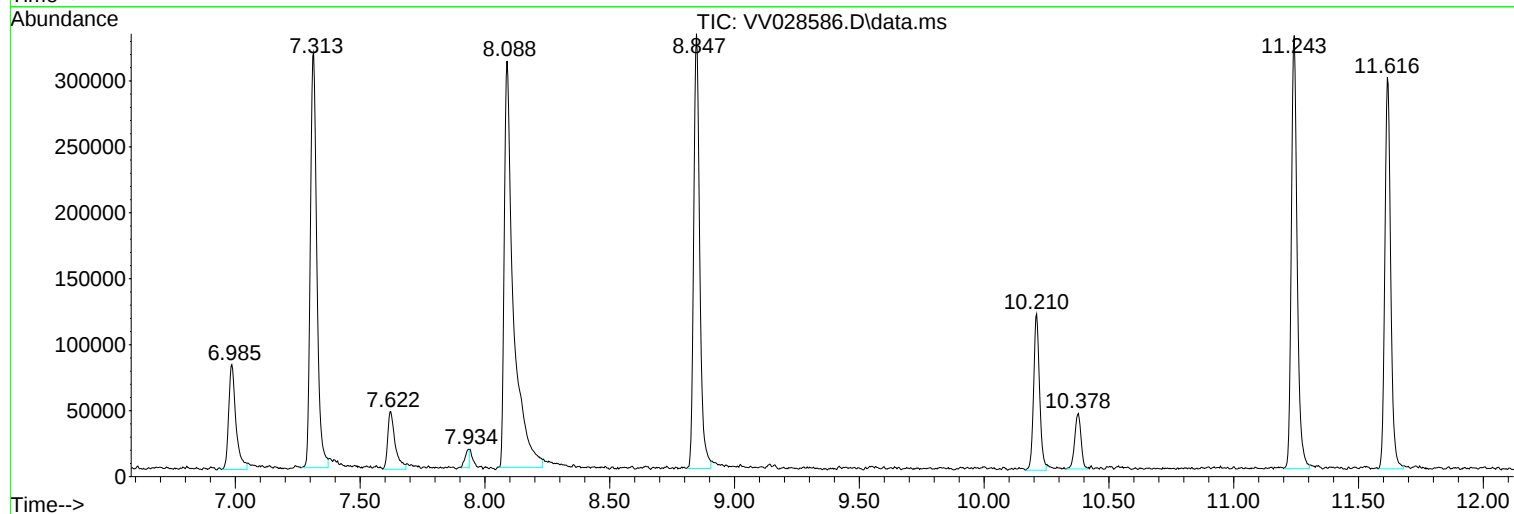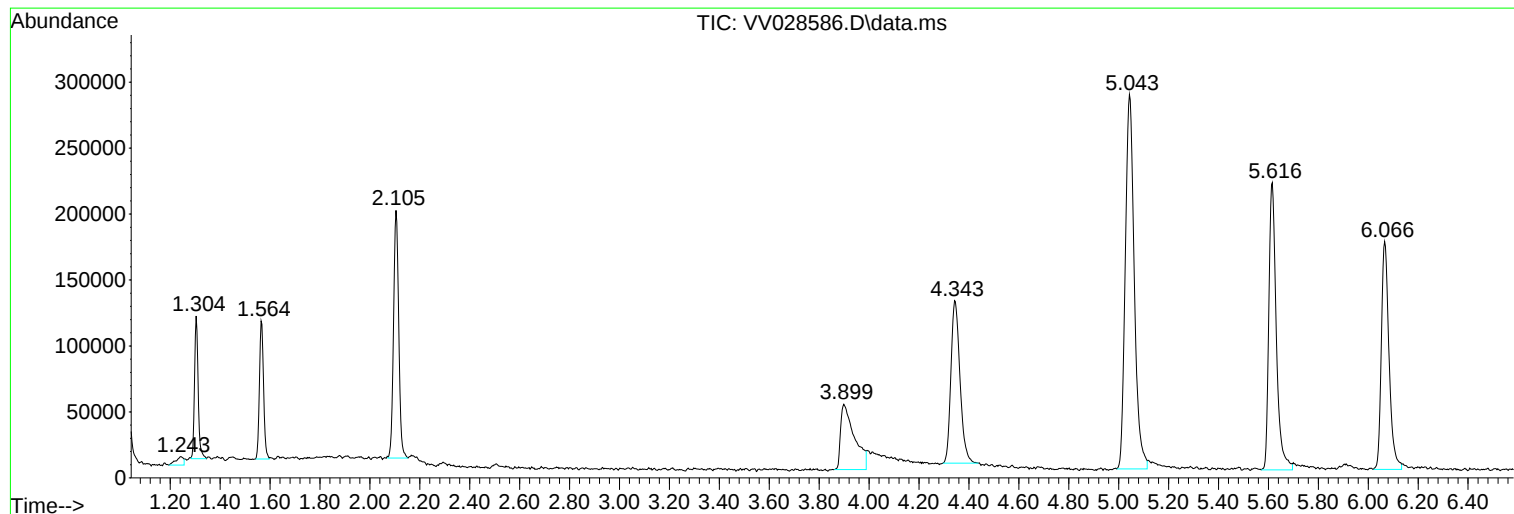

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028586.D
Acq On : 17 Oct 2022 14:09
Operator : SY/MD
Sample : N5144-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028586.D
Acq On : 17 Oct 2022 14:09
Operator : SY/MD
Sample : N5144-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc