

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028587.D
 Acq On : 17 Oct 2022 14:33
 Operator : SY/MD
 Sample : N5144-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rBV	122477	123623	14.19%	1.922%
2	1.564	156	163	176	rBV	119042	131456	15.09%	2.044%
3	2.105	320	331	348	rVB	206105	309470	35.53%	4.812%
4	3.915	882	894	915	rBV	45392	186883	21.46%	2.906%
5	4.346	1012	1028	1053	rBV	130171	337037	38.70%	5.240%
6	5.043	1229	1245	1268	rBV2	312059	770859	88.51%	11.985%
7	5.612	1411	1422	1445	rBV	224520	466482	53.56%	7.253%
8	6.066	1549	1563	1584	rBV	187730	393364	45.17%	6.116%
9	6.985	1837	1849	1870	rBV	84245	168549	19.35%	2.621%
10	7.313	1939	1951	1971	rBV	338664	613762	70.47%	9.543%
11	7.622	2037	2047	2068	rBV2	47771	96865	11.12%	1.506%
12	7.934	2134	2144	2151	rBV2	9781	15843	1.82%	0.246%
13	8.088	2179	2192	2238	rBV	339489	870936	100.00%	13.542%
14	8.847	2417	2428	2454	rBV	348626	585828	67.26%	9.109%
15	10.210	2840	2852	2866	rBV	122832	203741	23.39%	3.168%
16	10.374	2893	2903	2915	rVB4	20455	35178	4.04%	0.547%
17	11.242	3161	3173	3194	rBV	342026	557618	64.03%	8.670%
18	11.615	3278	3289	3307	rBV	317775	519976	59.70%	8.085%
19	12.246	3476	3485	3494	rVB	9417	14141	1.62%	0.220%
20	15.879	4594	4615	4617	rBV	11702	29986	3.44%	0.466%




Sum of corrected areas: 6431597

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028587.D
Acq On : 17 Oct 2022 14:33
Operator : SY/MD
Sample : N5144-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

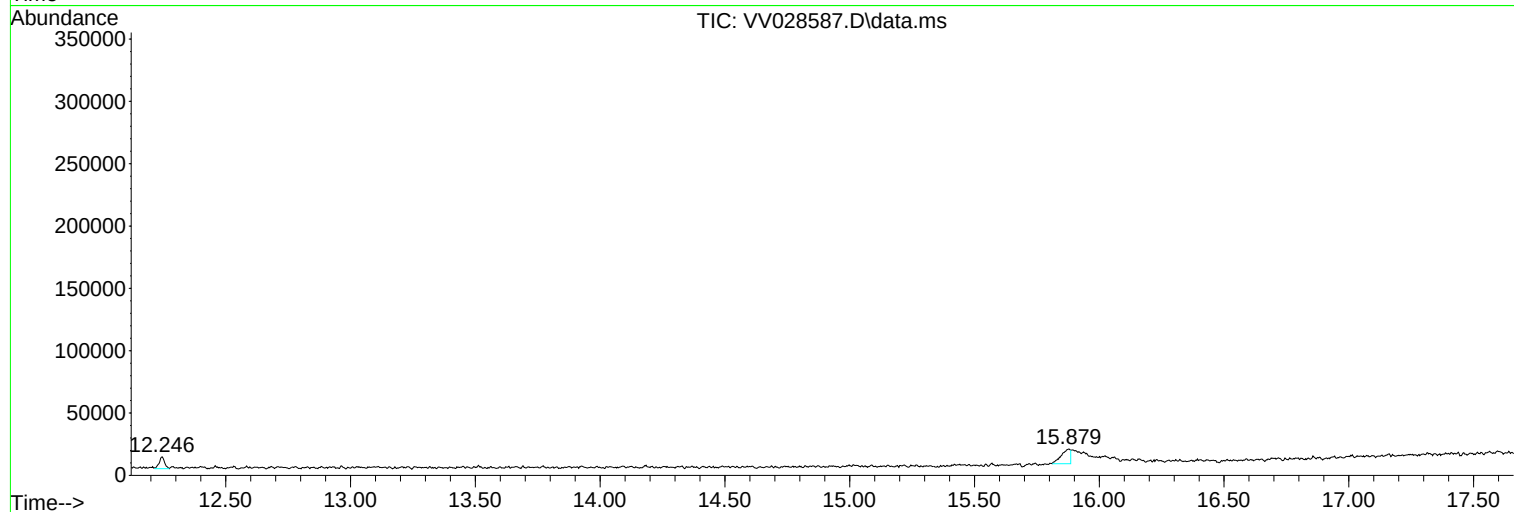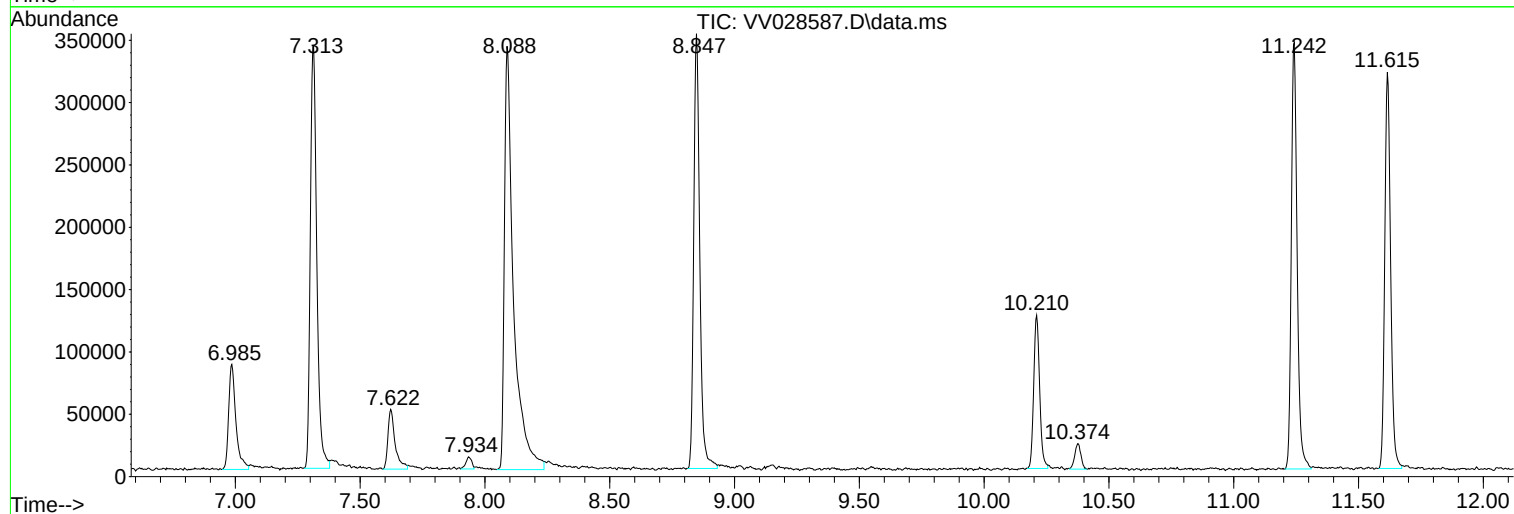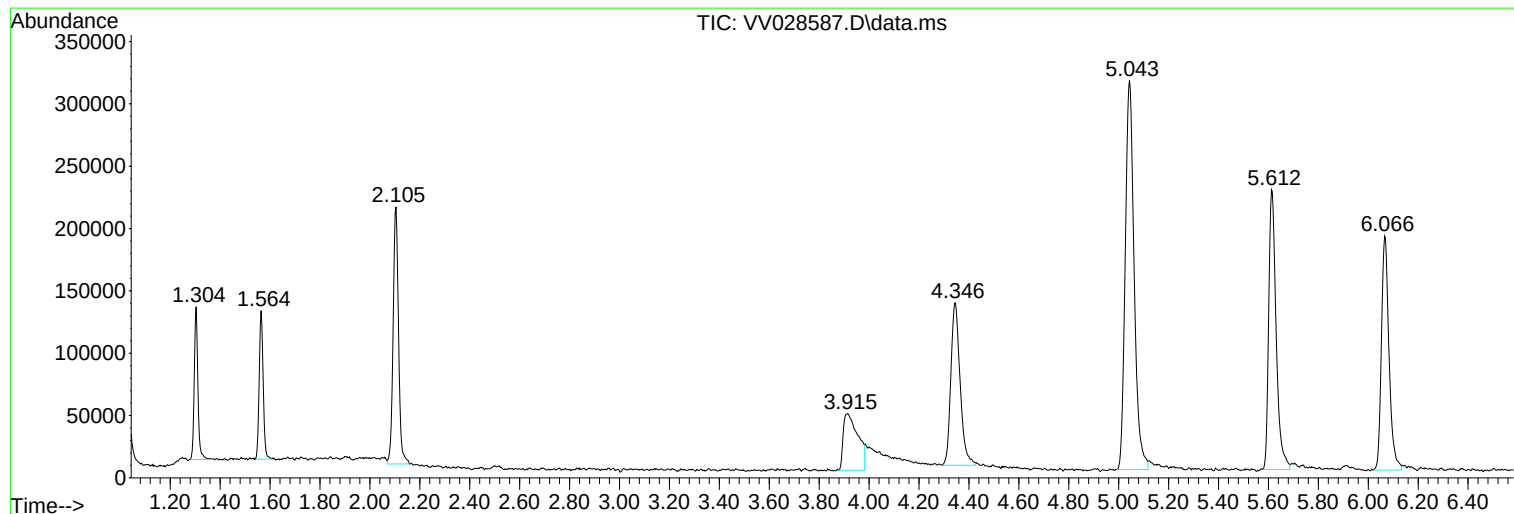

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028587.D
Acq On : 17 Oct 2022 14:33
Operator : SY/MD
Sample : N5144-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028587.D
Acq On : 17 Oct 2022 14:33
Operator : SY/MD
Sample : N5144-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
