

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028594.D
 Acq On : 17 Oct 2022 17:20
 Operator : SY/MD
 Sample : N5060-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1BG6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	55	60	66	rVV2	15149	20679	2.50%	0.335%
2	1.294	73	79	90	rBV	112116	110409	13.35%	1.789%
3	1.558	154	161	170	rVB	109584	120752	14.60%	1.957%
4	1.966	284	288	294	rVB3	14116	15886	1.92%	0.257%
5	2.095	319	328	337	rBV	185589	255498	30.88%	4.141%
6	3.957	890	907	908	rBV6	72921	142742	17.25%	2.313%
7	4.336	1010	1025	1040	rBV	143794	362150	43.77%	5.869%
8	5.031	1228	1241	1262	rVB2	379350	827342	100.00%	13.408%
9	5.606	1407	1420	1439	rBV	241703	491060	59.35%	7.958%
10	6.066	1547	1563	1580	rBV	168702	345942	41.81%	5.607%
11	6.982	1838	1848	1862	rBV	78378	140505	16.98%	2.277%
12	7.307	1938	1949	1966	rBV	294195	516233	62.40%	8.366%
13	7.622	2038	2047	2059	rBV2	40854	72090	8.71%	1.168%
14	8.101	2186	2196	2234	rBV	367942	761841	92.08%	12.347%
15	8.249	2234	2242	2254	rVV3	24462	44362	5.36%	0.719%
16	8.844	2416	2427	2450	rBV	364928	608559	73.56%	9.863%
17	9.558	2645	2649	2658	rVB9	7160	10200	1.23%	0.165%
18	9.812	2720	2728	2738	rBV9	4674	8962	1.08%	0.145%
19	10.210	2838	2852	2869	rVB	113531	182609	22.07%	2.959%
20	10.378	2900	2904	2912	rVB6	8847	11055	1.34%	0.179%
21	11.153	3133	3145	3148	rBV10	7005	10297	1.24%	0.167%
22	11.243	3160	3173	3192	rBV	357815	576907	69.73%	9.350%
23	11.529	3252	3262	3273	rBV2	23953	47799	5.78%	0.775%
24	11.616	3278	3289	3308	rVB	276256	443212	53.57%	7.183%
25	12.339	3506	3514	3527	rBV5	18510	30388	3.67%	0.492%
26	15.500	4489	4497	4509	rBV5	7599	12891	1.56%	0.209%




Sum of corrected areas: 6170370

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028594.D
Acq On : 17 Oct 2022 17:20
Operator : SY/MD
Sample : N5060-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1BG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

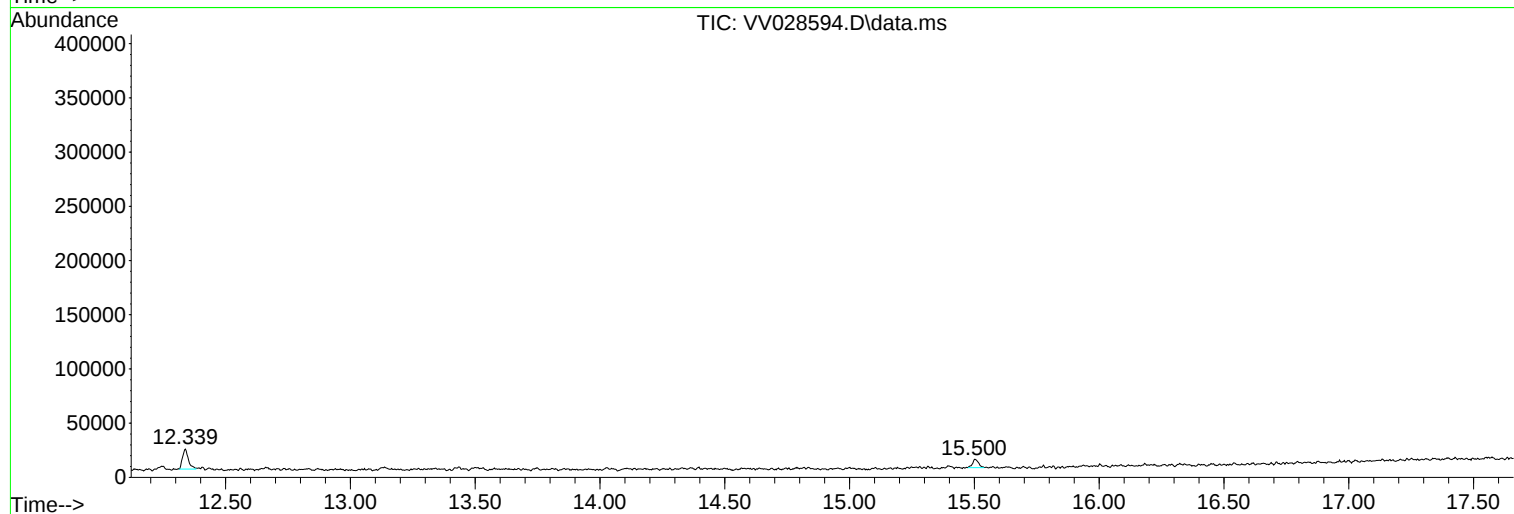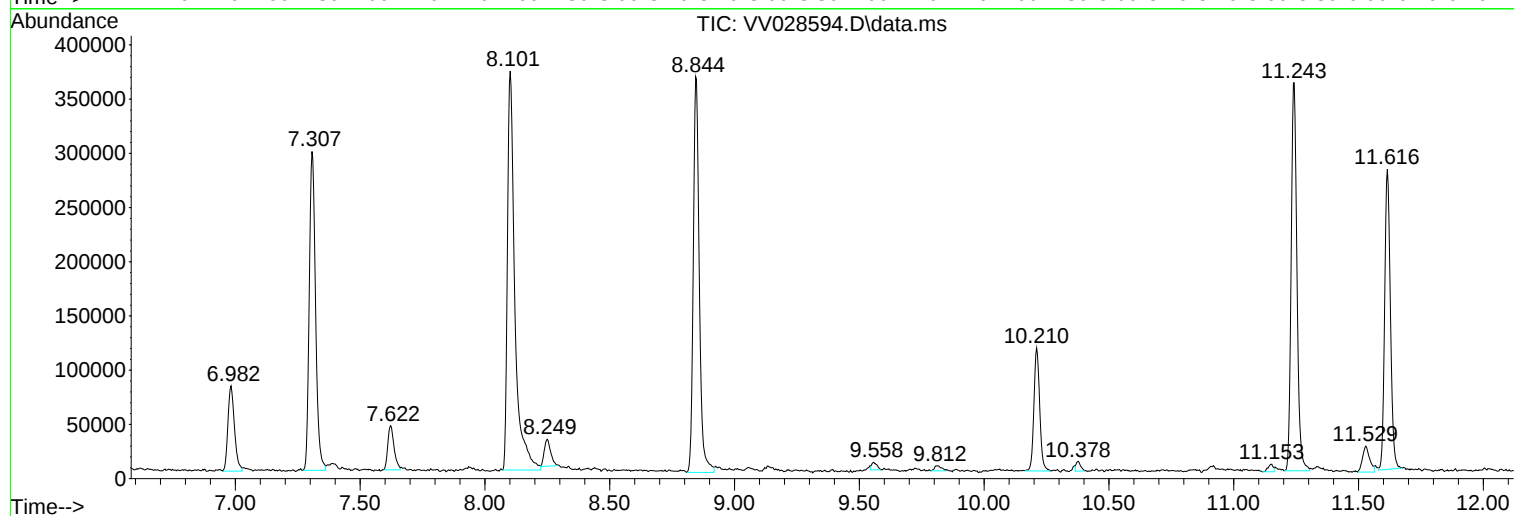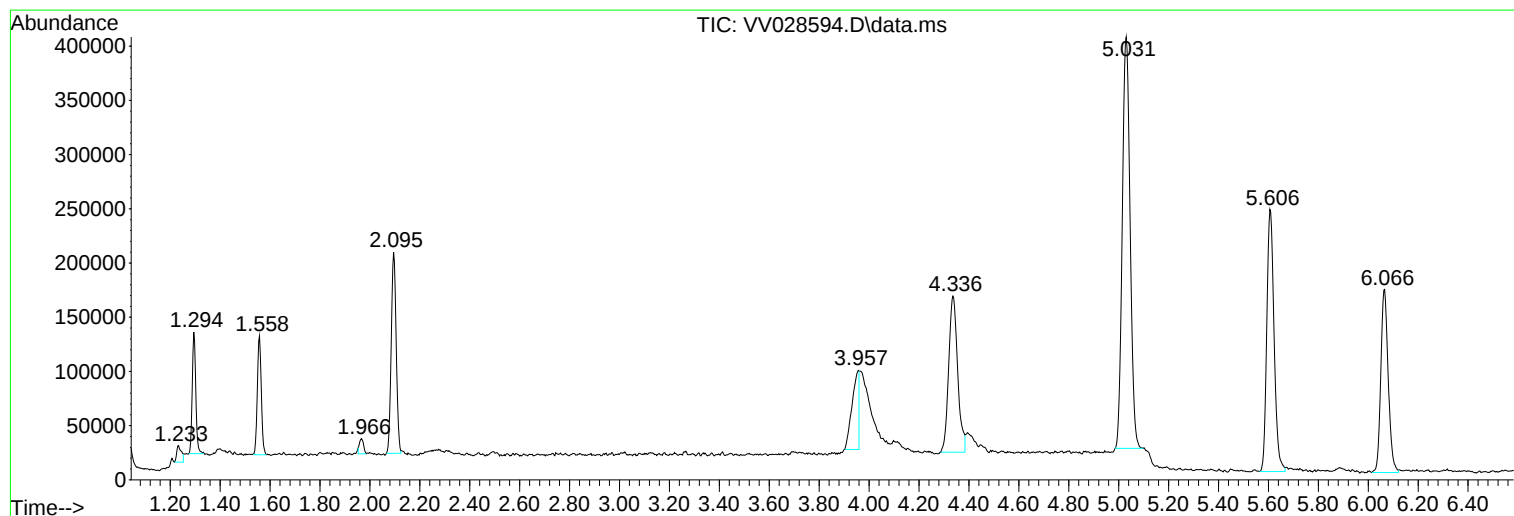

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028594.D
Acq On : 17 Oct 2022 17:20
Operator : SY/MD
Sample : N5060-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1BG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028594.D
Acq On : 17 Oct 2022 17:20
Operator : SY/MD
Sample : N5060-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1BG6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
