

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
 Data File : VV028597.D
 Acq On : 17 Oct 2022 18:56
 Operator : SY/MD
 Sample : N5103-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	53	63	69	rBV7	5646	12467	1.67%	0.212%
2	1.304	74	82	93	rVV	102716	110122	14.76%	1.875%
3	1.565	156	163	173	rVB	101139	112366	15.06%	1.913%
4	2.105	321	331	343	rVB	176311	251699	33.74%	4.286%
5	3.905	879	891	913	rBV2	48070	168495	22.59%	2.869%
6	4.343	1013	1027	1048	rBV	113318	284551	38.14%	4.845%
7	5.043	1230	1245	1269	rBV3	262103	663943	89.00%	11.305%
8	5.613	1410	1422	1444	rBV	226209	472407	63.33%	8.043%
9	6.066	1549	1563	1580	rBV	160616	333537	44.71%	5.679%
10	6.986	1835	1849	1866	rBV2	72260	145461	19.50%	2.477%
11	7.314	1938	1951	1973	rBV	292400	531788	71.29%	9.054%
12	7.622	2038	2047	2066	rBV	40193	80802	10.83%	1.376%
13	7.934	2132	2144	2157	rBV	24845	48191	6.46%	0.821%
14	8.088	2181	2192	2234	rBV	273399	745992	100.00%	12.702%
15	8.847	2411	2428	2452	rBV	343865	592804	79.47%	10.093%
16	10.210	2842	2852	2869	rBV	104794	175969	23.59%	2.996%
17	10.374	2892	2903	2915	rBV2	53582	92236	12.36%	1.570%
18	11.243	3161	3173	3192	rBV	344144	557886	74.78%	9.499%
19	11.616	3275	3289	3308	rBV	270212	453914	60.85%	7.729%
20	12.246	3476	3485	3497	rVB2	11201	19979	2.68%	0.340%
21	15.857	4596	4608	4609	rBV9	11970	18589	2.49%	0.317%




Sum of corrected areas: 5873198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028597.D
Acq On : 17 Oct 2022 18:56
Operator : SY/MD
Sample : N5103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

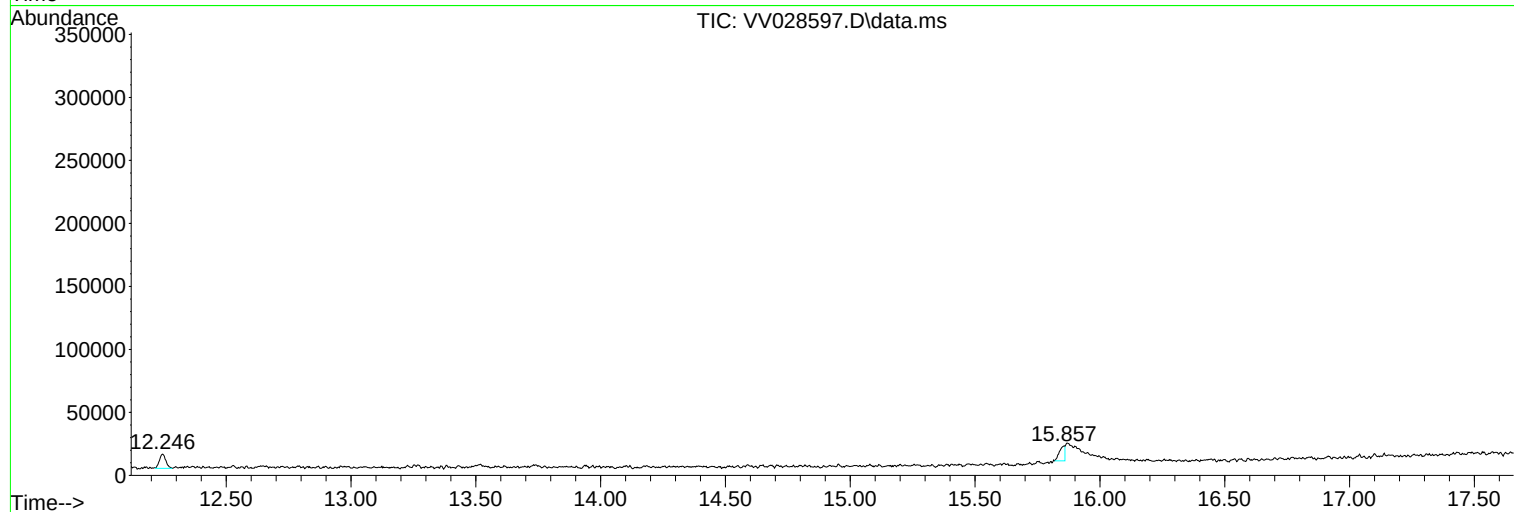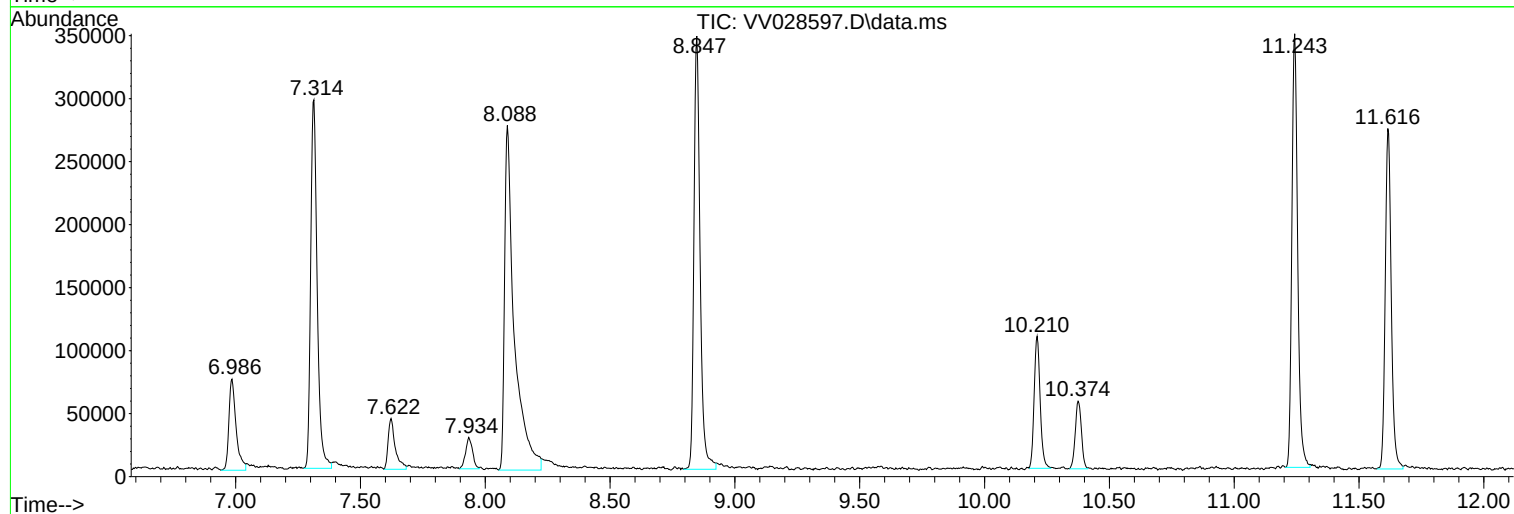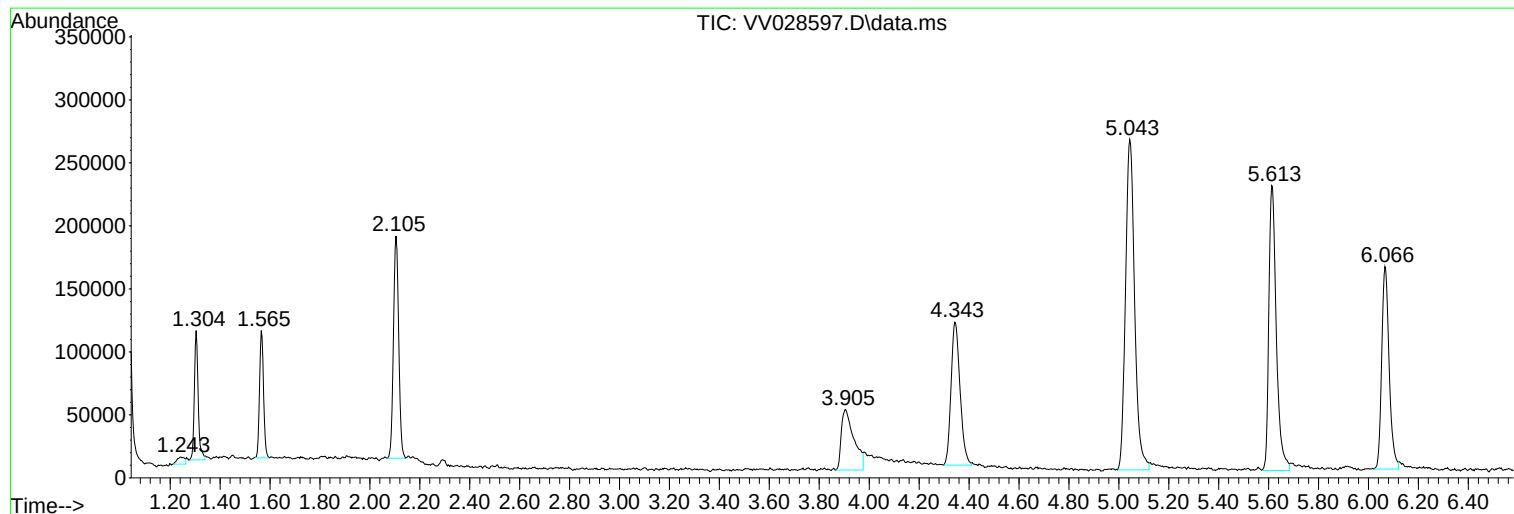

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028597.D
Acq On : 17 Oct 2022 18:56
Operator : SY/MD
Sample : N5103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV101722\
Data File : VV028597.D
Acq On : 17 Oct 2022 18:56
Operator : SY/MD
Sample : N5103-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR101422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc