

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037883.D
 Acq On : 17 Oct 2024 10:28
 Operator : SY/MD
 Sample : VV1017MBL01
 Misc : 5.00g/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 18 06:18:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 18 06:13:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	540804	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	538308	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	248404	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	207815	43.775	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.540%
7) Chloroethane-d5	1.536	69	183836	49.888	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.780%
11) 1,1-Dichloroethene-d2	2.060	65	95792	48.297	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.600%
21) 2-Butanone-d5	3.796	46	138819	82.096	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.100%
24) Chloroform-d	4.243	84	426095	50.448	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.900%
26) 1,2-Dichloroethane-d4	4.937	65	254270	51.432	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.860%
32) Benzene-d6	4.953	84	845167	50.174	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.340%
36) 1,2-Dichloropropane-d6	5.982	67	265621	49.520	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.040%
41) Toluene-d8	7.236	98	736064	48.190	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.380%
43) trans-1,3-Dichloroprop...	7.548	79	107718	43.230	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.460%
47) 2-Hexanone-d5	8.024	63	79765	70.425	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.420%
56) 1,1,2,2-Tetrachloroeth...	10.143	84	270549	43.410	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.820%
66) 1,2-Dichlorobenzene-d4	11.551	152	273454	52.242	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.480%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3098	0.804	ug/L	Qvalue # 29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037883.D
Acq On : 17 Oct 2024 10:28
Operator : SY/MD
Sample : VV1017MBL01
Misc : 5.00g/5mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 18 06:18:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 18 06:13:48 2024
Response via : Initial Calibration

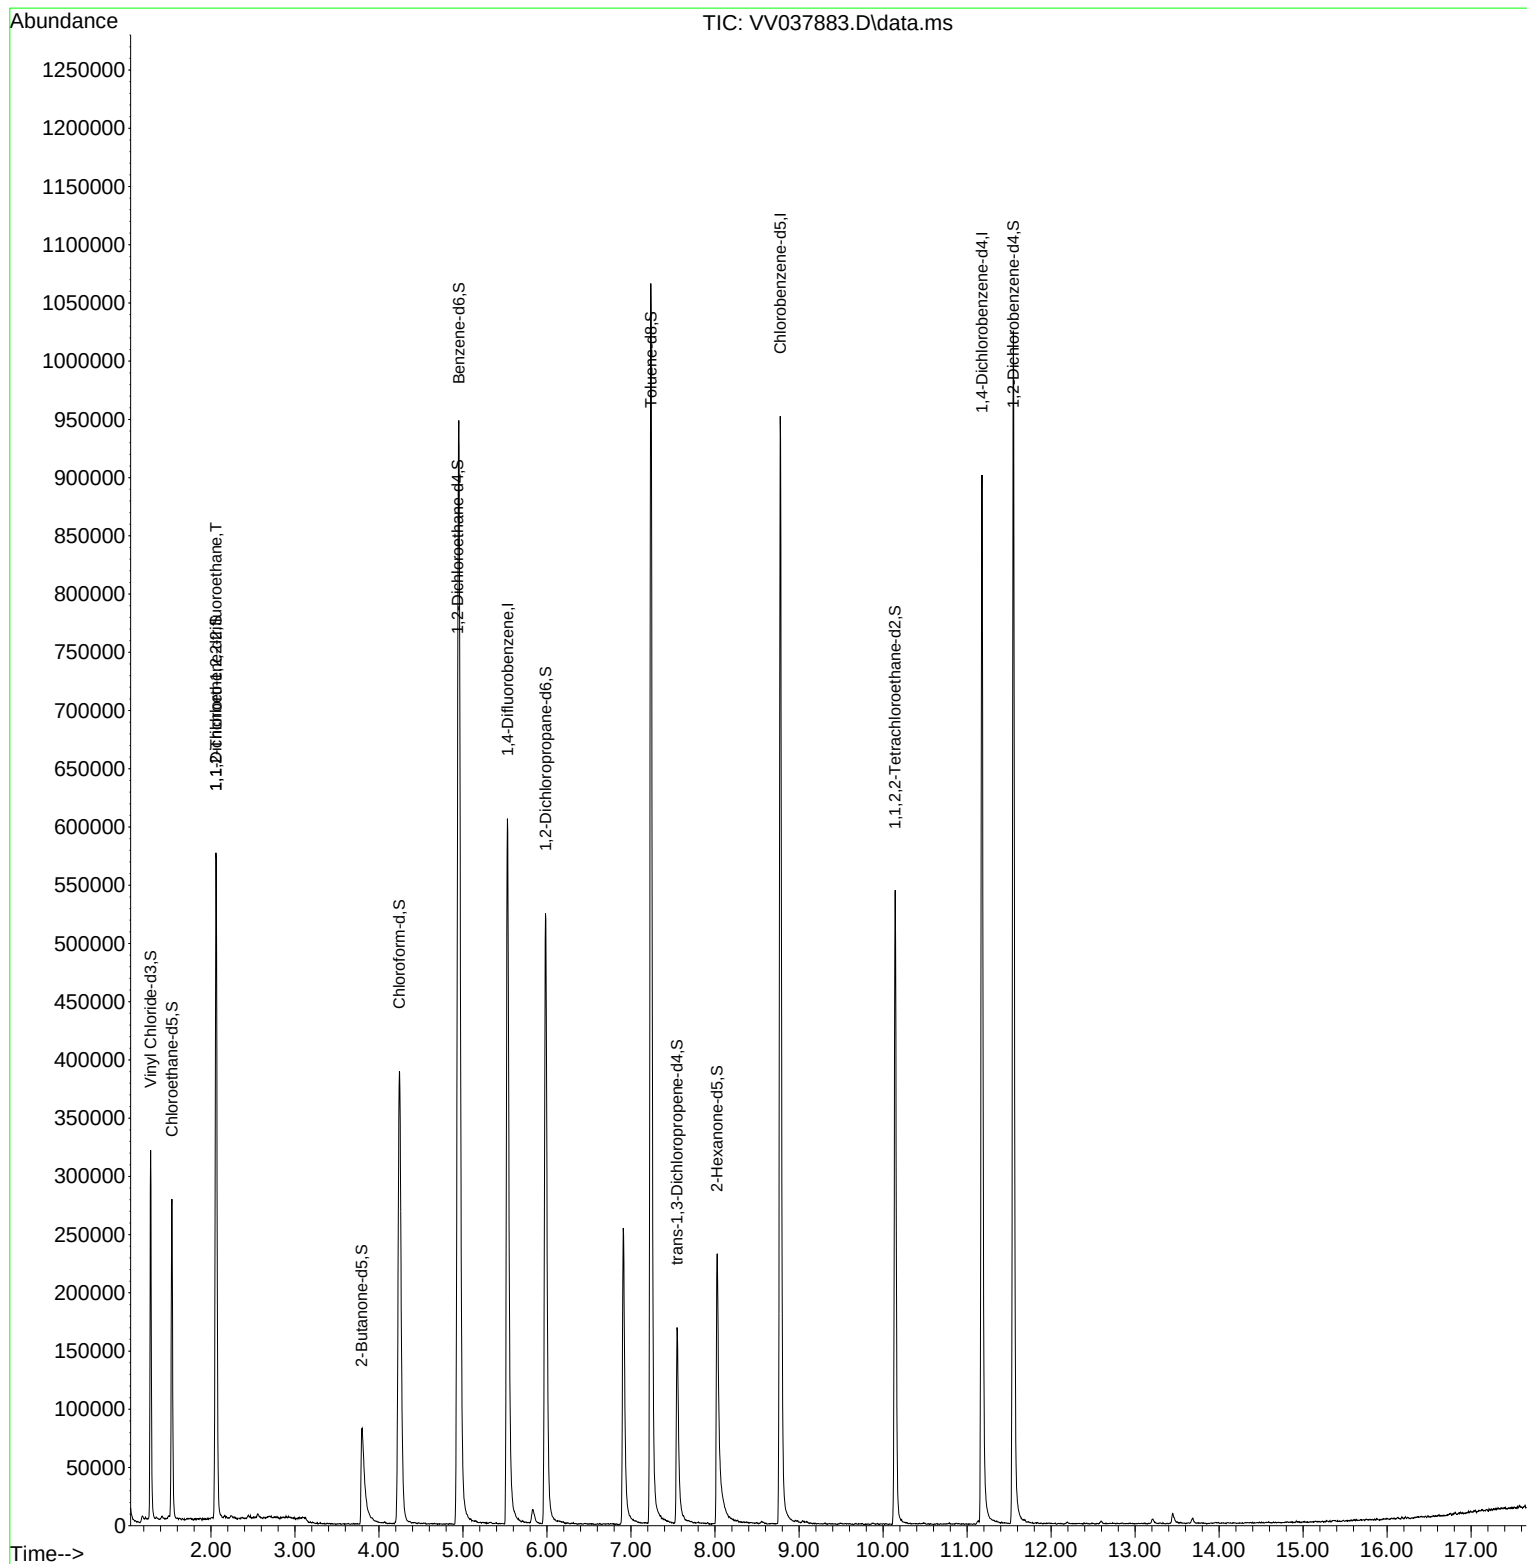

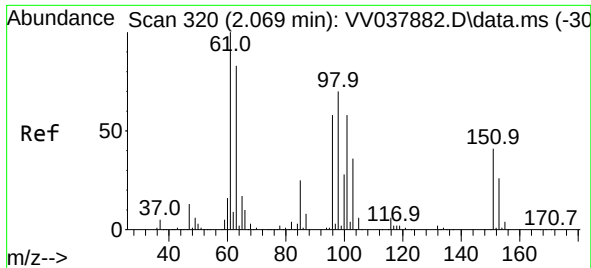

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.804 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV037883.D
 Acq: 17 Oct 2024 10:28

Instrument :
 MSVOA_V
 ClientSampleId :

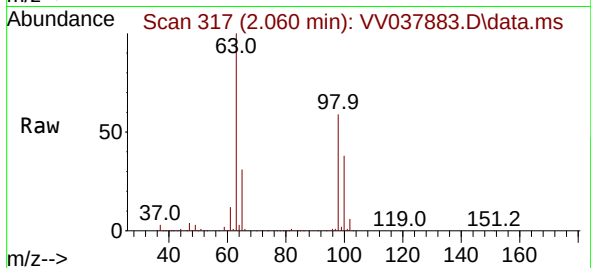

Tgt Ion:101 Resp: 3098
 Ion Ratio Lower Upper
 101 100
 85 3.9 34.6 52.0#
 151 8.1 57.5 86.3#

