

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037884.D
 Acq On : 17 Oct 2024 10:50
 Operator : SY/MD
 Sample : VV1017WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 18 06:18:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 18 06:13:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	530866	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	525195	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	242470	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	217656	46.706	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	93.420%	
7) Chloroethane-d5	1.535	69	188127	52.008	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	104.020%	
11) 1,1-Dichloroethene-d2	2.060	65	98964	50.830	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	101.660%	
21) 2-Butanone-d5	3.796	46	154516	93.090	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.090%	
24) Chloroform-d	4.243	84	440202	53.094	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.180%	
26) 1,2-Dichloroethane-d4	4.937	65	267717	55.166	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	110.340%	
32) Benzene-d6	4.953	84	879304	53.504	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	107.000%	
36) 1,2-Dichloropropane-d6	5.982	67	278388	53.197	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.400%	
41) Toluene-d8	7.236	98	758962	50.929	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.860%	
43) trans-1,3-Dichloroprop...	7.548	79	114922	47.273	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.540%	
47) 2-Hexanone-d5	8.024	63	91828	83.099	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	83.100%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	291411	47.925	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	95.840%	
66) 1,2-Dichlorobenzene-d4	11.551	152	282144	55.221	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	110.440%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.063	101	2954	0.781	ug/L	Qvalue # 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037884.D
Acq On : 17 Oct 2024 10:50
Operator : SY/MD
Sample : VV1017WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 18 06:18:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 18 06:13:48 2024
Response via : Initial Calibration

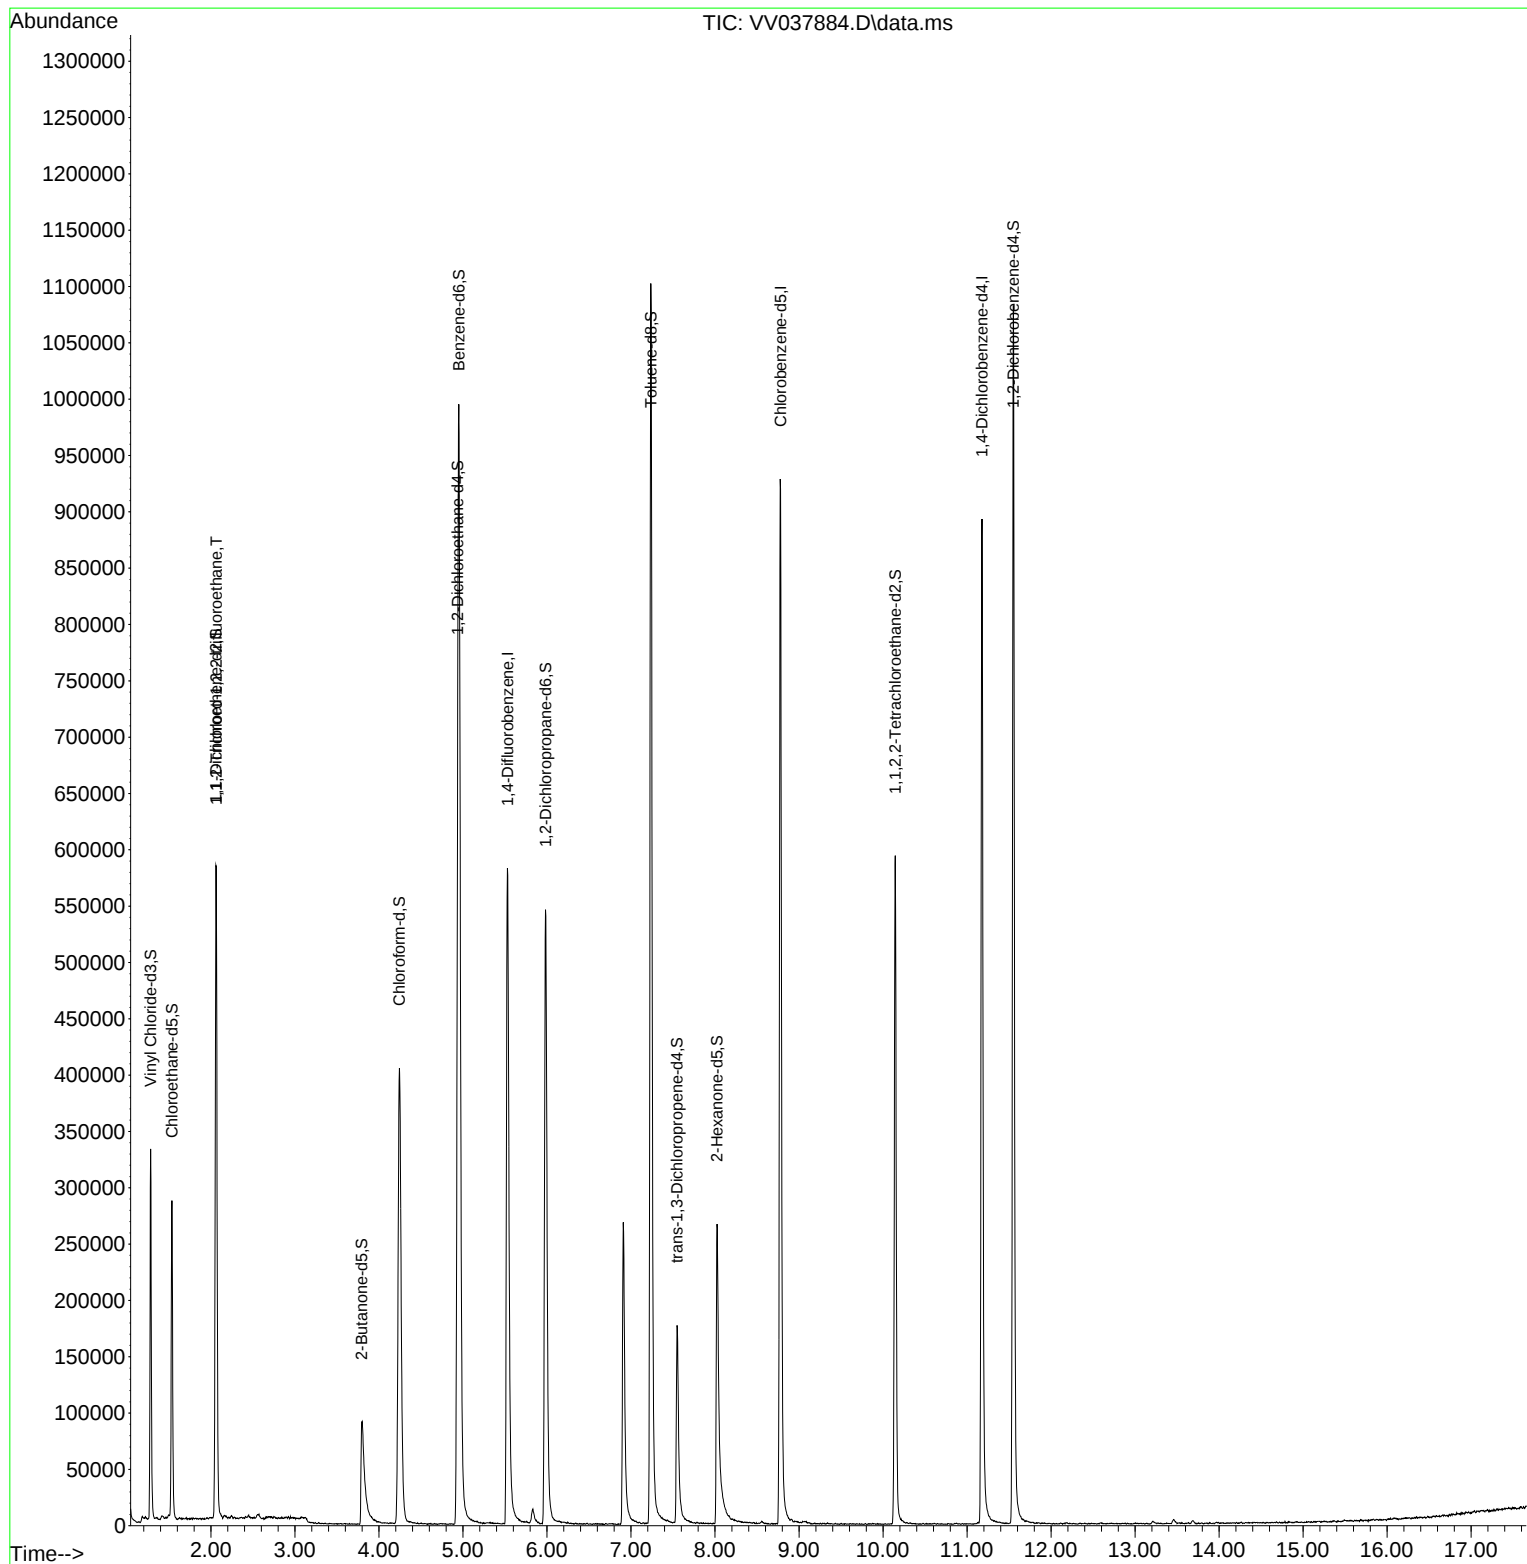

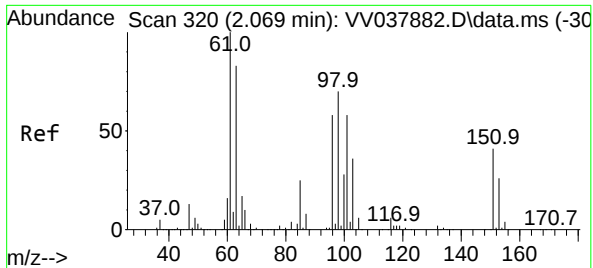

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.781 ug/L
 RT: 2.063 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV037884.D
 Acq: 17 Oct 2024 10:50

Instrument :
 MSVOA_V
 ClientSampleId :

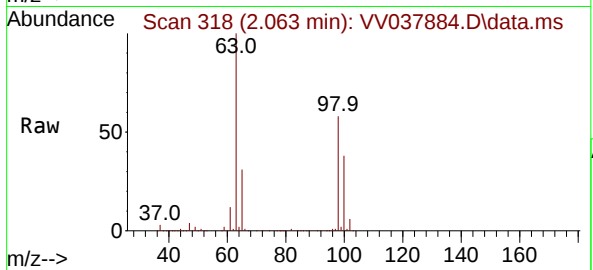

Tgt Ion:101 Resp: 2954
 Ion Ratio Lower Upper
 101 100
 85 5.7 34.6 52.0#
 151 0.0 57.5 86.3#

