

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037887.D
 Acq On : 17 Oct 2024 13:37
 Operator : SY/MD
 Sample : P4414-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 18 06:16:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 18 06:13:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	585845	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	580535	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	264308	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	205596	39.978	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.960%
7) Chloroethane-d5	1.532	69	177550	44.478	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.960%
11) 1,1-Dichloroethene-d2	2.056	65	93856	43.682	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.360%
21) 2-Butanone-d5	3.793	46	117706	64.258	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	64.260%
24) Chloroform-d	4.236	84	406077	44.382	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.760%
26) 1,2-Dichloroethane-d4	4.931	65	242705	45.319	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.640%
32) Benzene-d6	4.947	84	798365	43.948	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.900%
36) 1,2-Dichloropropane-d6	5.979	67	248648	42.984	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	85.960%
41) Toluene-d8	7.233	98	679916	41.276	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.560%
43) trans-1,3-Dichloroprop...	7.548	79	100114	37.256	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.520%
47) 2-Hexanone-d5	8.024	63	69316	56.748	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	56.750%
56) 1,1,2,2-Tetrachloroeth...	10.143	84	251913	37.480	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	74.960%
66) 1,2-Dichlorobenzene-d4	11.551	152	260042	46.690	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.380%
Target Compounds						
39) cis-1,3-Dichloropropene	6.908	75	6636	0.919	ug/L	Qvalue # 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037887.D
Acq On : 17 Oct 2024 13:37
Operator : SY/MD
Sample : P4414-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 18 06:16:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 18 06:13:48 2024
Response via : Initial Calibration

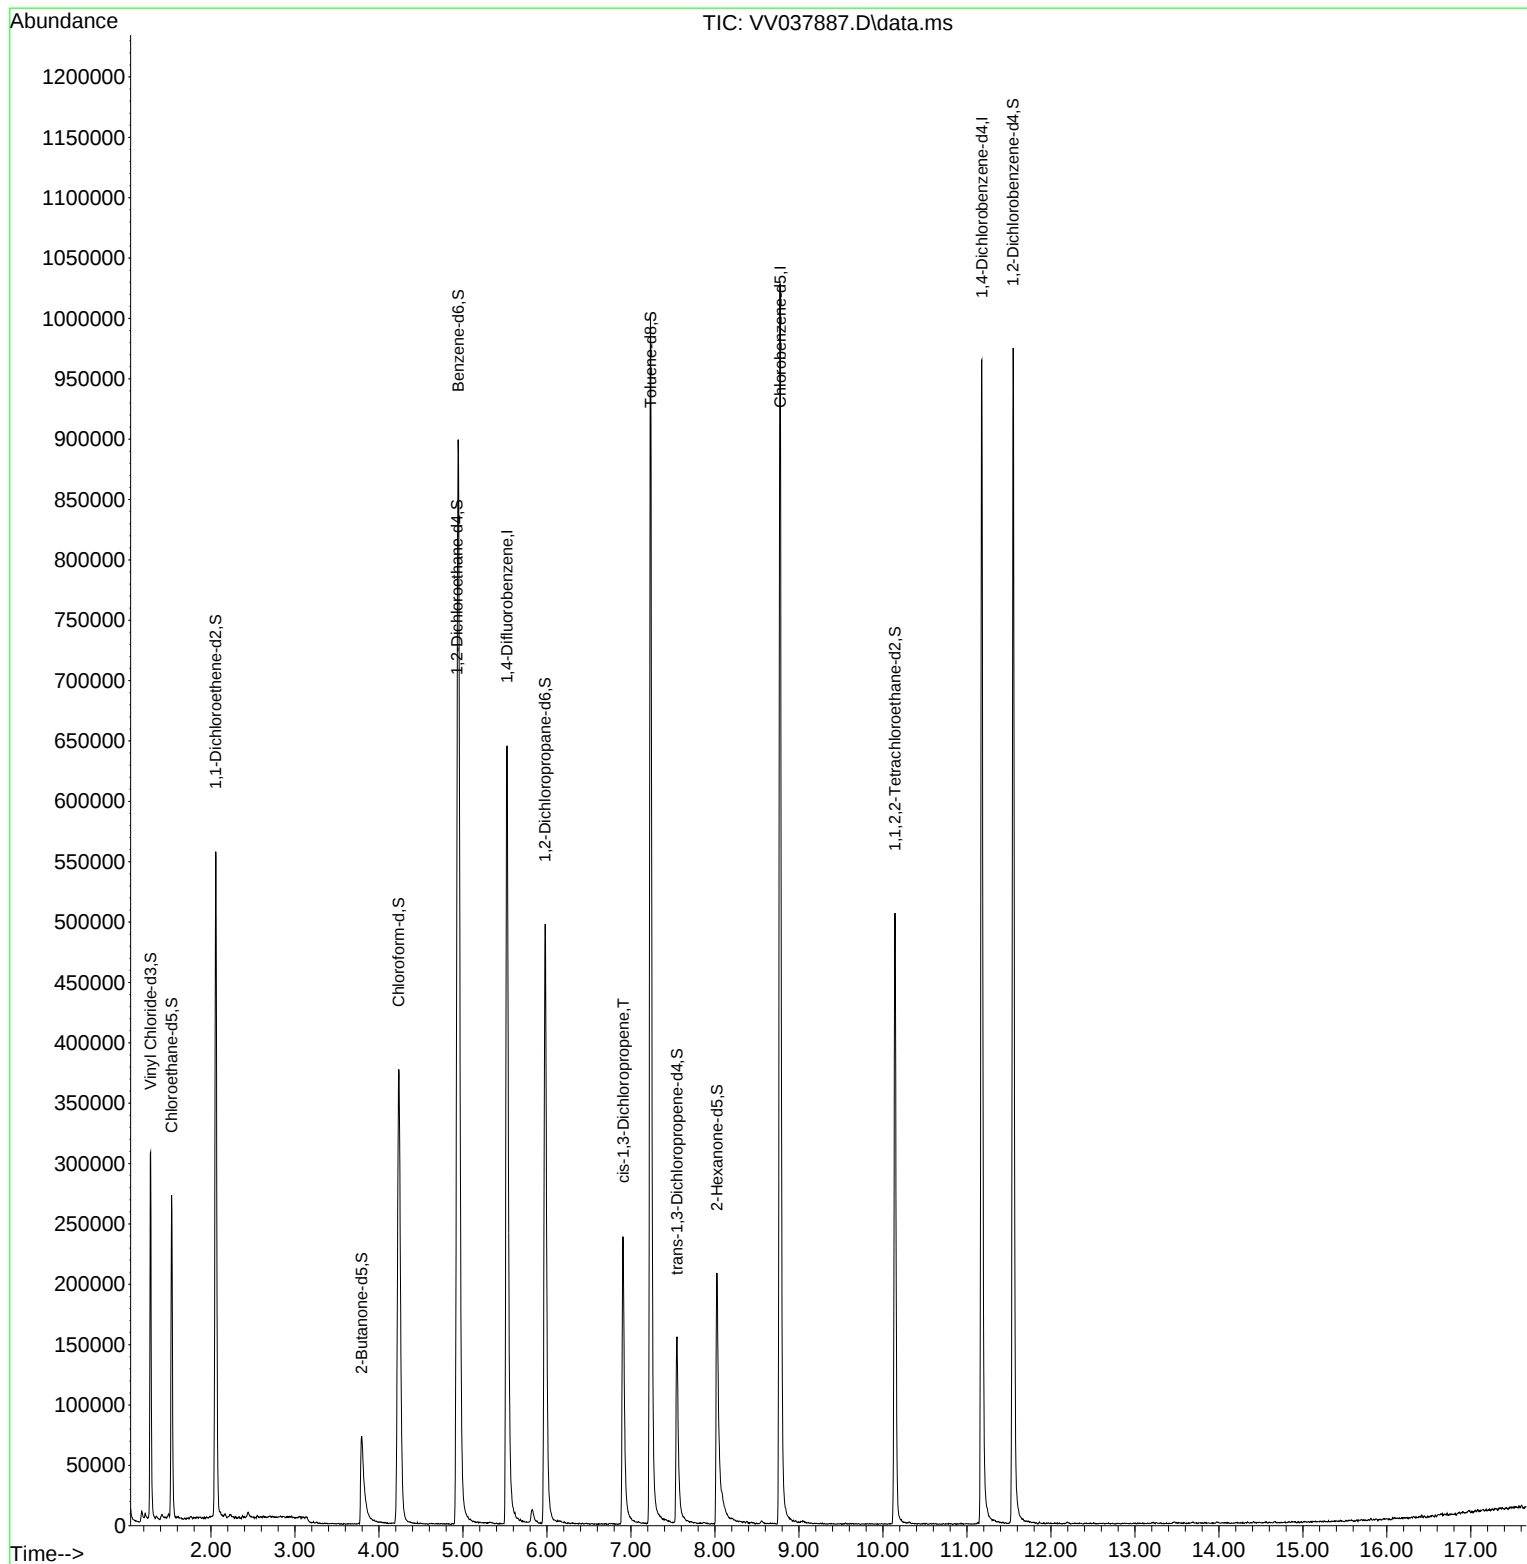

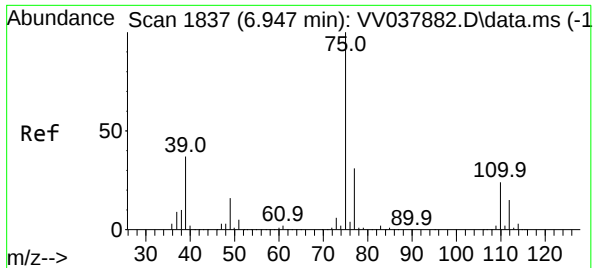

#39
cis-1,3-Dichloropropene
Concen: 0.919 ug/L
RT: 6.908 min Scan# 11
Delta R.T. -0.039 min
Lab File: VV037887.D
Acq: 17 Oct 2024 13:37

Instrument :
MSVOA_V
ClientSampleId :

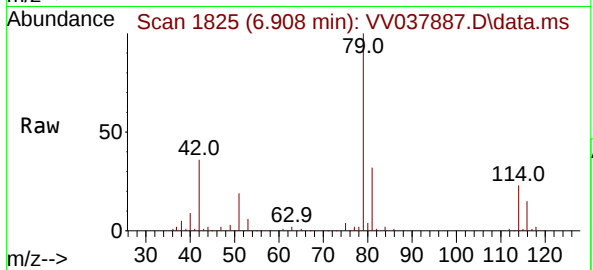

Tgt Ion: 75 Resp: 6636
Ion Ratio Lower Upper
75 100
77 53.3 21.8 40.4#

