

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037885.D
 Acq On : 17 Oct 2024 11:40
 Operator : SY/MD
 Sample : P4414-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037885.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	38	44	52	rBV2	7273	13356	0.58%	0.080%
2	1.281	69	75	93	rVB	284585	307145	13.38%	1.850%
3	1.535	147	154	168	rVB	259206	307829	13.41%	1.854%
4	2.060	308	317	329	rBV	527831	759086	33.07%	4.571%
5	3.442	745	747	749	rBV	612	322	0.01%	0.002%
6	3.580	787	790	793	rBV2	305	194	0.01%	0.001%
7	3.645	808	810	814	rBV2	420	284	0.01%	0.002%
8	3.683	818	822	824	rBV3	463	433	0.02%	0.003%
9	3.760	842	846	848	rBV2	570	455	0.02%	0.003%
10	3.793	848	856	890	rBV	82366	247492	10.78%	1.490%
11	4.240	979	995	1025	rBV	382442	978195	42.62%	5.890%
12	4.494	1072	1074	1077	rBV2	549	317	0.01%	0.002%
13	4.654	1119	1124	1125	rBV	519	429	0.02%	0.003%
14	4.696	1134	1137	1141	rBV3	723	595	0.03%	0.004%
15	4.731	1146	1148	1152	rVV3	463	286	0.01%	0.002%
16	4.815	1170	1174	1181	rBV2	969	768	0.03%	0.005%
17	4.841	1181	1182	1183	rBV2	537	196	0.01%	0.001%
18	4.947	1197	1215	1251	rBV2	896234	2295333	100.00%	13.822%
19	5.358	1341	1343	1345	rBV3	559	287	0.01%	0.002%
20	5.436	1363	1367	1370	rVB4	788	565	0.02%	0.003%
21	5.484	1380	1382	1384	rBV2	437	245	0.01%	0.001%
22	5.526	1384	1395	1433	rBV	682521	1428359	62.23%	8.601%
23	5.979	1523	1536	1564	rBV	515765	1077043	46.92%	6.486%
24	6.336	1644	1647	1649	rBV3	700	398	0.02%	0.002%
25	6.358	1649	1654	1655	rBV2	837	576	0.03%	0.003%
26	6.468	1686	1688	1690	rBV2	416	179	0.01%	0.001%
27	6.519	1702	1704	1707	rBV	420	271	0.01%	0.002%
28	6.558	1713	1716	1717	rBV2	370	207	0.01%	0.001%
29	6.587	1723	1725	1728	rVB4	1040	528	0.02%	0.003%
30	6.619	1732	1735	1738	rBV2	348	259	0.01%	0.002%
31	6.641	1738	1742	1743	rBV3	555	375	0.02%	0.002%
32	6.738	1770	1772	1773	rBV3	367	158	0.01%	0.001%
33	6.809	1791	1794	1797	rBV4	635	471	0.02%	0.003%
34	6.905	1813	1824	1851	rBV	244887	478734	20.86%	2.883%
35	7.233	1916	1926	1972	rBV	987257	1780085	77.55%	10.719%
36	7.548	2015	2024	2054	rBV	164047	315542	13.75%	1.900%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037885.D
 Acq On : 17 Oct 2024 11:40
 Operator : SY/MD
 Sample : P4414-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.908	2133	2136	2140	rBV5	1119	706	0.03%	0.004%
38	7.940	2143	2146	2149	rBV4	759	367	0.02%	0.002%
39	7.966	2149	2154	2156	rBV3	851	691	0.03%	0.004%
40	8.024	2162	2172	2207	rBV2	234976	557604	24.29%	3.358%
41	8.715	2384	2387	2390	rBV3	798	483	0.02%	0.003%
42	8.738	2393	2394	2395	rBV	504	169	0.01%	0.001%
43	8.776	2395	2406	2439	rBV	1099641	1803686	78.58%	10.861%
44	9.210	2538	2541	2542	rBV2	387	225	0.01%	0.001%
45	9.226	2542	2546	2547	rBV2	631	396	0.02%	0.002%
46	9.271	2558	2560	2561	rBV	458	225	0.01%	0.001%
47	9.304	2567	2570	2571	rBV2	691	443	0.02%	0.003%
48	9.333	2578	2579	2584	rVB2	422	202	0.01%	0.001%
49	9.358	2584	2587	2590	rVB4	443	218	0.01%	0.001%
50	9.397	2596	2599	2601	rBV2	828	473	0.02%	0.003%
51	9.410	2601	2603	2605	rVB2	473	217	0.01%	0.001%
52	9.432	2606	2610	2612	rBV2	637	473	0.02%	0.003%
53	9.471	2621	2622	2624	rBV	427	175	0.01%	0.001%
54	9.538	2642	2643	2648	rBV2	361	201	0.01%	0.001%
55	9.564	2649	2651	2655	rVB3	418	218	0.01%	0.001%
56	9.583	2655	2657	2661	rVB4	814	474	0.02%	0.003%
57	9.603	2661	2663	2666	rBV2	934	644	0.03%	0.004%
58	9.644	2673	2676	2680	rBV3	764	626	0.03%	0.004%
59	9.673	2683	2685	2688	rBV	387	236	0.01%	0.001%
60	9.722	2696	2700	2704	rBV3	815	806	0.04%	0.005%
61	9.837	2733	2736	2740	rVB4	698	499	0.02%	0.003%
62	10.008	2786	2789	2790	rBV	429	222	0.01%	0.001%
63	10.069	2805	2808	2811	rVB3	450	321	0.01%	0.002%
64	10.082	2811	2812	2814	rBV2	369	193	0.01%	0.001%
65	10.098	2814	2817	2818	rBV2	396	219	0.01%	0.001%
66	10.143	2818	2831	2851	rBV	554863	879682	38.32%	5.297%
67	10.361	2896	2899	2901	rBV2	427	352	0.02%	0.002%
68	10.452	2925	2927	2933	rVB3	685	543	0.02%	0.003%
69	10.480	2933	2936	2937	rBV2	392	199	0.01%	0.001%
70	10.542	2951	2955	2957	rBV3	912	562	0.02%	0.003%
71	10.558	2957	2960	2961	rBV2	667	378	0.02%	0.002%
72	10.625	2978	2981	2987	rBV6	1649	1728	0.08%	0.010%
73	10.683	2996	2999	3003	rVB	687	436	0.02%	0.003%
74	10.767	3023	3025	3026	rBV	460	219	0.01%	0.001%
75	10.802	3035	3036	3039	rVB	477	216	0.01%	0.001%
76	10.828	3042	3044	3045	rBV	366	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037885.D
 Acq On : 17 Oct 2024 11:40
 Operator : SY/MD
 Sample : P4414-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.889	3061	3063	3065	rBV	269	166	0.01%	0.001%
78	10.976	3088	3090	3091	rBV	502	196	0.01%	0.001%
79	11.075	3117	3121	3122	rBV2	339	234	0.01%	0.001%
80	11.085	3122	3124	3127	rBV2	325	190	0.01%	0.001%
81	11.120	3127	3135	3142	rBV10	4831	8049	0.35%	0.048%
82	11.175	3142	3152	3185	rVV	1027733	1642099	71.54%	9.888%
83	11.458	3238	3240	3242	rBV3	1007	656	0.03%	0.004%
84	11.551	3258	3269	3297	rBV	1048616	1682526	73.30%	10.132%
85	11.931	3385	3387	3388	rBV2	1012	484	0.02%	0.003%
86	12.069	3427	3430	3432	rBV3	916	639	0.03%	0.004%
87	12.255	3482	3488	3492	rBV6	3392	4333	0.19%	0.026%
88	12.342	3513	3515	3516	rBV	720	226	0.01%	0.001%
89	12.461	3549	3552	3554	rBV3	626	392	0.02%	0.002%
90	12.648	3607	3610	3612	rBV2	650	349	0.02%	0.002%
91	12.802	3656	3658	3661	rBV2	661	371	0.02%	0.002%
92	12.818	3661	3663	3665	rBV2	644	279	0.01%	0.002%
93	12.853	3672	3674	3678	rBV4	599	476	0.02%	0.003%
94	12.892	3684	3686	3688	rBV2	1245	619	0.03%	0.004%
95	13.075	3739	3743	3746	rBV5	1182	1205	0.05%	0.007%
96	13.210	3778	3785	3793	rBV9	2410	4177	0.18%	0.025%
97	13.268	3801	3803	3808	rVB3	1062	614	0.03%	0.004%
98	13.416	3845	3849	3852	rBV4	775	671	0.03%	0.004%
99	13.686	3923	3933	3939	rBV7	2403	4288	0.19%	0.026%
100	14.892	4306	4308	4310	rBV2	857	502	0.02%	0.003%




Sum of corrected areas: 16606625

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037885.D
Acq On : 17 Oct 2024 11:40
Operator : SY/MD
Sample : P4414-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

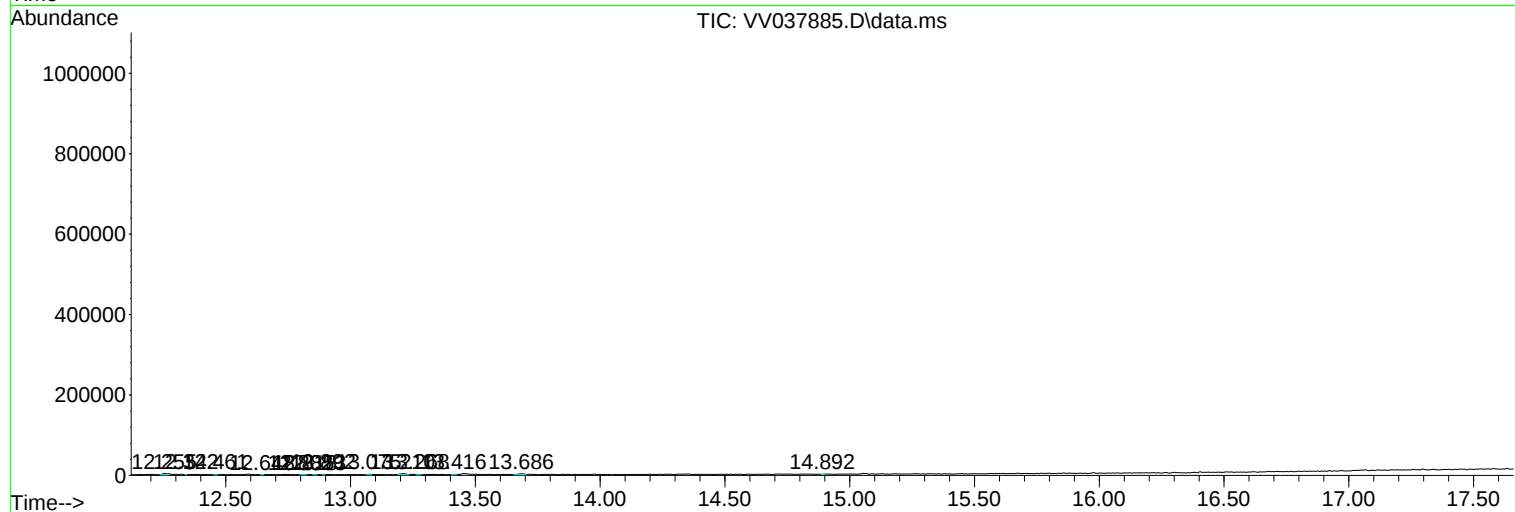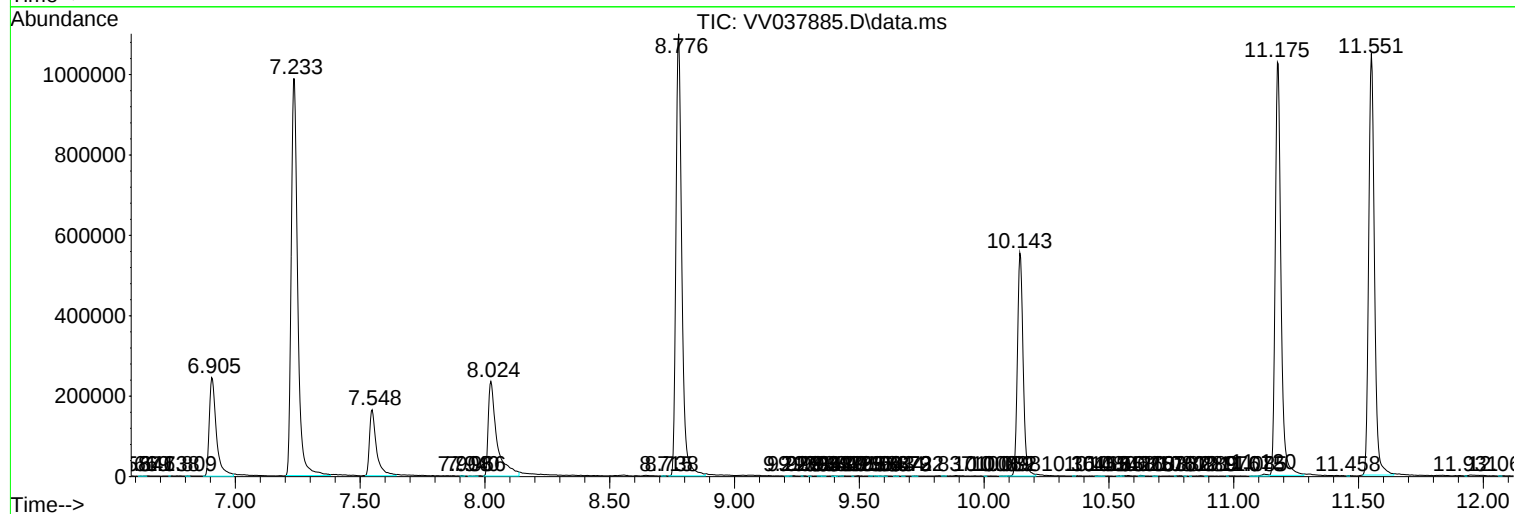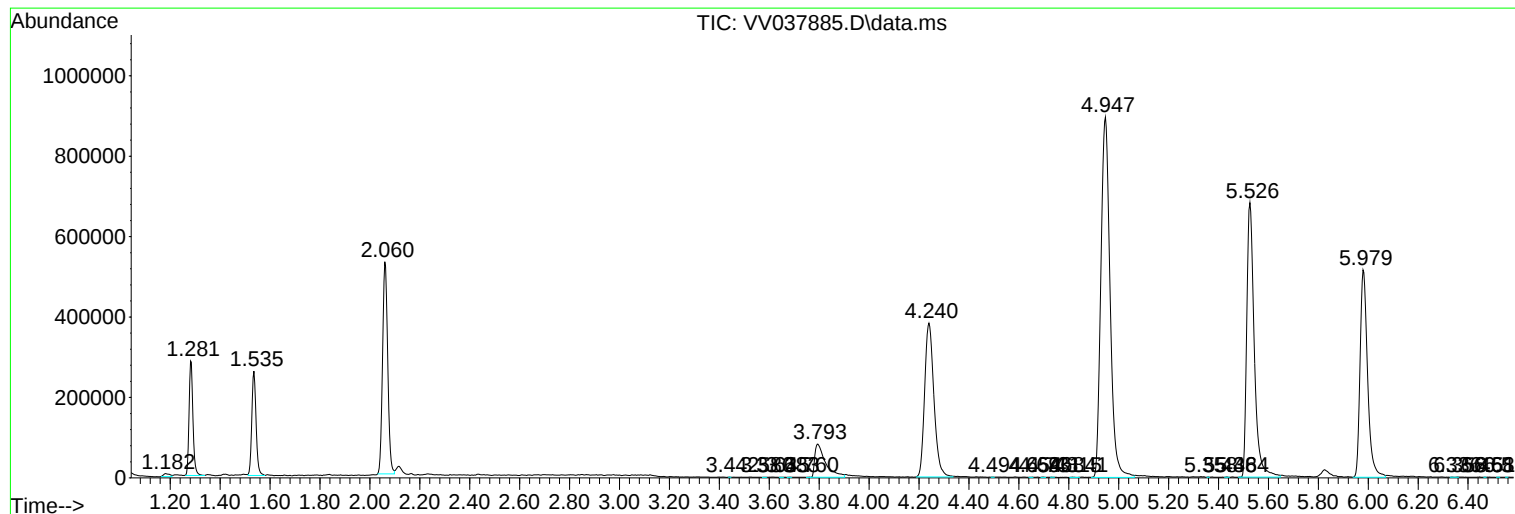

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037885.D
Acq On : 17 Oct 2024 11:40
Operator : SY/MD
Sample : P4414-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037885.D
Acq On : 17 Oct 2024 11:40
Operator : SY/MD
Sample : P4414-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------