

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037886.D
 Acq On : 17 Oct 2024 12:40
 Operator : SY/MD
 Sample : P4429-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	52	rBV	7331	11810	0.52%	0.072%
2	1.278	68	74	89	rVB	277891	298802	13.25%	1.817%
3	1.532	146	153	167	rVB	266730	306174	13.57%	1.862%
4	2.056	307	316	328	rBV	517648	749817	33.24%	4.560%
5	3.494	759	763	764	rBV2	718	481	0.02%	0.003%
6	3.526	771	773	775	rBV	522	283	0.01%	0.002%
7	3.590	791	793	796	rBV	535	240	0.01%	0.001%
8	3.632	804	806	807	rBV	347	143	0.01%	0.001%
9	3.706	827	829	833	rVB2	644	364	0.02%	0.002%
10	3.793	847	856	887	rBV	82451	241472	10.70%	1.469%
11	4.236	979	994	1020	rBV	376752	960140	42.56%	5.840%
12	4.478	1067	1069	1071	rBV2	753	353	0.02%	0.002%
13	4.561	1093	1095	1100	rVB2	1143	615	0.03%	0.004%
14	4.600	1104	1107	1109	rBV3	442	268	0.01%	0.002%
15	4.632	1115	1117	1120	rVB2	580	264	0.01%	0.002%
16	4.719	1139	1144	1148	rVB4	687	744	0.03%	0.005%
17	4.754	1150	1155	1159	rBV2	721	685	0.03%	0.004%
18	4.780	1159	1163	1166	rVB2	803	703	0.03%	0.004%
19	4.805	1166	1171	1177	rBV5	805	1042	0.05%	0.006%
20	4.838	1177	1181	1185	rBV4	542	438	0.02%	0.003%
21	4.873	1190	1192	1193	rVB	668	206	0.01%	0.001%
22	4.944	1199	1214	1250	rBV2	882861	2255719	100.00%	13.719%
23	5.413	1358	1360	1363	rBV3	383	223	0.01%	0.001%
24	5.461	1372	1375	1379	rBV3	518	444	0.02%	0.003%
25	5.522	1383	1394	1424	rBV	694696	1450616	64.31%	8.823%
26	5.979	1523	1536	1567	rBV	506841	1060443	47.01%	6.450%
27	6.358	1649	1654	1657	rBV6	852	916	0.04%	0.006%
28	6.413	1669	1671	1674	rBV2	705	407	0.02%	0.002%
29	6.468	1685	1688	1689	rBV3	560	277	0.01%	0.002%
30	6.477	1689	1691	1694	rVB2	629	324	0.01%	0.002%
31	6.497	1694	1697	1699	rBV4	700	449	0.02%	0.003%
32	6.548	1711	1713	1716	rBV3	403	150	0.01%	0.001%
33	6.600	1724	1729	1733	rVB3	684	596	0.03%	0.004%
34	6.629	1733	1738	1739	rBV3	641	530	0.02%	0.003%
35	6.638	1739	1741	1746	rVB2	642	491	0.02%	0.003%
36	6.664	1746	1749	1753	rBV4	846	780	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037886.D
 Acq On : 17 Oct 2024 12:40
 Operator : SY/MD
 Sample : P4429-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.683	1753	1755	1756	rBV	449	228	0.01%	0.001%
38	6.799	1789	1791	1794	rVB2	598	395	0.02%	0.002%
39	6.818	1794	1797	1799	rBV2	695	434	0.02%	0.003%
40	6.828	1799	1800	1805	rVB3	589	395	0.02%	0.002%
41	6.854	1805	1808	1811	rBV2	638	324	0.01%	0.002%
42	6.866	1811	1812	1814	rBV2	190	92	0.00%	0.001%
43	6.905	1814	1824	1853	rBV	239844	473660	21.00%	2.881%
44	7.191	1911	1913	1914	rBV2	742	329	0.01%	0.002%
45	7.233	1916	1926	1959	rVV	963640	1727215	76.57%	10.505%
46	7.548	2015	2024	2056	rBV	158286	305362	13.54%	1.857%
47	7.911	2133	2137	2139	rBV4	1226	852	0.04%	0.005%
48	7.973	2154	2156	2160	rBV2	842	526	0.02%	0.003%
49	8.024	2163	2172	2220	rVV2	226130	550993	24.43%	3.351%
50	8.548	2331	2335	2338	rBV5	1702	1773	0.08%	0.011%
51	8.719	2386	2388	2392	rVB4	674	347	0.02%	0.002%
52	8.776	2392	2406	2441	rBV	1092526	1844193	81.76%	11.216%
53	9.146	2519	2521	2526	rBV4	1053	923	0.04%	0.006%
54	9.310	2569	2572	2575	rBV2	757	576	0.03%	0.004%
55	9.397	2598	2599	2603	rVB2	245	133	0.01%	0.001%
56	9.419	2603	2606	2607	rBV2	399	131	0.01%	0.001%
57	9.432	2607	2610	2612	rBV2	501	410	0.02%	0.002%
58	9.468	2619	2621	2622	rBV2	325	124	0.01%	0.001%
59	9.519	2634	2637	2638	rBV2	483	287	0.01%	0.002%
60	9.567	2649	2652	2653	rVB2	340	136	0.01%	0.001%
61	9.612	2663	2666	2671	rVB3	683	587	0.03%	0.004%
62	9.648	2675	2677	2679	rBV	340	107	0.00%	0.001%
63	9.706	2689	2695	2696	rBV2	878	746	0.03%	0.005%
64	9.796	2721	2723	2725	rBV	559	349	0.02%	0.002%
65	9.850	2737	2740	2742	rBV2	601	333	0.01%	0.002%
66	9.870	2742	2746	2747	rBV3	931	634	0.03%	0.004%
67	10.024	2791	2794	2796	rBV3	578	358	0.02%	0.002%
68	10.053	2801	2803	2806	rVV3	739	360	0.02%	0.002%
69	10.085	2811	2813	2815	rVB3	576	230	0.01%	0.001%
70	10.146	2820	2832	2854	rBV	528235	855758	37.94%	5.205%
71	10.445	2920	2925	2929	rBV3	1123	985	0.04%	0.006%
72	10.474	2932	2934	2937	rBV3	991	703	0.03%	0.004%
73	10.529	2947	2951	2953	rVB2	393	283	0.01%	0.002%
74	10.558	2953	2960	2961	rBV4	1415	1195	0.05%	0.007%
75	10.673	2993	2996	3001	rVB3	555	462	0.02%	0.003%
76	10.712	3003	3008	3010	rBV2	837	757	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
 Data File : VV037886.D
 Acq On : 17 Oct 2024 12:40
 Operator : SY/MD
 Sample : P4429-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.821	3039	3042	3045	rBV3	733	620	0.03%	0.004%
78	10.876	3057	3059	3062	rBV2	504	254	0.01%	0.002%
79	10.976	3088	3090	3094	rBV3	557	398	0.02%	0.002%
80	11.043	3109	3111	3116	rVB3	706	502	0.02%	0.003%
81	11.098	3124	3128	3129	rBV2	695	471	0.02%	0.003%
82	11.124	3129	3136	3142	rVV8	4414	6203	0.27%	0.038%
83	11.178	3142	3153	3186	rVV	1027967	1669559	74.01%	10.154%
84	11.551	3258	3269	3299	rBV	1017078	1635663	72.51%	9.948%
85	12.098	3438	3439	3441	rBV	487	240	0.01%	0.001%
86	12.474	3553	3556	3558	rBV3	1003	526	0.02%	0.003%
87	12.564	3581	3584	3586	rBV3	887	581	0.03%	0.004%
88	12.779	3649	3651	3653	rBV3	537	244	0.01%	0.001%
89	13.037	3728	3731	3734	rBV4	829	659	0.03%	0.004%
90	13.313	3813	3817	3819	rBV3	1165	865	0.04%	0.005%
91	13.458	3855	3862	3865	rBV5	2582	3414	0.15%	0.021%
92	13.538	3885	3887	3892	rBV4	657	510	0.02%	0.003%




Sum of corrected areas: 16441803

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037886.D
Acq On : 17 Oct 2024 12:40
Operator : SY/MD
Sample : P4429-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

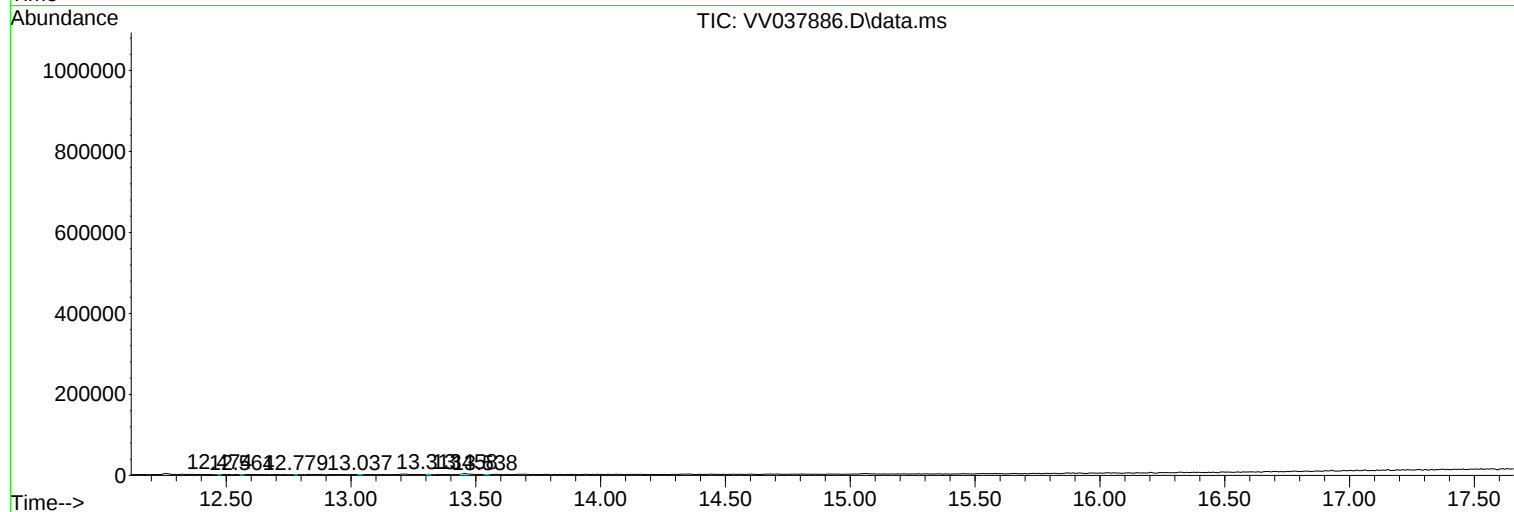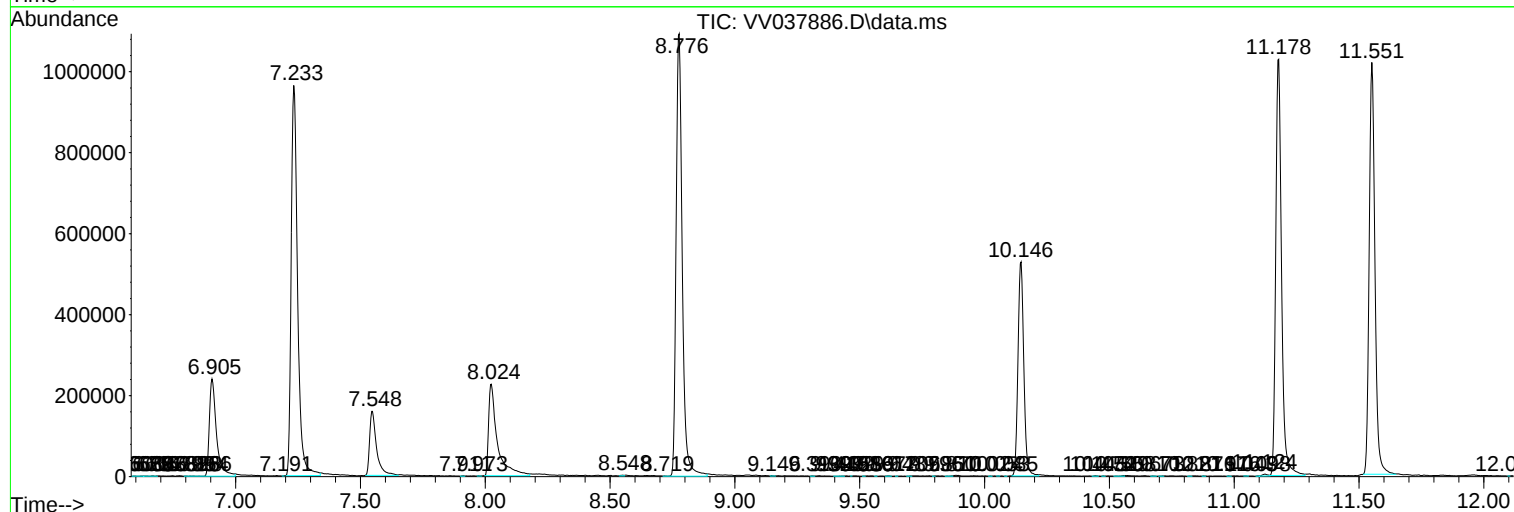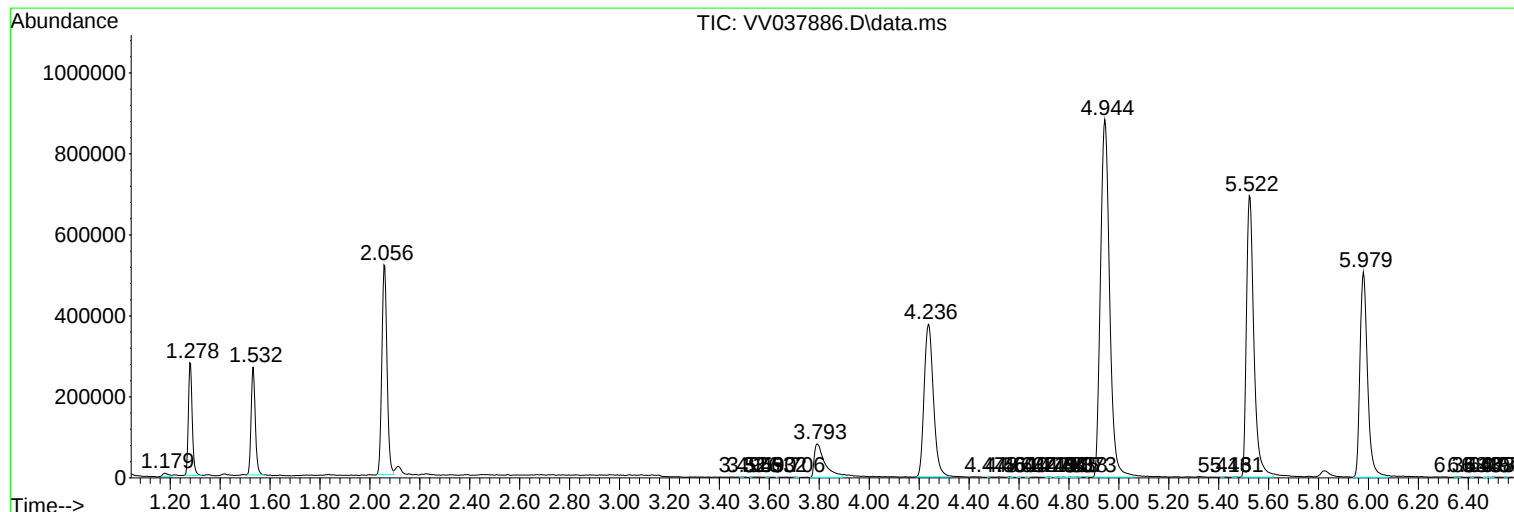

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037886.D
Acq On : 17 Oct 2024 12:40
Operator : SY/MD
Sample : P4429-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101724\
Data File : VV037886.D
Acq On : 17 Oct 2024 12:40
Operator : SY/MD
Sample : P4429-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------